




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026925.D
 Acq On : 23 Jul 2022 16:26
 Operator : SY/MD
 Sample : N3741-11ME
 Misc : 4.89g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B36ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

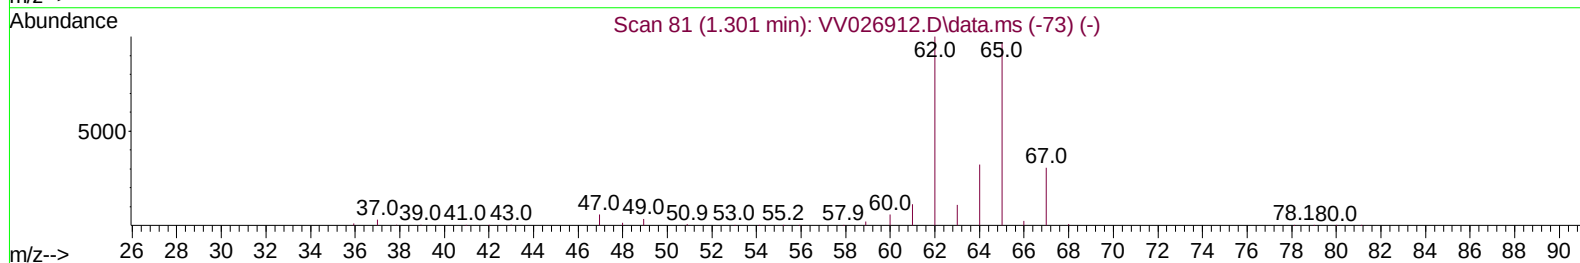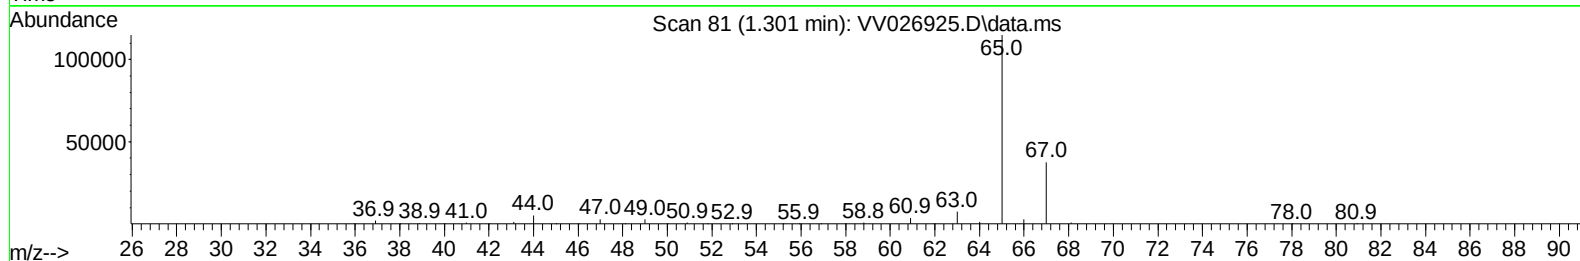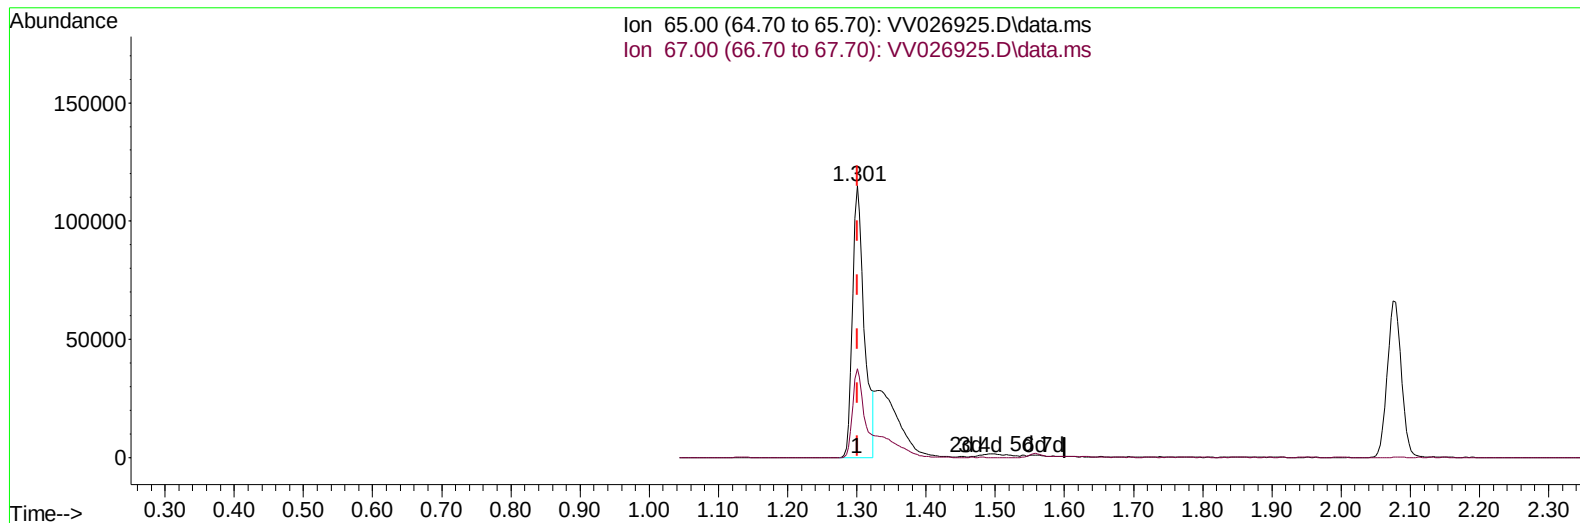

TIC: VV026925.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.301min (-0.000) 22.07 ug/L

response 136055

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.50	48.83#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026925.D
 Acq On : 23 Jul 2022 16:26
 Operator : SY/MD
 Sample : N3741-11ME
 Misc : 4.89g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B36ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

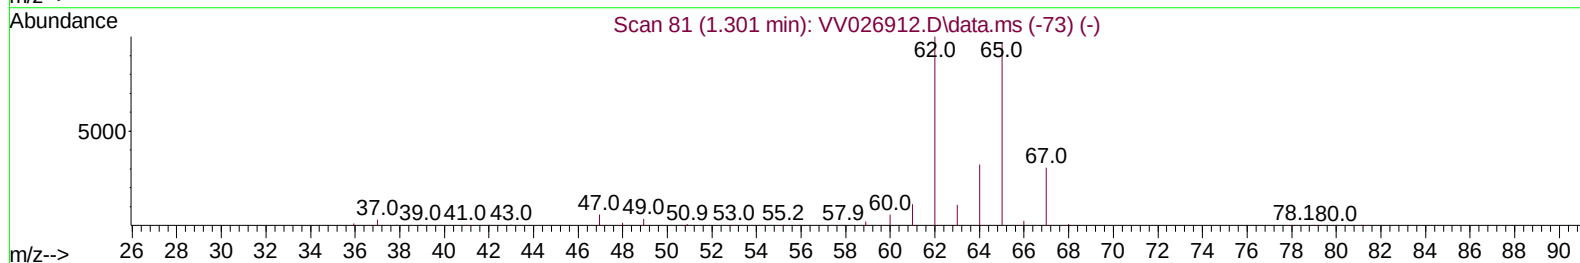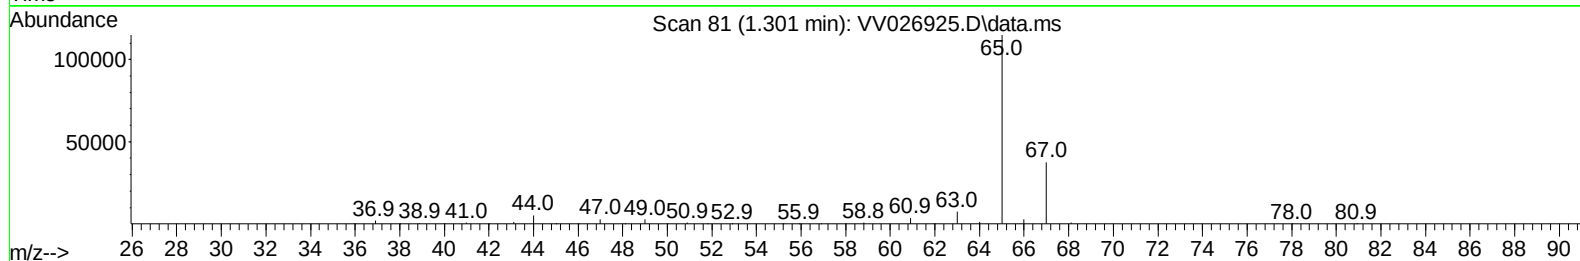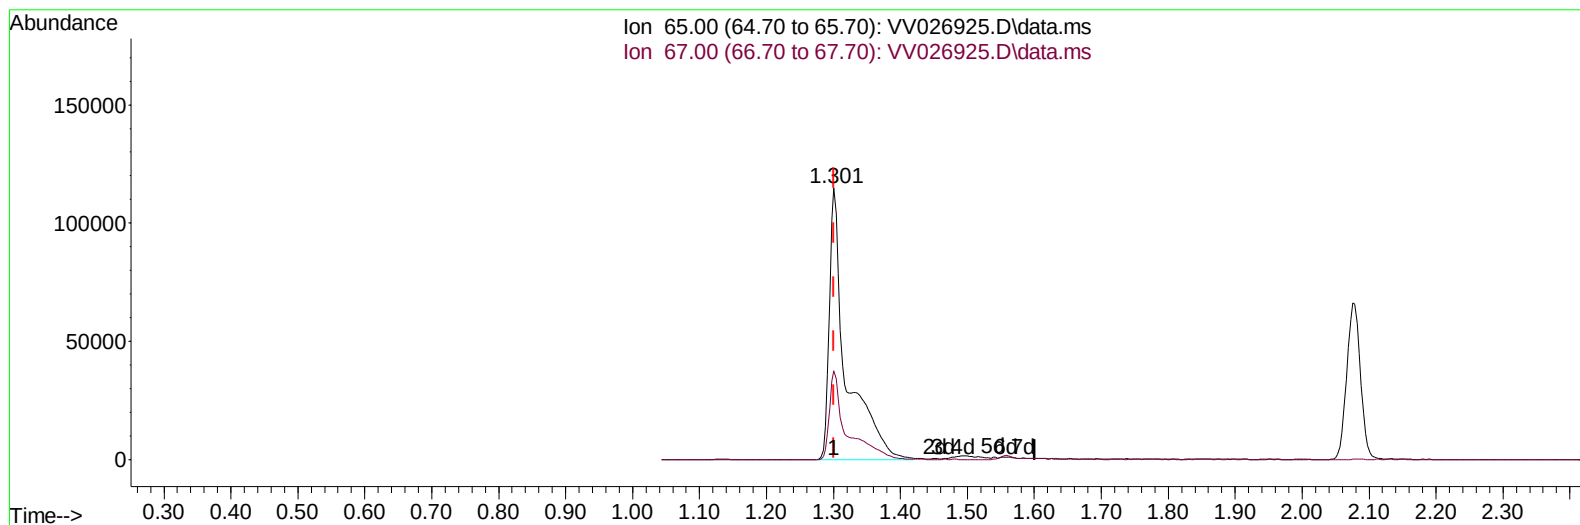

TIC: VV026925.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.301min (-0.000) 33.20 ug/L m

response 204635

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.50	32.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026925.D
Acq On : 23 Jul 2022 16:26
Operator : SY/MD
Sample : N3741-11ME
Misc : 4.89g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B36ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

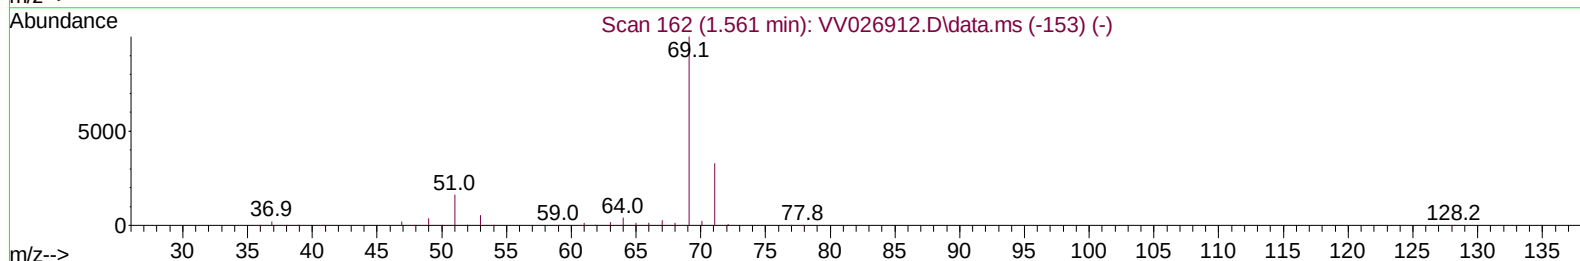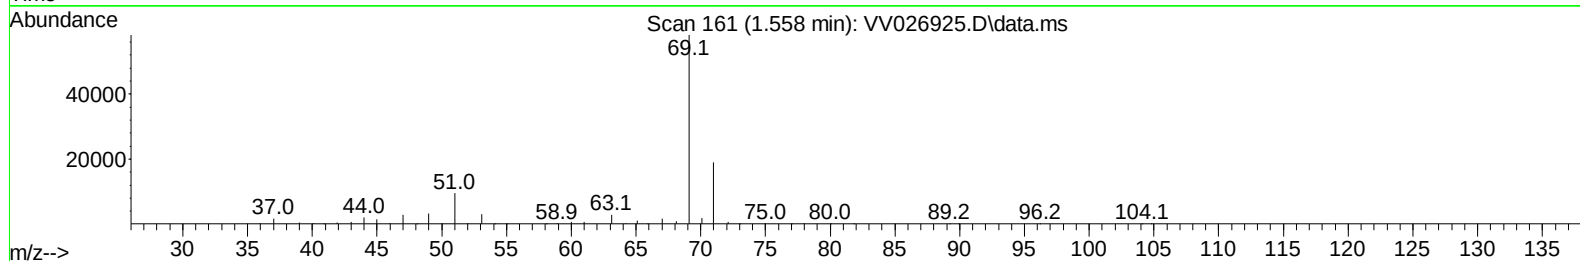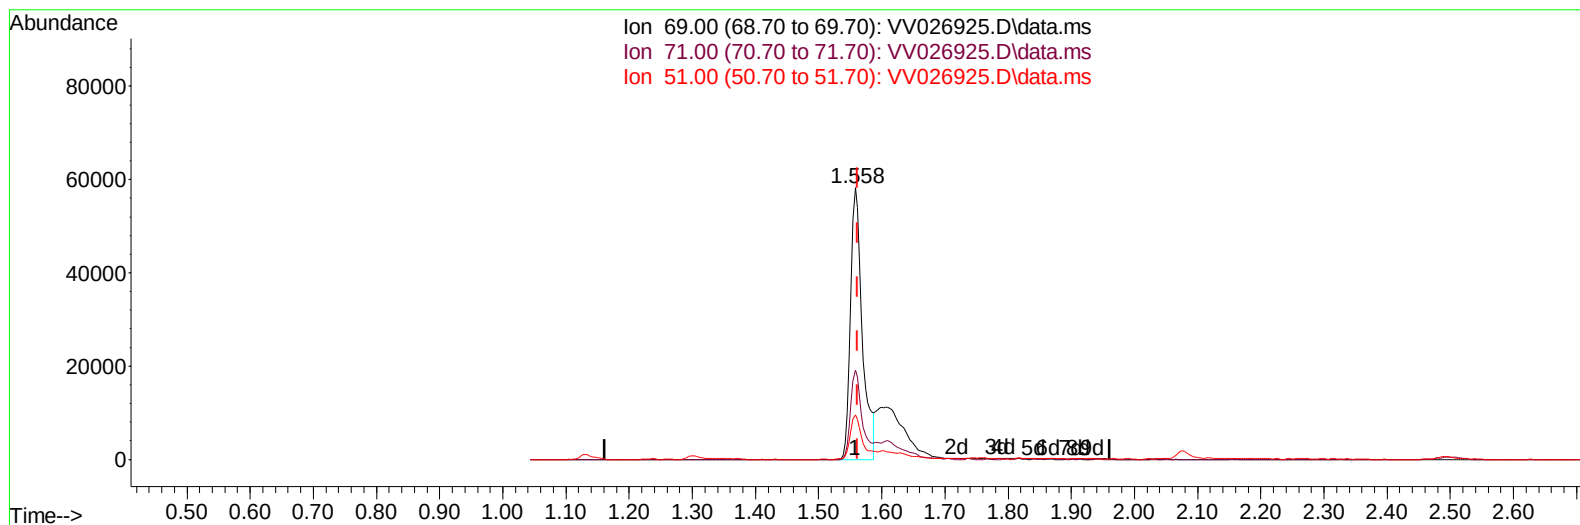

TIC: VV026925.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.003) 15.13 ug/L

response 75439

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	31.91
51.00	23.00	17.55
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026925.D
 Acq On : 23 Jul 2022 16:26
 Operator : SY/MD
 Sample : N3741-11ME
 Misc : 4.89g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B36ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

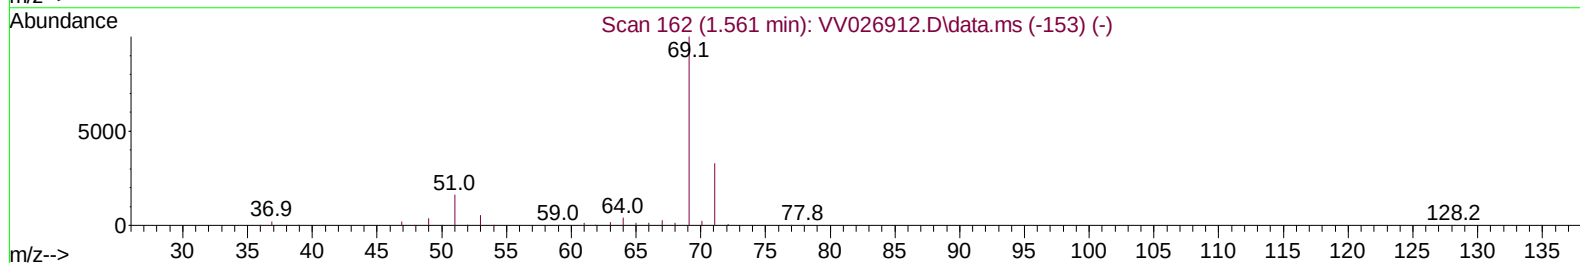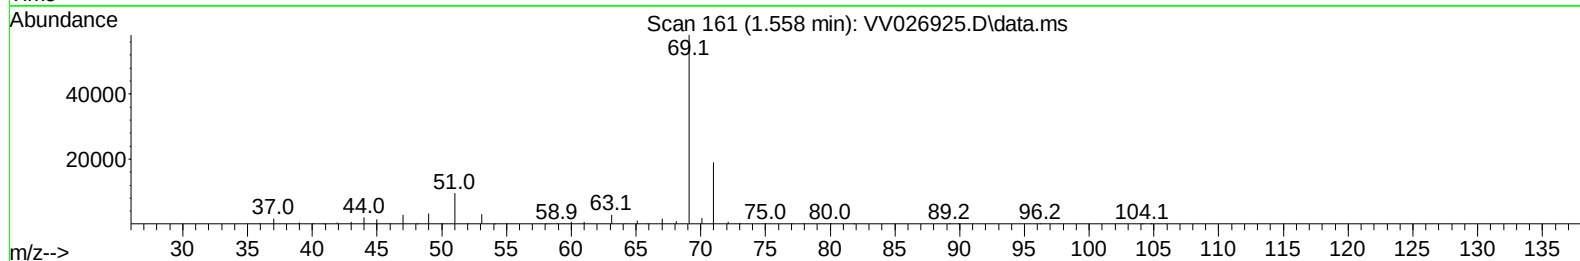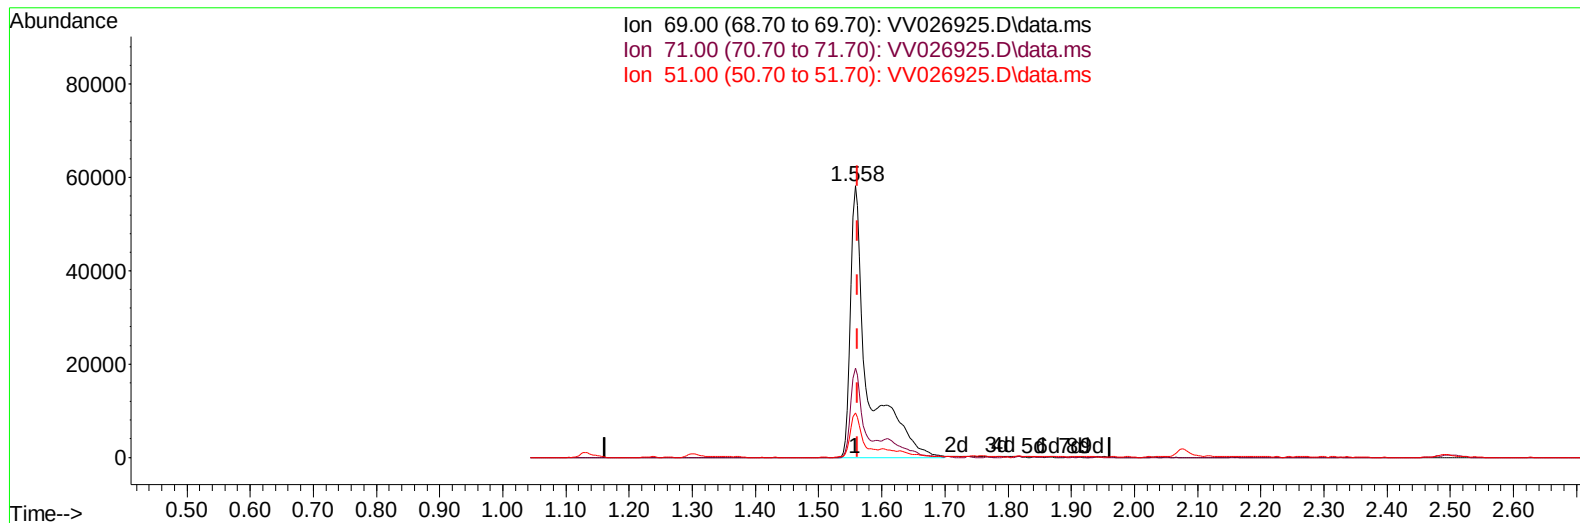

TIC: VV026925.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.003) 22.28 ug/L m

response 111120

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	21.67#
51.00	23.00	11.91#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026925.D
 Acq On : 23 Jul 2022 16:26
 Operator : SY/MD
 Sample : N3741-11ME
 Misc : 4.89g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B36ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	734895	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	730399	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	328341	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	204635m	33.200	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	66.400%	
7) Chloroethane-d5	1.558	69	111120m	22.285	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	44.560%#	
11) 1,1-Dichloroethene-d2	2.076	63	296549	26.743	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	53.480%#	
21) 2-Butanone-d5	3.899	46	373652	89.938	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	89.940%	
24) Chloroform-d	4.339	84	490984	40.475	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	80.960%	
26) 1,2-Dichloroethane-d4	5.024	65	306835	44.220	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.440%	
32) Benzene-d6	5.037	84	999642	45.277	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	90.560%	
36) 1,2-Dichloropropane-d6	6.063	67	327275	45.998	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	92.000%	
41) Toluene-d8	7.310	98	829565	42.943	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	85.880%	
43) trans-1,3-Dichloroprop...	7.619	79	122821	41.197	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	82.400%	
47) 2-Hexanone-d5	8.095	63	285157	92.045	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	92.050%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	463356	42.869	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	85.740%	
66) 1,2-Dichlorobenzene-d4	11.625	152	317556	51.552	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	103.100%	
Target Compounds						
15) Methyl Acetate	2.432	43	45274	7.036	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026925.D
Acq On : 23 Jul 2022 16:26
Operator : SY/MD
Sample : N3741-11ME
Misc : 4.89g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B36ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

