




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026928.D
 Acq On : 23 Jul 2022 17:40
 Operator : SY/MD
 Sample : N3766-06ME
 Misc : 6.15g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ZD1ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:10:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

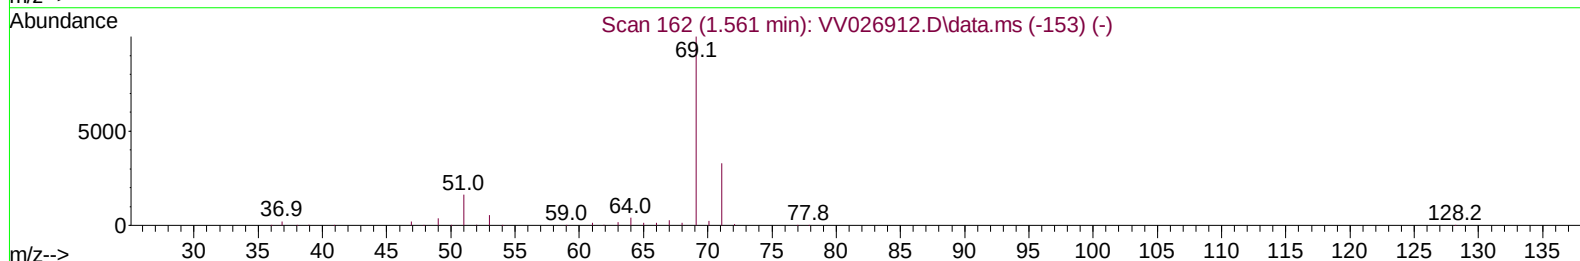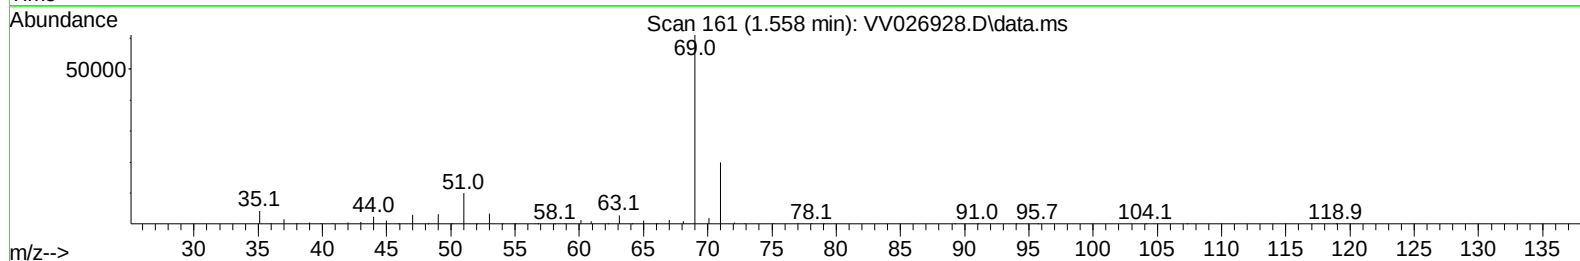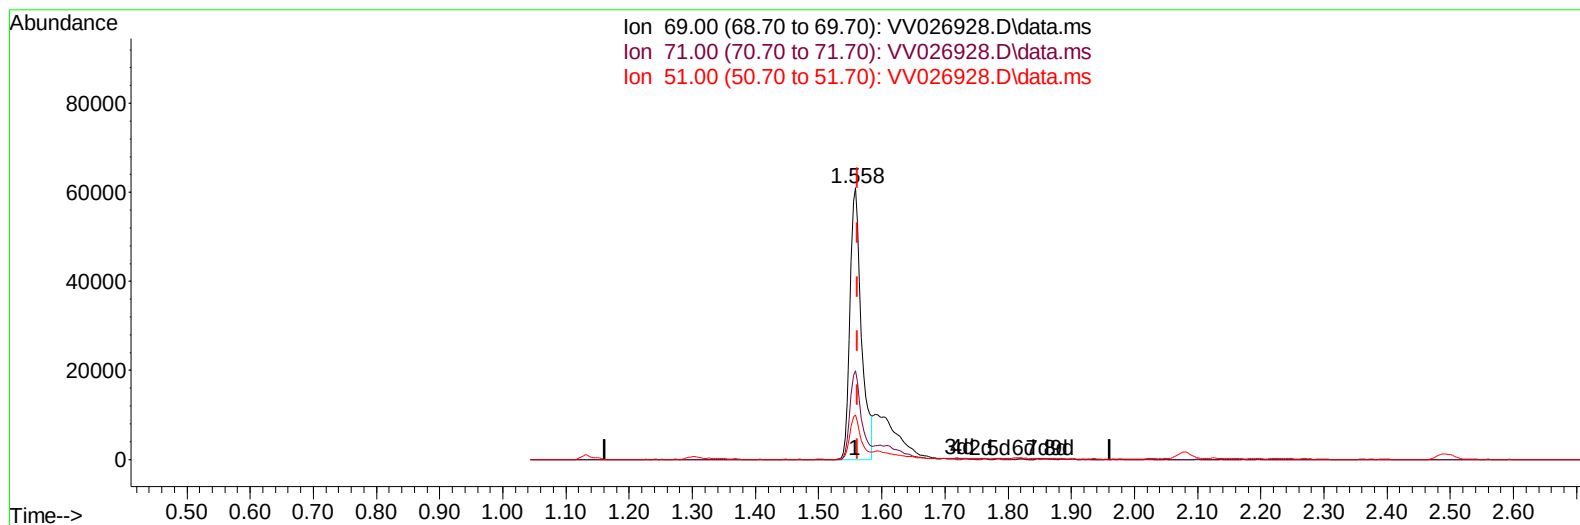

TIC: VV026928.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.003) 16.73 ug/L

response 76202

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	32.99
51.00	23.00	16.47
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026928.D
Acq On : 23 Jul 2022 17:40
Operator : SY/MD
Sample : N3766-06ME
Misc : 6.15g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ZD1ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

Quant Time: Jul 25 02:10:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

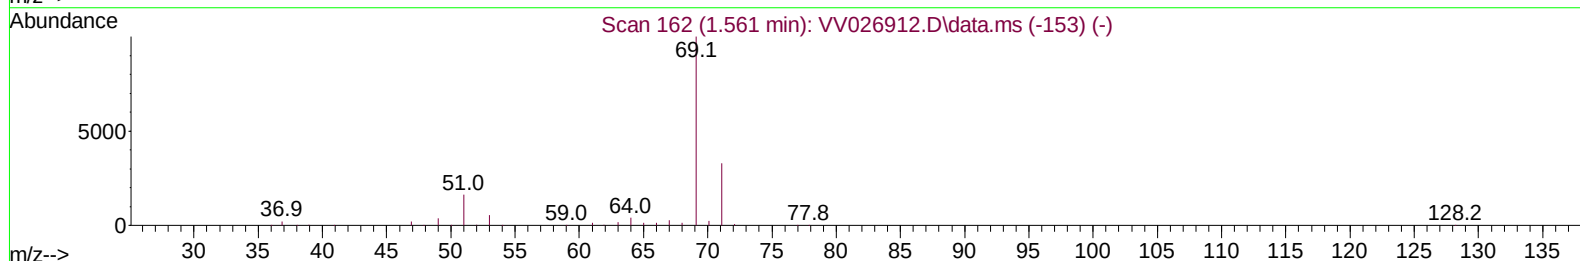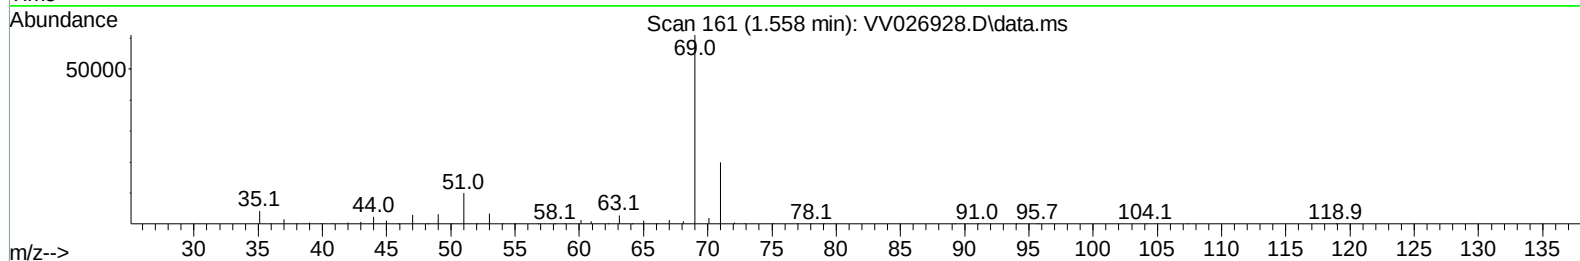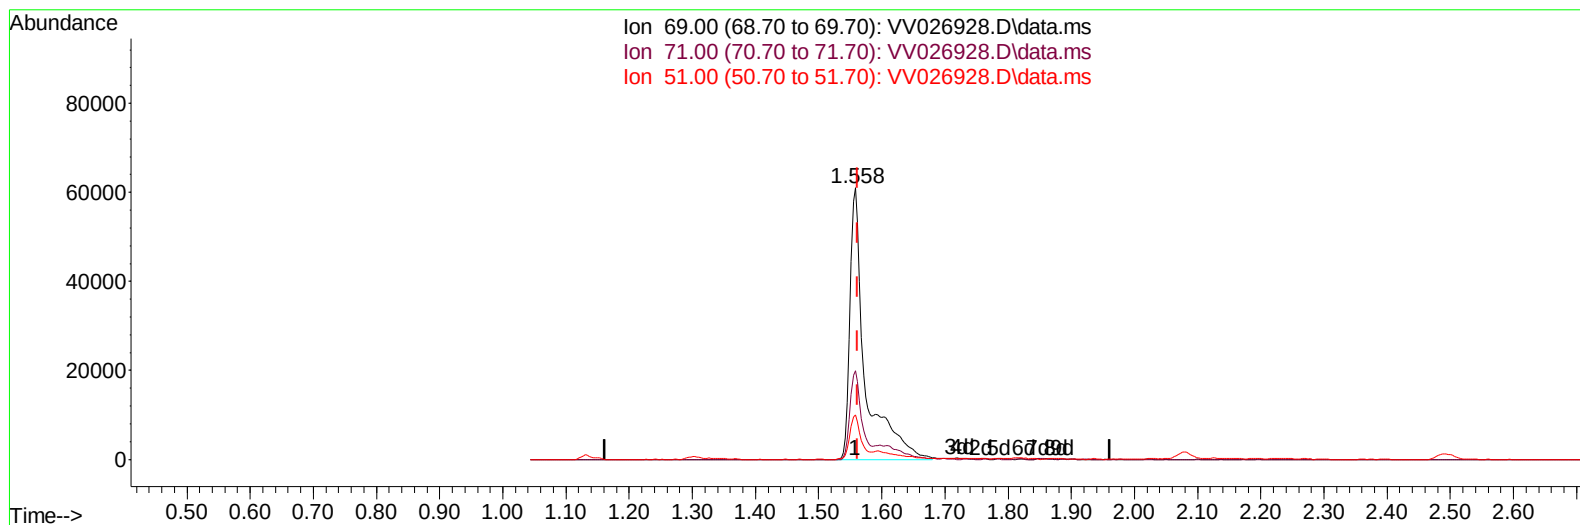

TIC: VV026928.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.003) 22.78 ug/L m

response 103769

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	24.23
51.00	23.00	12.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026928.D
 Acq On : 23 Jul 2022 17:40
 Operator : SY/MD
 Sample : N3766-06ME
 Misc : 6.15g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ZD1ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:10:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	671362	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	671914	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	296380	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	191806	34.064	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	68.120%	
7) Chloroethane-d5	1.558	69	103769m	22.780	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	45.560%#	
11) 1,1-Dichloroethene-d2	2.079	63	282938	27.930	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	55.860%#	
21) 2-Butanone-d5	3.896	46	348724	91.881	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	91.880%	
24) Chloroform-d	4.339	84	465522	42.008	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	84.020%	
26) 1,2-Dichloroethane-d4	5.024	65	288607	45.529	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.060%	
32) Benzene-d6	5.037	84	935599	46.065	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.120%	
36) 1,2-Dichloropropane-d6	6.063	67	307362	46.959	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	93.920%	
41) Toluene-d8	7.310	98	773882	43.548	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	87.100%	
43) trans-1,3-Dichloroprop...	7.619	79	114278	41.668	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	83.340%	
47) 2-Hexanone-d5	8.095	63	273855	96.091	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	96.090%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	440708	44.322	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	88.640%	
66) 1,2-Dichlorobenzene-d4	11.625	152	299939	53.943	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	107.880%	
Target Compounds						
					Qvalue	
14) Carbon disulfide	2.265	76	7954	0.537	ug/L #	91
15) Methyl Acetate	2.433	43	95056	16.171	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026928.D
Acq On : 23 Jul 2022 17:40
Operator : SY/MD
Sample : N3766-06ME
Misc : 6.15g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ZD1ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:10:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

