




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026929.D
Acq On : 23 Jul 2022 18:04
Operator : SY/MD
Sample : N3743-06ME
Misc : 5.55g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5C93ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:10:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

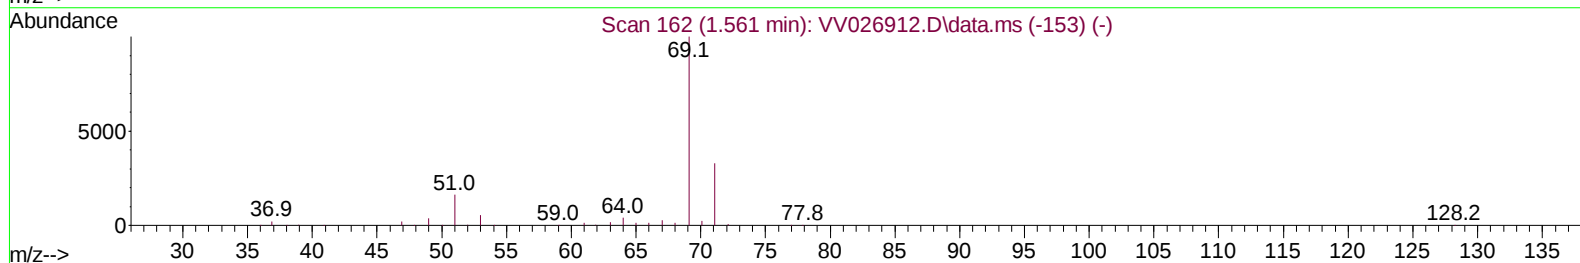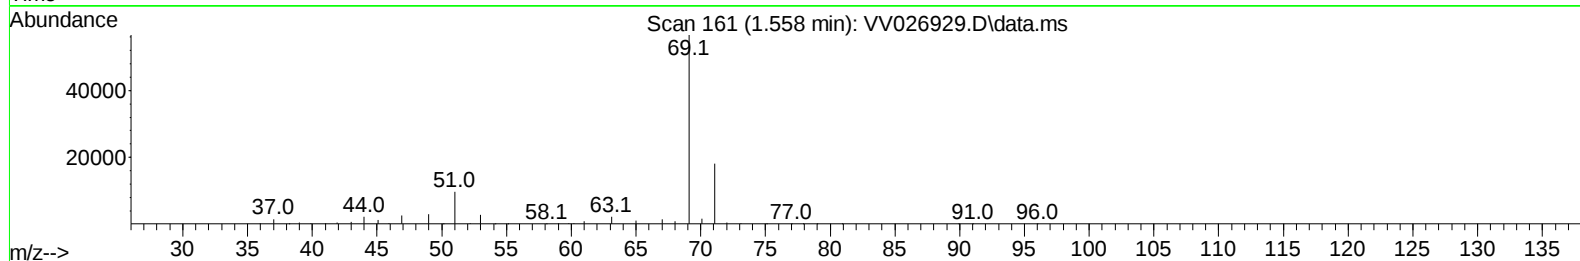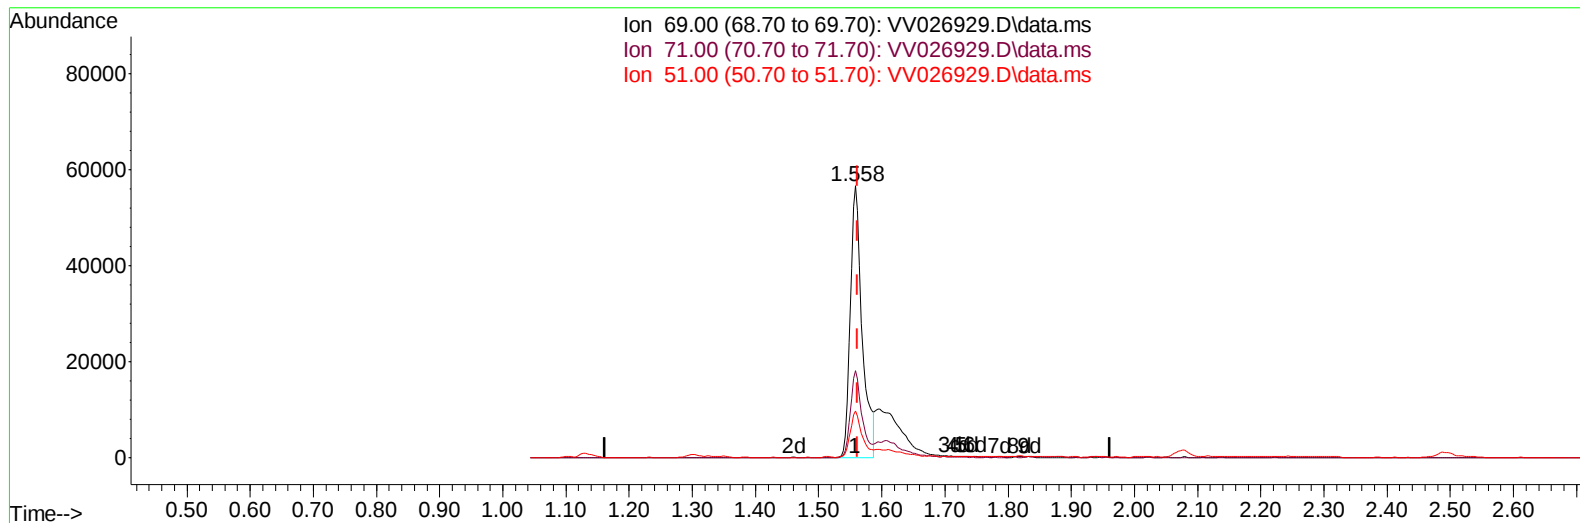

TIC: VV026929.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.003) 17.83 ug/L

response 74342

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	30.91
51.00	23.00	17.36
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026929.D
 Acq On : 23 Jul 2022 18:04
 Operator : SY/MD
 Sample : N3743-06ME
 Misc : 5.55g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5C93ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:10:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

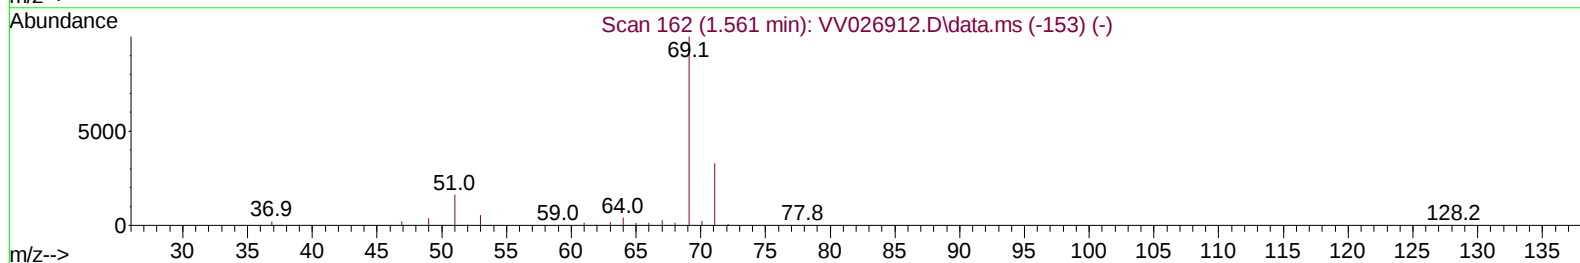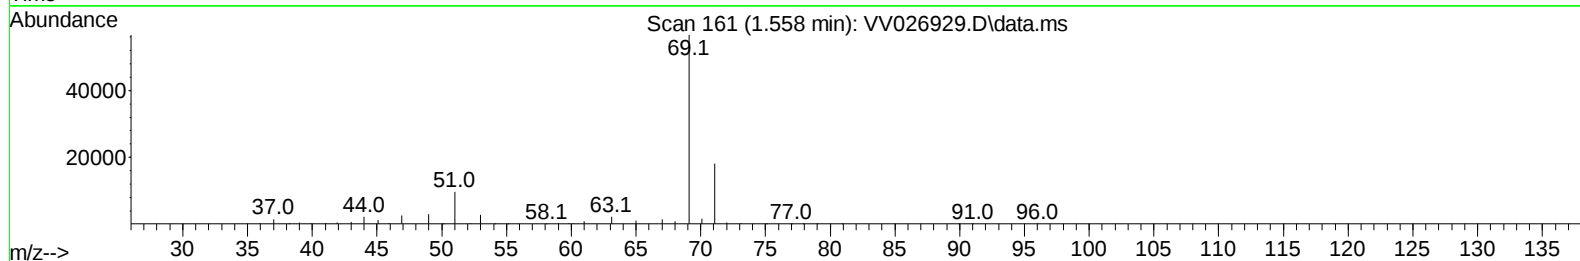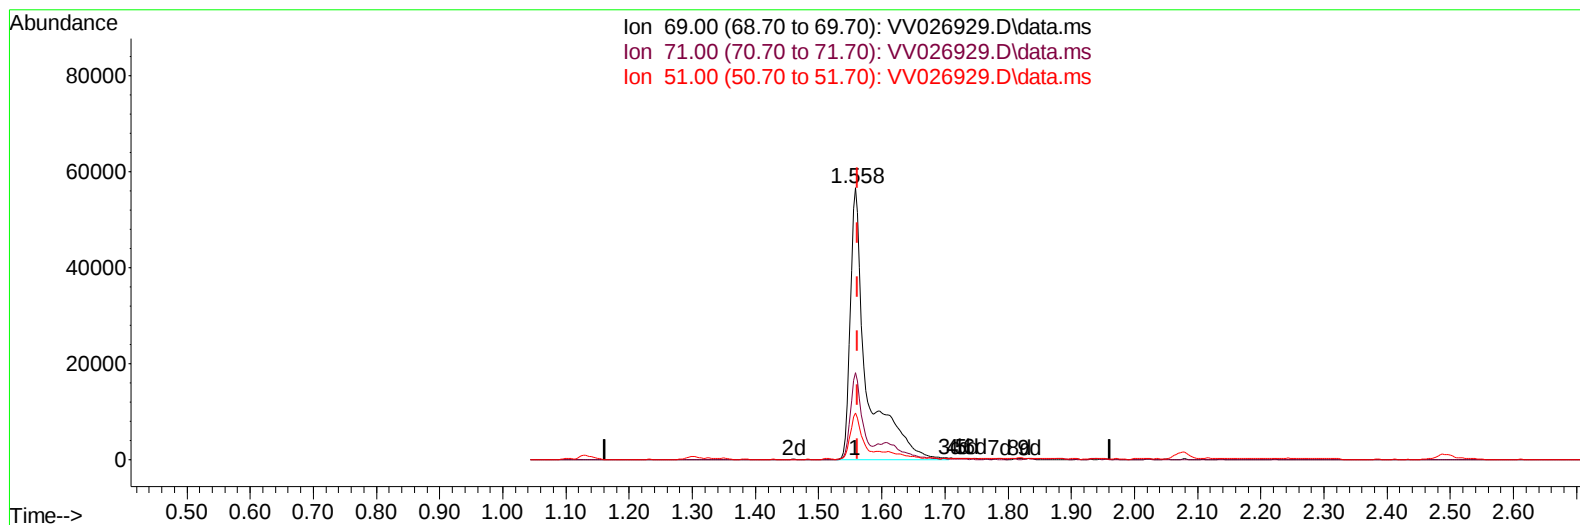

TIC: VV026929.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.003) 24.88 ug/L m

response 103741

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	22.15#
51.00	23.00	12.44#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026929.D
 Acq On : 23 Jul 2022 18:04
 Operator : SY/MD
 Sample : N3743-06ME
 Misc : 5.55g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5C93ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

Quant Time: Jul 25 02:10:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

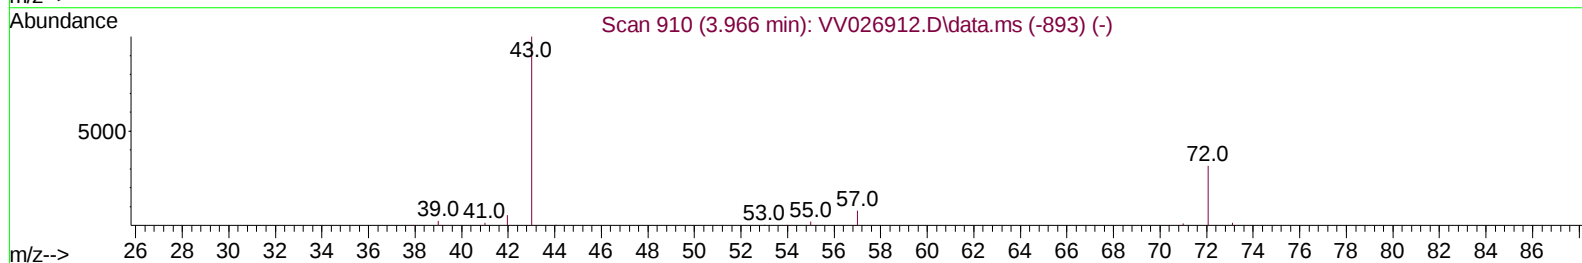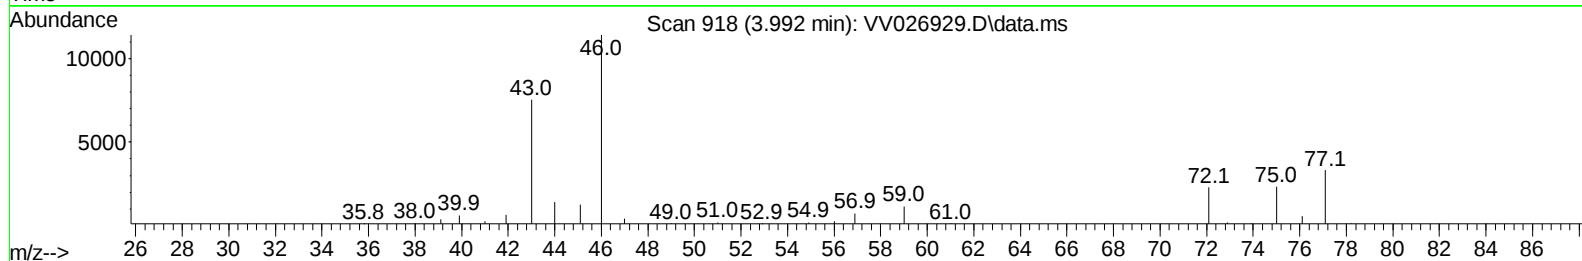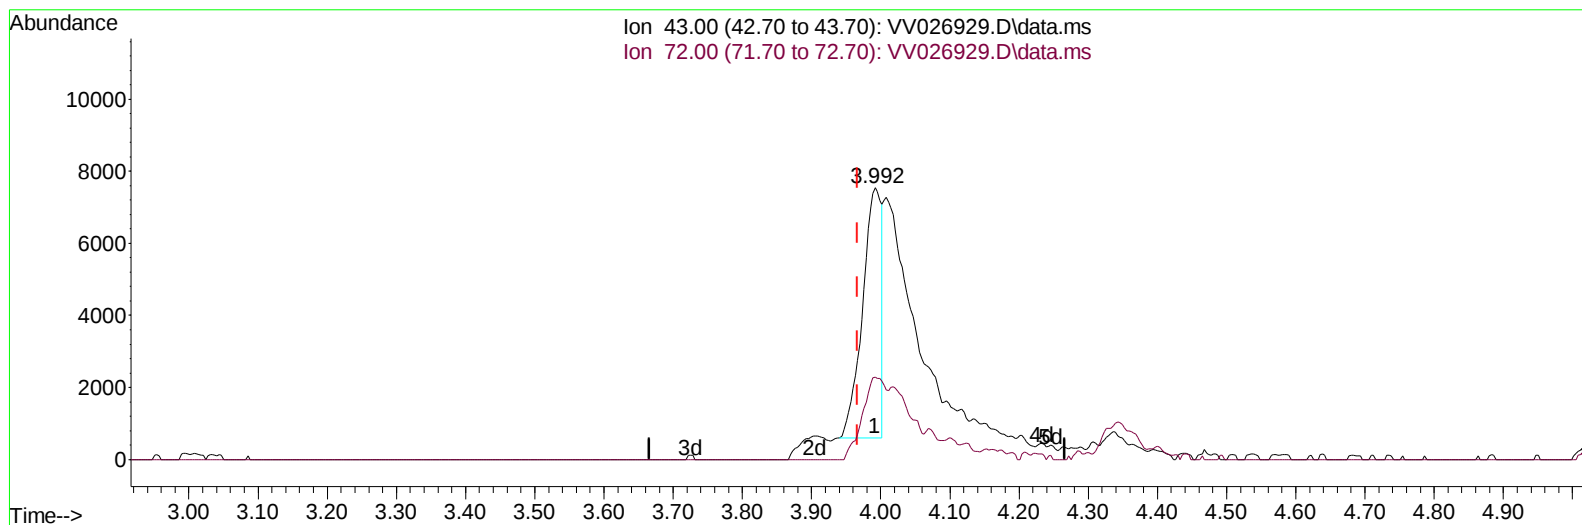

TIC: VV026929.D\data.ms

(22) 2-Butanone (T)

3.992min (+ 0.026) 3.97 ug/L

response 13219

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.70	42.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026929.D
 Acq On : 23 Jul 2022 18:04
 Operator : SY/MD
 Sample : N3743-06ME
 Misc : 5.55g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5C93ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:10:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

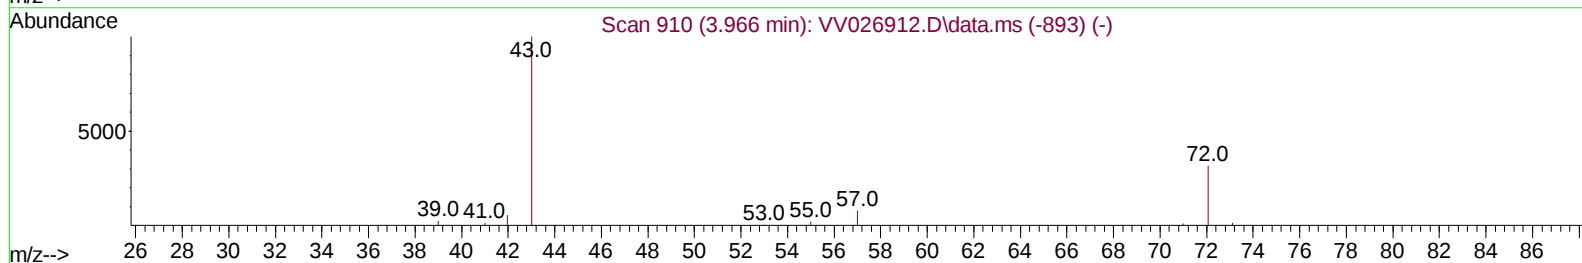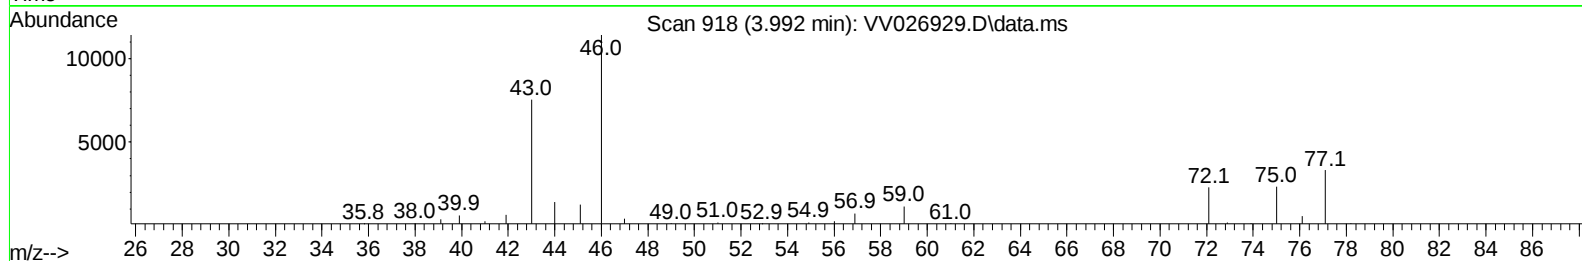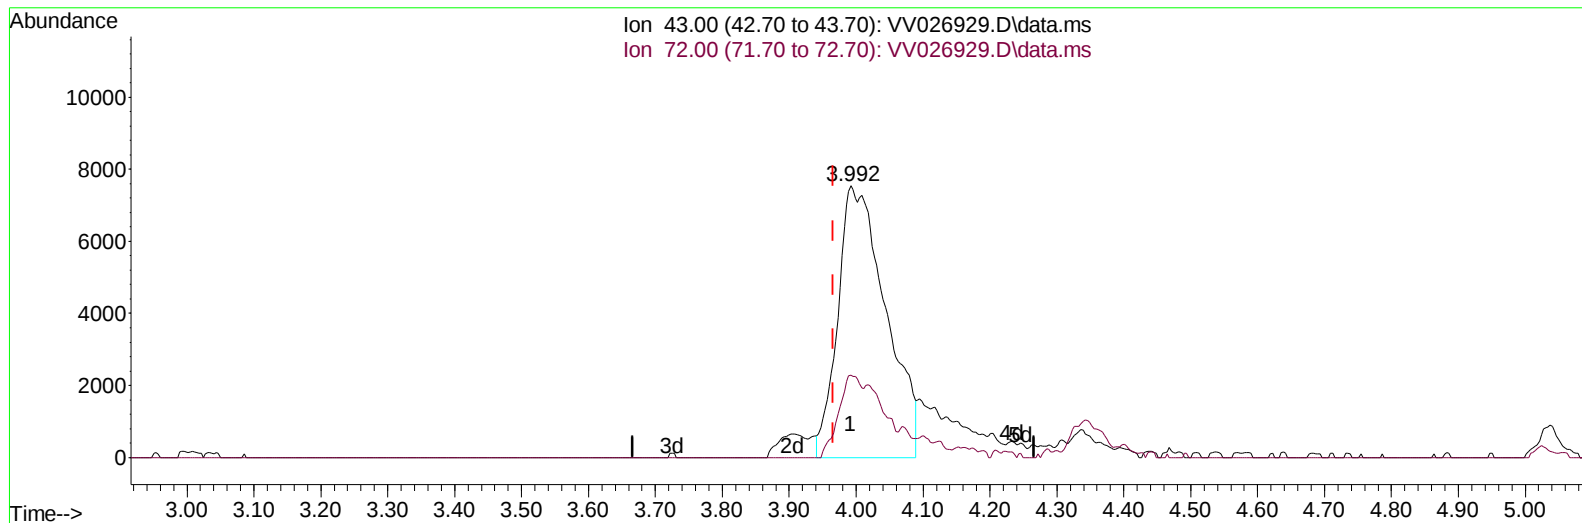

TIC: VV026929.D\data.ms

(22) 2-Butanone (T)

3.992min (+ 0.026) 11.24 ug/L m

response 37396

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.70	14.89
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026929.D
 Acq On : 23 Jul 2022 18:04
 Operator : SY/MD
 Sample : N3743-06ME
 Misc : 5.55g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5C93ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:10:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	614534	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	607107	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	263438	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	183986	35.697	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	71.400%	
7) Chloroethane-d5	1.558	69	103741m	24.880	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	49.760%#	
11) 1,1-Dichloroethene-d2	2.076	63	264168	28.489	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	56.980%#	
21) 2-Butanone-d5	3.899	46	353554	101.768	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	101.770%	
24) Chloroform-d	4.339	84	438113	43.191	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	86.380%	
26) 1,2-Dichloroethane-d4	5.024	65	275900	47.550	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.100%	
32) Benzene-d6	5.037	84	879292	47.914	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.820%	
36) 1,2-Dichloropropane-d6	6.063	67	289939	49.026	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	98.060%	
41) Toluene-d8	7.310	98	719447	44.806	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	89.620%	
43) trans-1,3-Dichloroprop...	7.619	79	108759	43.889	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	87.780%	
47) 2-Hexanone-d5	8.095	63	255435	99.195	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	99.200%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	412983	45.968	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	91.940%	
66) 1,2-Dichlorobenzene-d4	11.625	152	273021	55.242	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	110.480%	
Target Compounds						
22) 2-Butanone	3.992	43	37396m	11.240	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026929.D
Acq On : 23 Jul 2022 18:04
Operator : SY/MD
Sample : N3743-06ME
Misc : 5.55g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5C93ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:10:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

