

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072322\
 Data File : VW026924.D
 Acq On : 23 Jul 2022 16:01
 Operator : SY/MD
 Sample : N3745-02ME
 Misc : 6.79g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D06ME

Quant Time: Jul 25 02:09:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	722061	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	705088	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	310402	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	201095	33.206	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	66.420%		
7) Chloroethane-d5	1.558	69	108131m	22.071	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	44.140%#		
11) 1,1-Dichloroethene-d2	2.076	63	296184	27.185	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	54.360%#		
21) 2-Butanone-d5	3.896	46	391994	96.030	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.030%		
24) Chloroform-d	4.339	84	494132	41.459	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.920%		
26) 1,2-Dichloroethane-d4	5.021	65	301515	44.226	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.460%		
32) Benzene-d6	5.037	84	988095	46.360	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.720%		
36) 1,2-Dichloropropane-d6	6.063	67	326972	47.605	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.200%		
41) Toluene-d8	7.310	98	819011	43.919	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.840%		
43) trans-1,3-Dichloroprop...	7.619	79	123331	42.853	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.700%		
47) 2-Hexanone-d5	8.095	63	292305	97.739	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	97.740%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	462880	44.362	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.720%		
66) 1,2-Dichlorobenzene-d4	11.625	152	307547	52.813	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.620%		
Target Compounds					Qvalue	
22) 2-Butanone	3.999	43	41680m	10.662	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026924.D
Acq On : 23 Jul 2022 16:01
Operator : SY/MD
Sample : N3745-02ME
Misc : 6.79g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
F5D06ME

Quant Time: Jul 25 02:09:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

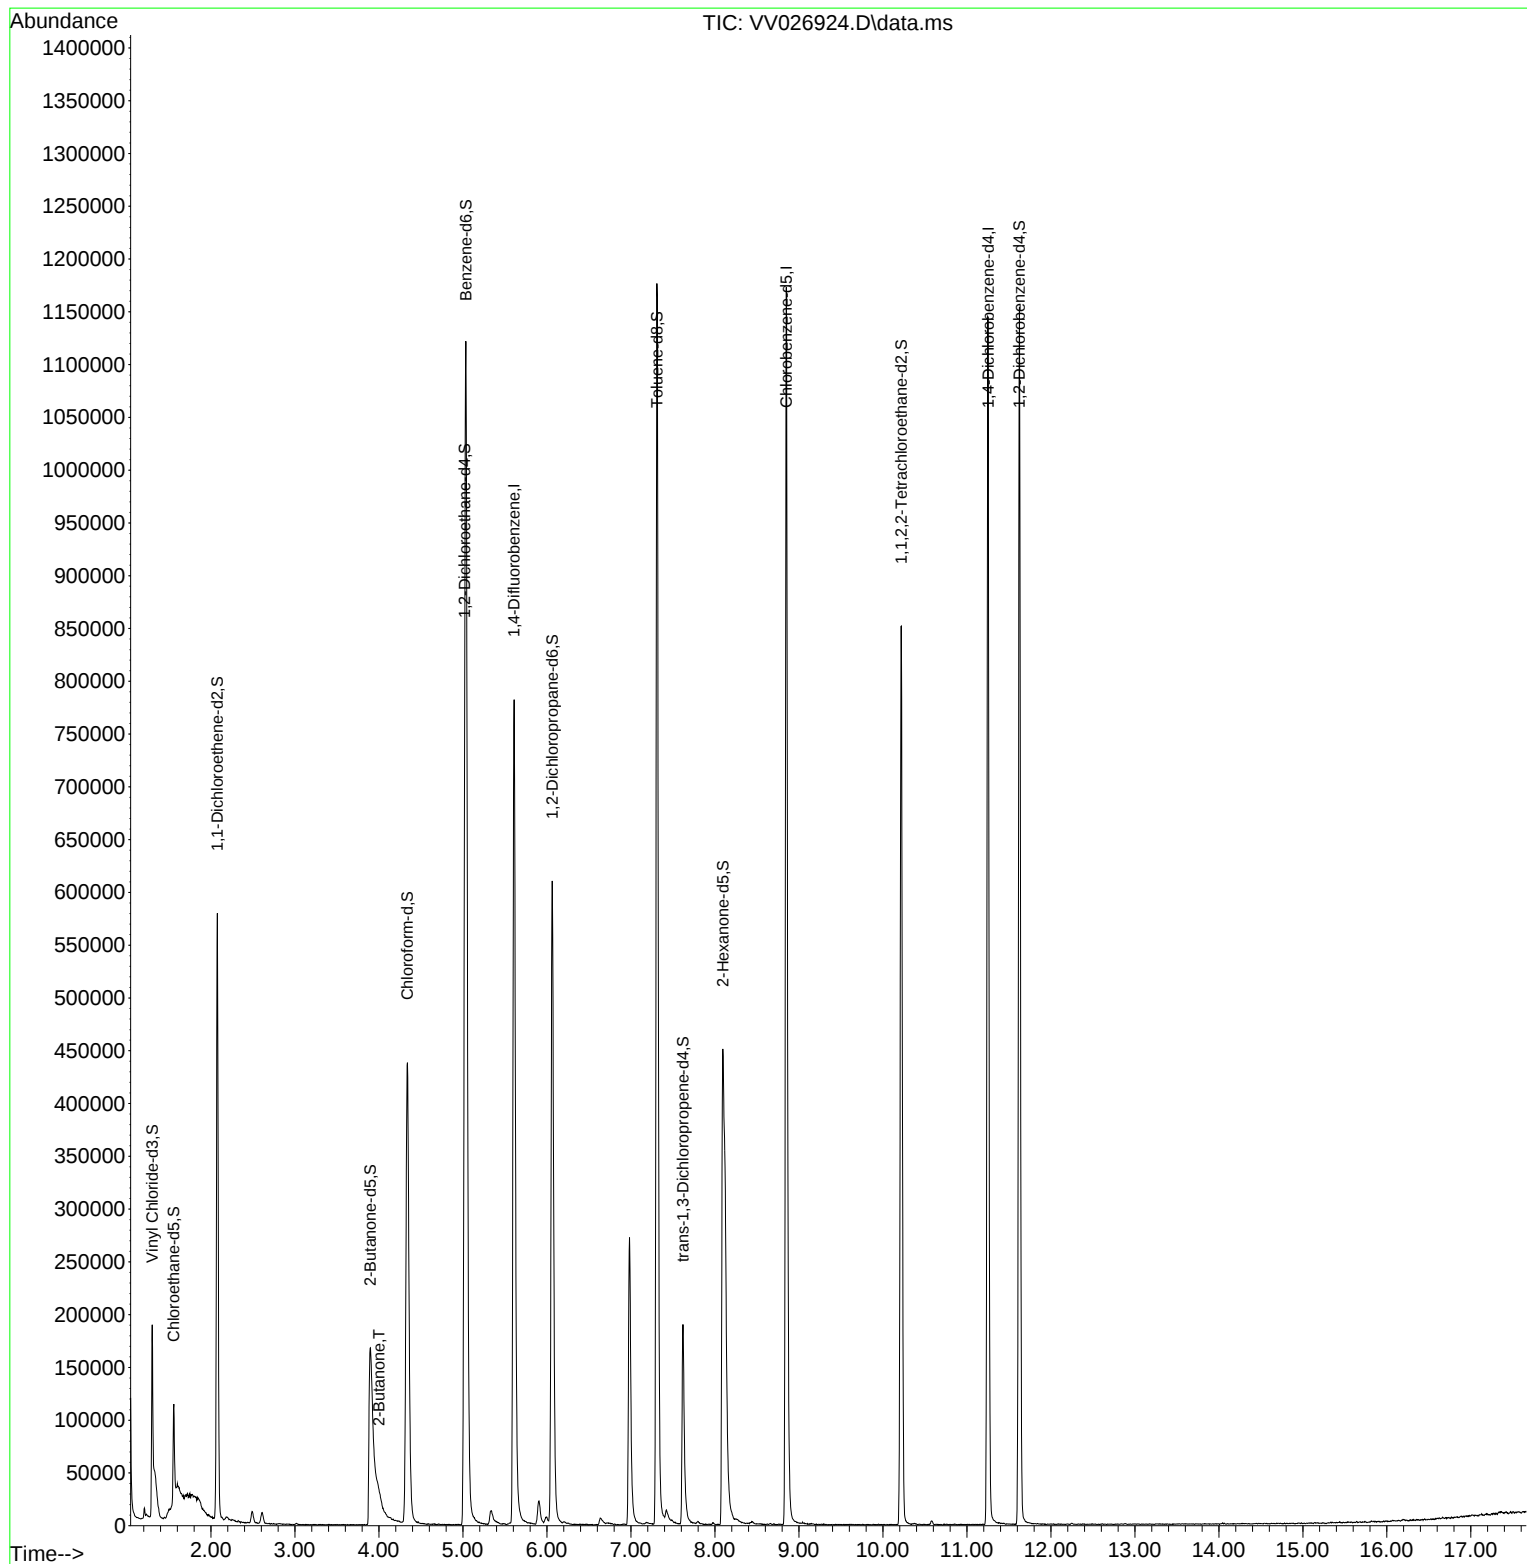

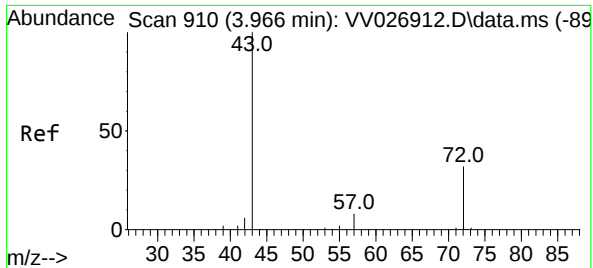

#22
 2-Butanone
 Concen: 10.662 ug/L m
 RT: 3.999 min Scan# 91
 Delta R.T. 0.032 min
 Lab File: VV026924.D
 Acq: 23 Jul 2022 16:01

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D06ME

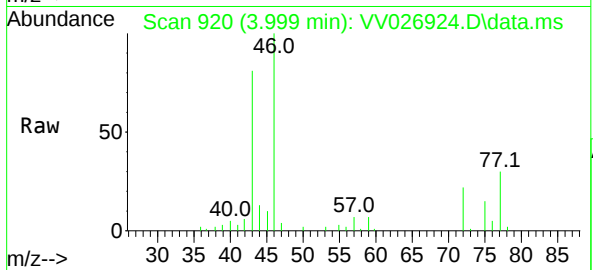

Tgt Ion: 43 Resp: 41680
 Ion Ratio Lower Upper
 43 100
 72 10.3 14.9 44.5

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

