

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072322\
 Data File : VW026925.D
 Acq On : 23 Jul 2022 16:26
 Operator : SY/MD
 Sample : N3741-11ME
 Misc : 4.89g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B36ME

Quant Time: Jul 25 02:09:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	734895	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	730399	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	328341	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	204635m	33.200	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	66.400%	
7) Chloroethane-d5	1.558	69	111120m	22.285	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	44.560%#	
11) 1,1-Dichloroethene-d2	2.076	63	296549	26.743	ug/L	-0.03
Spiked Amount	50.000	Range 60 - 125	Recovery	=	53.480%#	
21) 2-Butanone-d5	3.899	46	373652	89.938	ug/L	0.02
Spiked Amount	100.000	Range 40 - 130	Recovery	=	89.940%	
24) Chloroform-d	4.339	84	490984	40.475	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	80.960%	
26) 1,2-Dichloroethane-d4	5.024	65	306835	44.220	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.440%	
32) Benzene-d6	5.037	84	999642	45.277	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.560%	
36) 1,2-Dichloropropane-d6	6.063	67	327275	45.998	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	92.000%	
41) Toluene-d8	7.310	98	829565	42.943	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	85.880%	
43) trans-1,3-Dichloroprop...	7.619	79	122821	41.197	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	82.400%	
47) 2-Hexanone-d5	8.095	63	285157	92.045	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	92.050%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	463356	42.869	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	85.740%	
66) 1,2-Dichlorobenzene-d4	11.625	152	317556	51.552	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	103.100%	
Target Compounds						Qvalue
15) Methyl Acetate	2.432	43	45274	7.036	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026925.D
Acq On : 23 Jul 2022 16:26
Operator : SY/MD
Sample : N3741-11ME
Misc : 4.89g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
H0B36ME

Quant Time: Jul 25 02:09:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

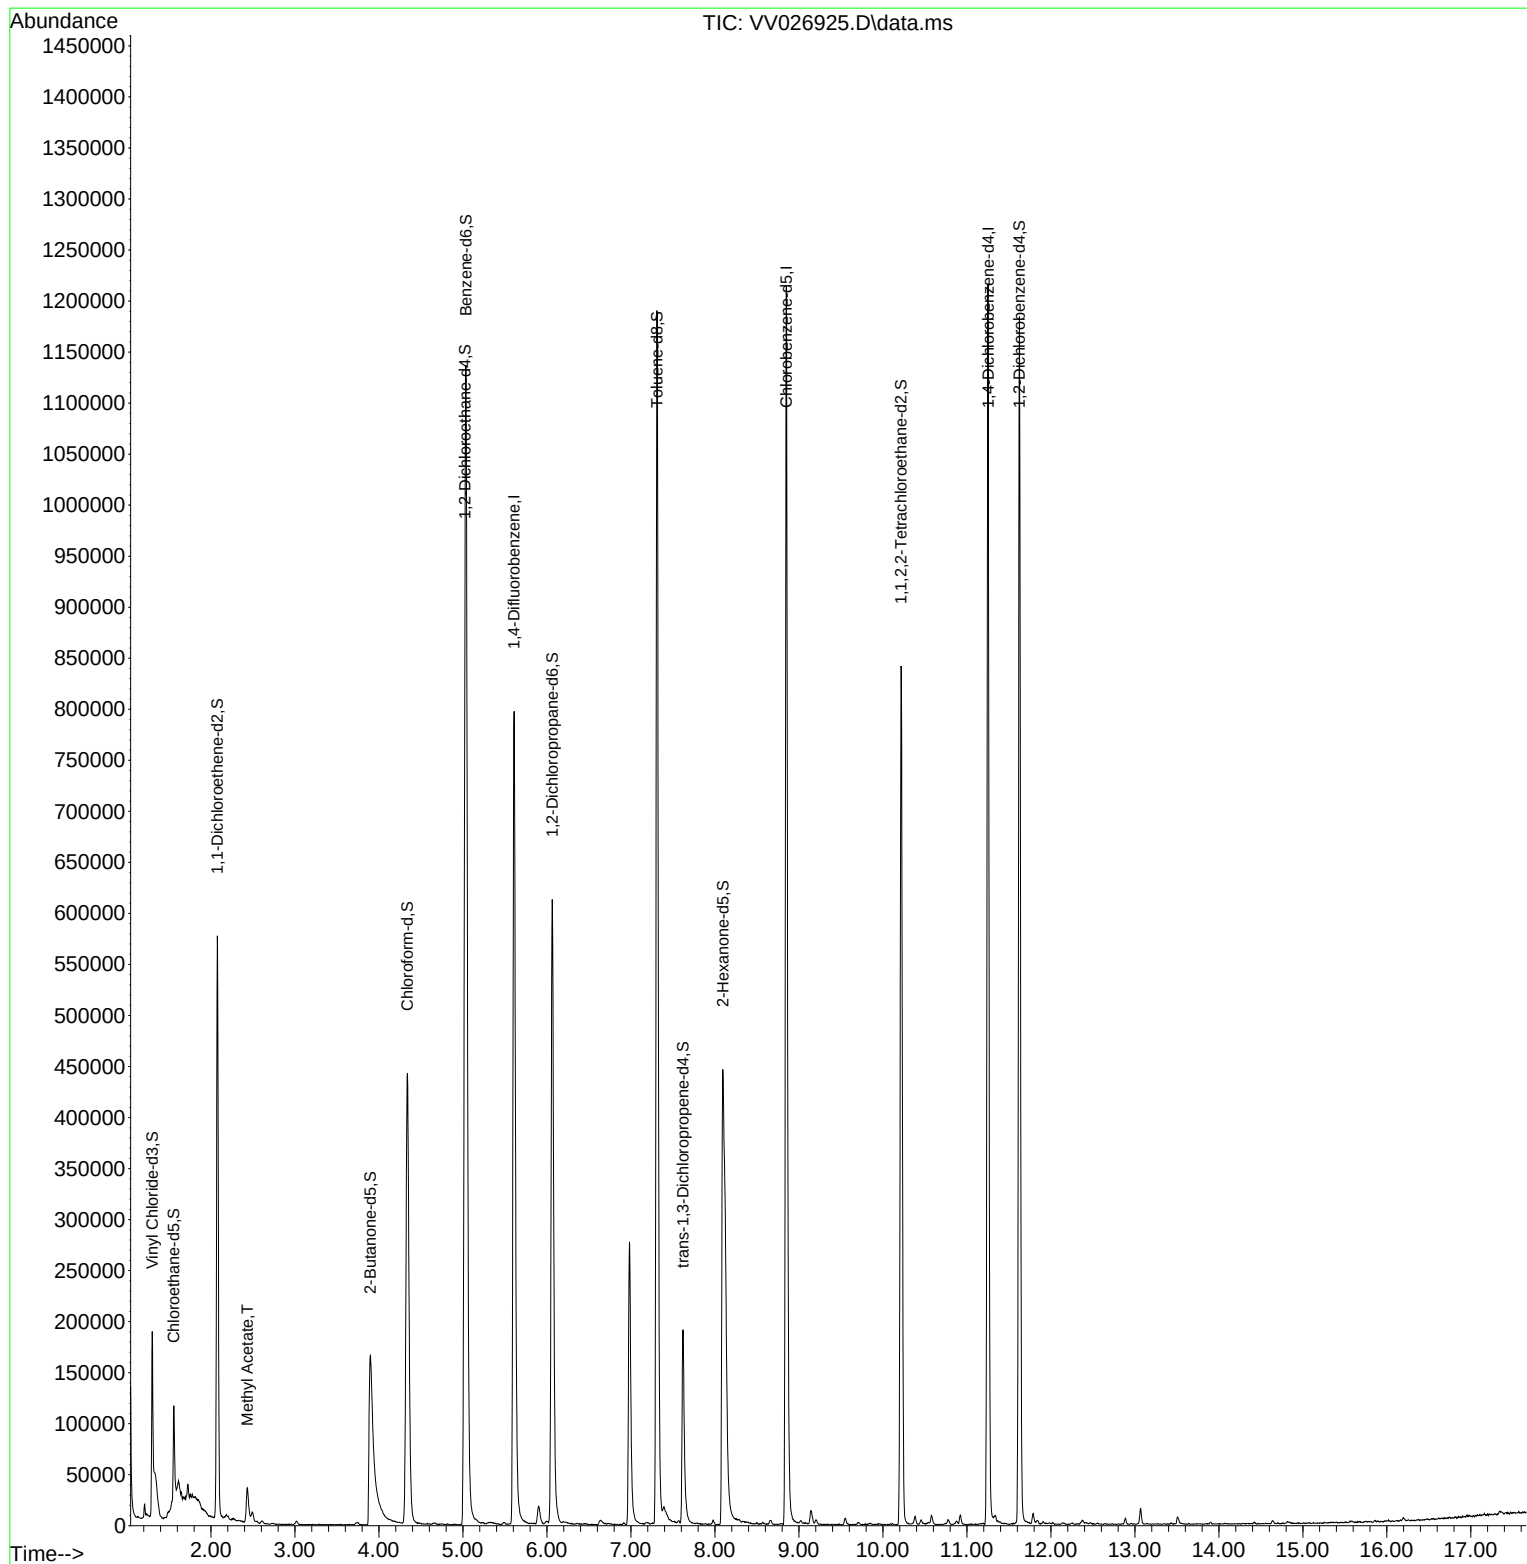

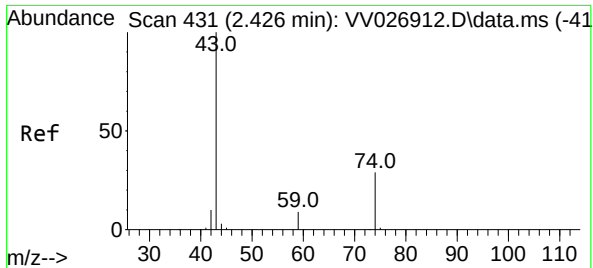

#15
Methyl Acetate
Concen: 7.036 ug/L
RT: 2.432 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV026925.D
Acq: 23 Jul 2022 16:26

Instrument :
MSVOA_V
ClientSampleId :
H0B36ME

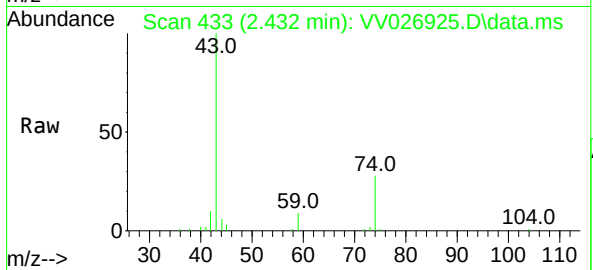

Tgt Ion: 43 Resp: 45274
Ion Ratio Lower Upper
43 100
74 28.0 22.1 33.1

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

