

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072322\
 Data File : VW026929.D
 Acq On : 23 Jul 2022 18:04
 Operator : SY/MD
 Sample : N3743-06ME
 Misc : 5.55g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5C93ME

Quant Time: Jul 25 02:10:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	614534	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	607107	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	263438	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	183986	35.697	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	71.400%		
7) Chloroethane-d5	1.558	69	103741m	24.880	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	49.760%#		
11) 1,1-Dichloroethene-d2	2.076	63	264168	28.489	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	56.980%#		
21) 2-Butanone-d5	3.899	46	353554	101.768	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.770%		
24) Chloroform-d	4.339	84	438113	43.191	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.380%		
26) 1,2-Dichloroethane-d4	5.024	65	275900	47.550	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.100%		
32) Benzene-d6	5.037	84	879292	47.914	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.820%		
36) 1,2-Dichloropropane-d6	6.063	67	289939	49.026	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.060%		
41) Toluene-d8	7.310	98	719447	44.806	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.620%		
43) trans-1,3-Dichloroprop...	7.619	79	108759	43.889	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.780%		
47) 2-Hexanone-d5	8.095	63	255435	99.195	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	99.200%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	412983	45.968	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.940%		
66) 1,2-Dichlorobenzene-d4	11.625	152	273021	55.242	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	110.480%		
Target Compounds					Qvalue	
22) 2-Butanone	3.992	43	37396m	11.240	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026929.D
Acq On : 23 Jul 2022 18:04
Operator : SY/MD
Sample : N3743-06ME
Misc : 5.55g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
F5C93ME

Quant Time: Jul 25 02:10:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

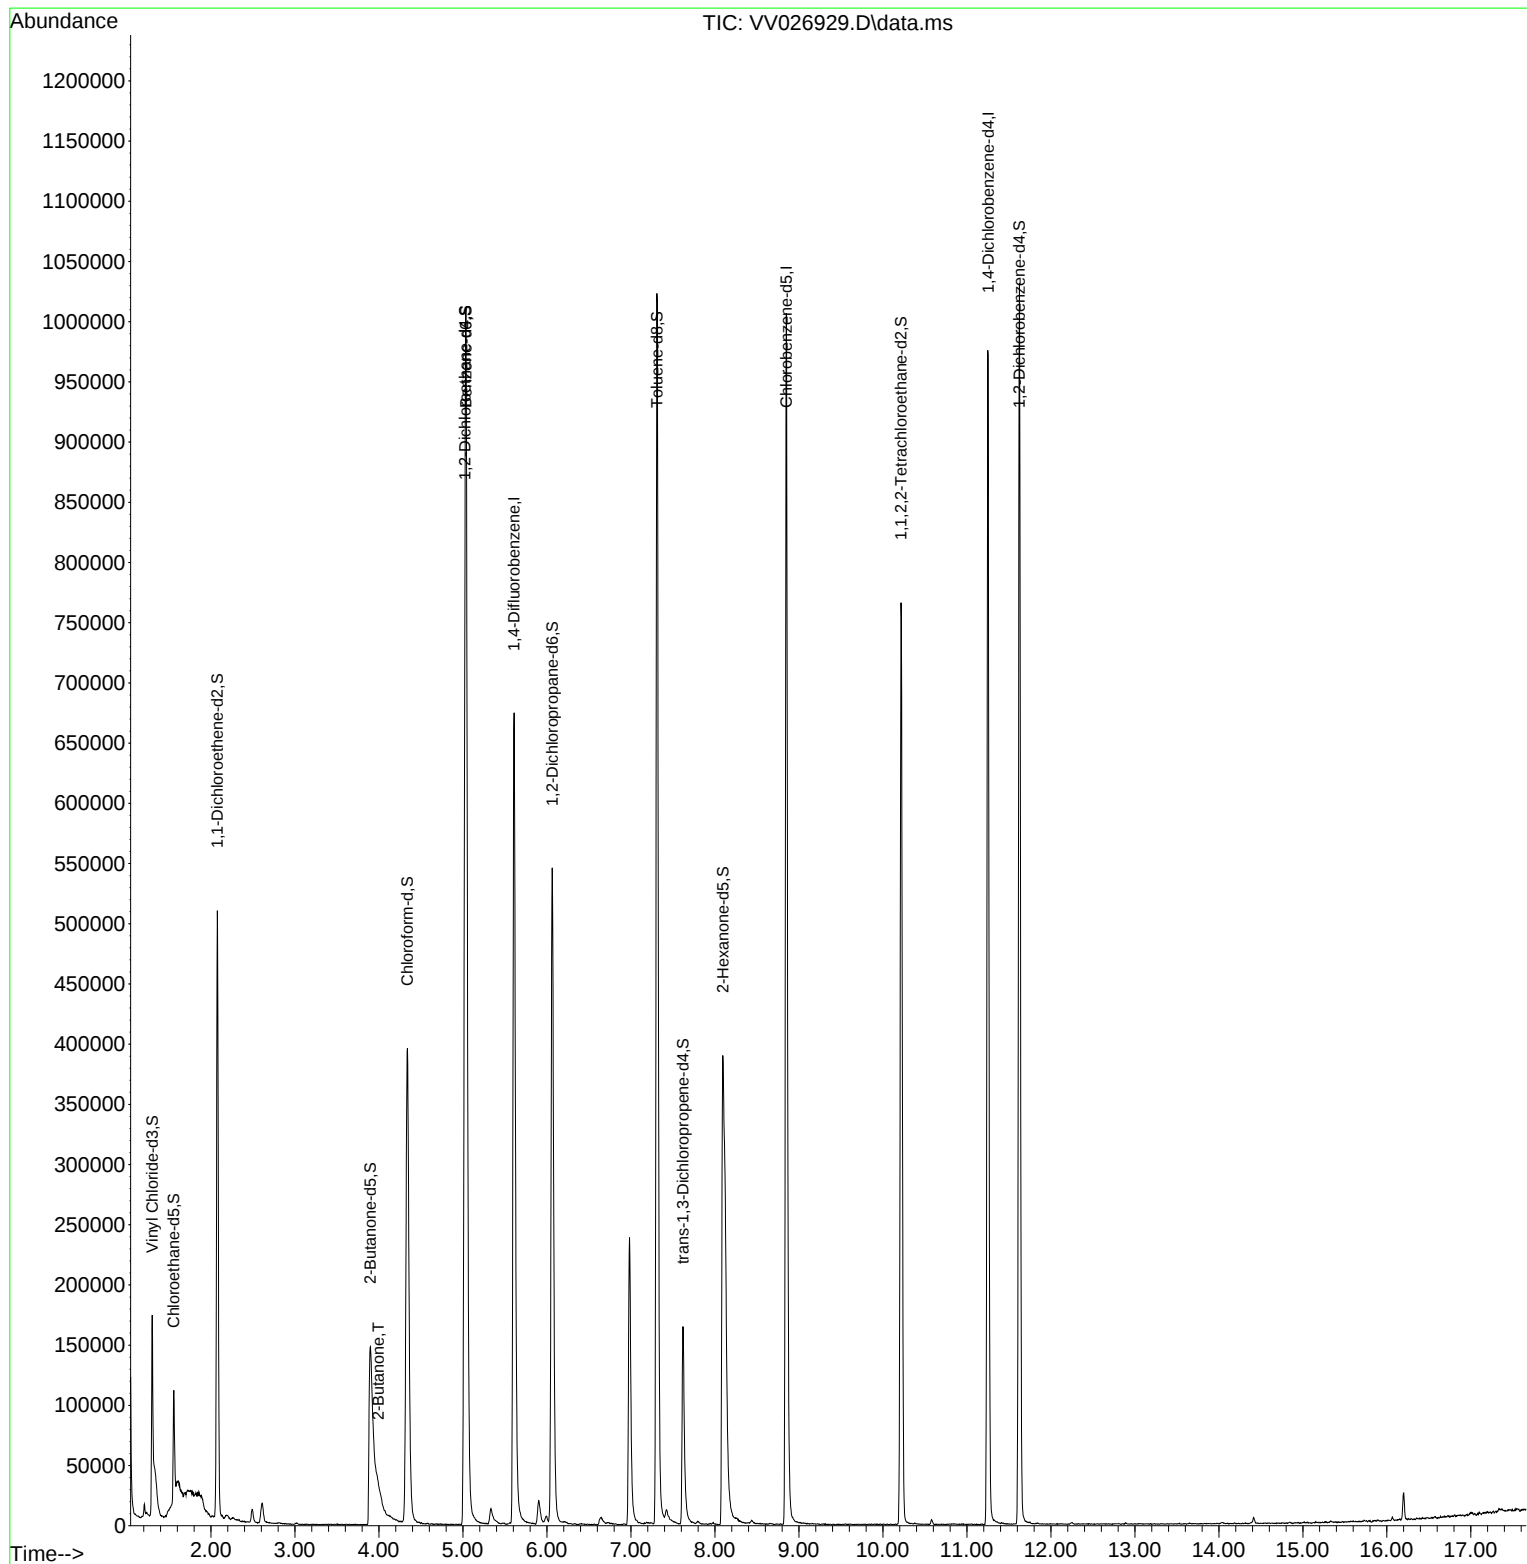

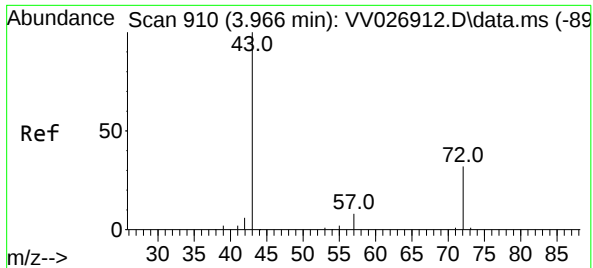

#22
 2-Butanone
 Concen: 11.240 ug/L m
 RT: 3.992 min Scan# 91
 Delta R.T. 0.026 min
 Lab File: VV026929.D
 Acq: 23 Jul 2022 18:04

Instrument :
 MSVOA_V
 ClientSampleId :
 F5C93ME

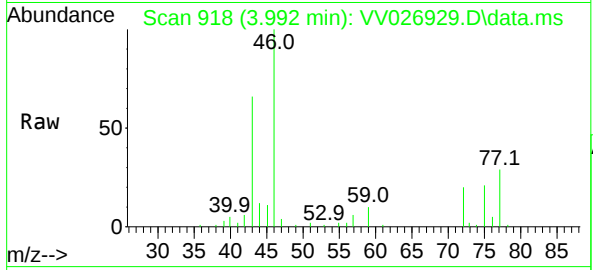

Tgt Ion: 43 Resp: 37390
 Ion Ratio Lower Upper
 43 100
 72 14.9 14.9 44.5

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

