

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026914.D
 Acq On : 23 Jul 2022 11:50
 Operator : SY/MD
 Sample : VV0723MBL01
 Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK226

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	99	rVB	278866	291679	12.32%	1.682%
2	1.565	155	163	180	rVB	264926	303243	12.81%	1.749%
3	2.101	319	330	352	rBV	518951	742404	31.37%	4.282%
4	2.253	374	377	379	rVB2	575	300	0.01%	0.002%
5	2.346	403	406	408	rBV3	374	261	0.01%	0.002%
6	2.503	446	455	466	rVV2	7273	12278	0.52%	0.071%
7	2.619	489	491	495	rVB3	416	275	0.01%	0.002%
8	2.815	548	552	555	rVV	508	348	0.01%	0.002%
9	2.873	568	570	574	rBV2	310	278	0.01%	0.002%
10	2.982	598	604	607	rVV2	413	449	0.02%	0.003%
11	3.185	661	667	671	rBV2	303	405	0.02%	0.002%
12	3.230	677	681	684	rBV3	325	302	0.01%	0.002%
13	3.626	801	804	809	rVV	310	236	0.01%	0.001%
14	3.767	844	848	852	rBV2	274	278	0.01%	0.002%
15	3.886	874	885	931	rBV	166462	569305	24.06%	3.284%
16	4.262	999	1002	1004	rBV4	468	280	0.01%	0.002%
17	4.343	1009	1027	1057	rBV	394582	981568	41.48%	5.662%
18	4.593	1102	1105	1107	rVB2	561	310	0.01%	0.002%
19	4.629	1114	1116	1120	rBV4	347	291	0.01%	0.002%
20	4.664	1125	1127	1132	rVB2	526	348	0.01%	0.002%
21	4.693	1132	1136	1139	rBV3	385	286	0.01%	0.002%
22	4.712	1139	1142	1147	rVB4	420	418	0.02%	0.002%
23	4.793	1166	1167	1171	rVB2	447	261	0.01%	0.002%
24	4.815	1171	1174	1176	rBV	534	293	0.01%	0.002%
25	4.835	1176	1180	1185	rVB4	533	440	0.02%	0.003%
26	4.944	1211	1214	1217	rVB2	553	346	0.01%	0.002%
27	4.966	1217	1221	1223	rBV2	404	336	0.01%	0.002%
28	5.040	1223	1244	1288	rBV2	917358	2366630	100.00%	13.651%
29	5.397	1353	1355	1358	rBV3	510	389	0.02%	0.002%
30	5.429	1363	1365	1372	rVB3	486	438	0.02%	0.003%
31	5.487	1380	1383	1384	rBV2	576	332	0.01%	0.002%
32	5.523	1388	1394	1395	rBV	362	304	0.01%	0.002%
33	5.613	1410	1422	1465	rBV	630178	1284468	54.27%	7.409%
34	5.802	1479	1481	1484	rBV4	649	446	0.02%	0.003%
35	5.902	1502	1512	1535	rVB4	14184	32517	1.37%	0.188%
36	6.066	1549	1563	1591	rBV	538095	1107519	46.80%	6.388%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026914.D
 Acq On : 23 Jul 2022 11:50
 Operator : SY/MD
 Sample : VV0723MBL01
 Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK226

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.310	1636	1639	1641	rBV2	437	267	0.01%	0.002%
38	6.326	1641	1644	1647	rBV3	331	259	0.01%	0.001%
39	6.461	1682	1686	1692	rVB2	367	356	0.02%	0.002%
40	6.638	1736	1741	1746	rBV6	1274	1781	0.08%	0.010%
41	6.683	1753	1755	1759	rVB3	518	269	0.01%	0.002%
42	6.757	1775	1778	1785	rVB2	478	360	0.02%	0.002%
43	6.834	1797	1802	1803	rVV2	285	263	0.01%	0.002%
44	6.982	1837	1848	1877	rBV	239340	449452	18.99%	2.592%
45	7.314	1939	1951	1983	rBV	985498	1728851	73.05%	9.972%
46	7.526	2015	2017	2020	rVB2	1027	395	0.02%	0.002%
47	7.619	2035	2046	2072	rBV	174055	313560	13.25%	1.809%
48	7.844	2111	2116	2118	rBV3	480	428	0.02%	0.002%
49	7.950	2142	2149	2154	rVV4	693	740	0.03%	0.004%
50	7.979	2154	2158	2160	rBV3	525	411	0.02%	0.002%
51	8.088	2181	2192	2233	rBV	666941	1271632	53.73%	7.335%
52	8.420	2291	2295	2297	rBV3	639	619	0.03%	0.004%
53	8.449	2302	2304	2308	rVB3	723	508	0.02%	0.003%
54	8.600	2347	2351	2354	rVB2	546	397	0.02%	0.002%
55	8.638	2359	2363	2364	rBV2	367	278	0.01%	0.002%
56	8.648	2364	2366	2369	rVB	782	399	0.02%	0.002%
57	8.680	2369	2376	2379	rBV3	292	351	0.01%	0.002%
58	8.709	2379	2385	2386	rBV2	349	305	0.01%	0.002%
59	8.850	2417	2429	2461	rBV	996530	1626655	68.73%	9.383%
60	9.149	2518	2522	2524	rBV2	362	241	0.01%	0.001%
61	9.204	2532	2539	2543	rBV2	358	570	0.02%	0.003%
62	9.307	2568	2571	2574	rBV2	376	270	0.01%	0.002%
63	9.381	2590	2594	2595	rBV2	377	306	0.01%	0.002%
64	9.474	2619	2623	2627	rVB3	342	334	0.01%	0.002%
65	9.657	2678	2680	2685	rVB2	355	239	0.01%	0.001%
66	9.805	2722	2726	2729	rBV	389	321	0.01%	0.002%
67	9.821	2729	2731	2739	rVB3	503	461	0.02%	0.003%
68	9.886	2748	2751	2754	rVB	395	235	0.01%	0.001%
69	9.940	2765	2768	2771	rVB2	444	293	0.01%	0.002%
70	9.973	2776	2778	2781	rVV2	591	362	0.02%	0.002%
71	10.133	2825	2828	2833	rVB2	343	298	0.01%	0.002%
72	10.214	2839	2853	2881	rBV	833350	1297796	54.84%	7.486%
73	10.416	2914	2916	2920	rVB3	439	334	0.01%	0.002%
74	10.458	2927	2929	2932	rVB	394	251	0.01%	0.001%
75	10.506	2941	2944	2948	rBV2	549	411	0.02%	0.002%
76	10.574	2962	2965	2971	rBV3	664	586	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026914.D
 Acq On : 23 Jul 2022 11:50
 Operator : SY/MD
 Sample : VV0723MBL01
 Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK226

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M

Title : VOC Analysis

77	10.680	2994	2998	3003	rBV2	511	551	0.02%	0.003%
78	10.902	3064	3067	3072	rVB3	348	289	0.01%	0.002%
79	10.979	3087	3091	3095	rBV3	277	310	0.01%	0.002%
80	11.063	3114	3117	3124	rVB2	482	473	0.02%	0.003%
81	11.133	3136	3139	3145	rVB2	526	445	0.02%	0.003%
82	11.246	3162	3174	3196	rBV	897986	1389724	58.72%	8.016%
83	11.532	3259	3263	3266	rBV2	667	455	0.02%	0.003%
84	11.551	3266	3269	3274	rBV3	606	481	0.02%	0.003%
85	11.622	3278	3291	3319	rBV	985802	1536264	64.91%	8.861%
86	11.812	3347	3350	3355	rBV4	666	581	0.02%	0.003%
87	12.027	3413	3417	3420	rBV3	412	396	0.02%	0.002%
88	12.333	3509	3512	3516	rBV2	361	285	0.01%	0.002%
89	12.384	3525	3528	3533	rBV4	286	310	0.01%	0.002%
90	12.677	3616	3619	3624	rBV2	515	524	0.02%	0.003%
91	13.149	3764	3766	3770	rBV2	346	247	0.01%	0.001%
92	13.188	3774	3778	3780	rBV	366	302	0.01%	0.002%
93	13.249	3795	3797	3801	rVB3	605	336	0.01%	0.002%
94	13.590	3900	3903	3907	rBV4	426	347	0.01%	0.002%
95	13.783	3960	3963	3966	rVB	721	370	0.02%	0.002%
96	13.808	3969	3971	3975	rVB2	498	288	0.01%	0.002%
97	14.066	4048	4051	4058	rBV5	411	391	0.02%	0.002%
98	14.181	4083	4087	4090	rBV4	360	339	0.01%	0.002%
99	14.660	4232	4236	4241	rBV2	580	705	0.03%	0.004%
100	14.754	4262	4265	4267	rBV3	639	412	0.02%	0.002%




Sum of corrected areas: 17336930

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026914.D
Acq On : 23 Jul 2022 11:50
Operator : SY/MD
Sample : VV0723MBL01
Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK226

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

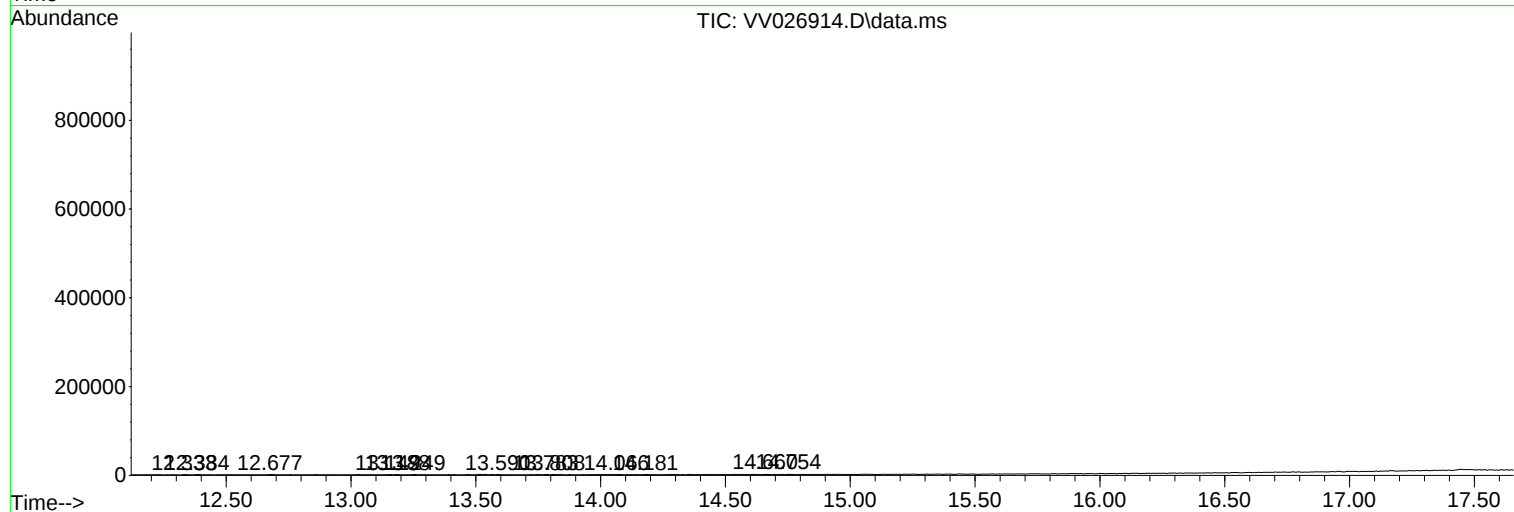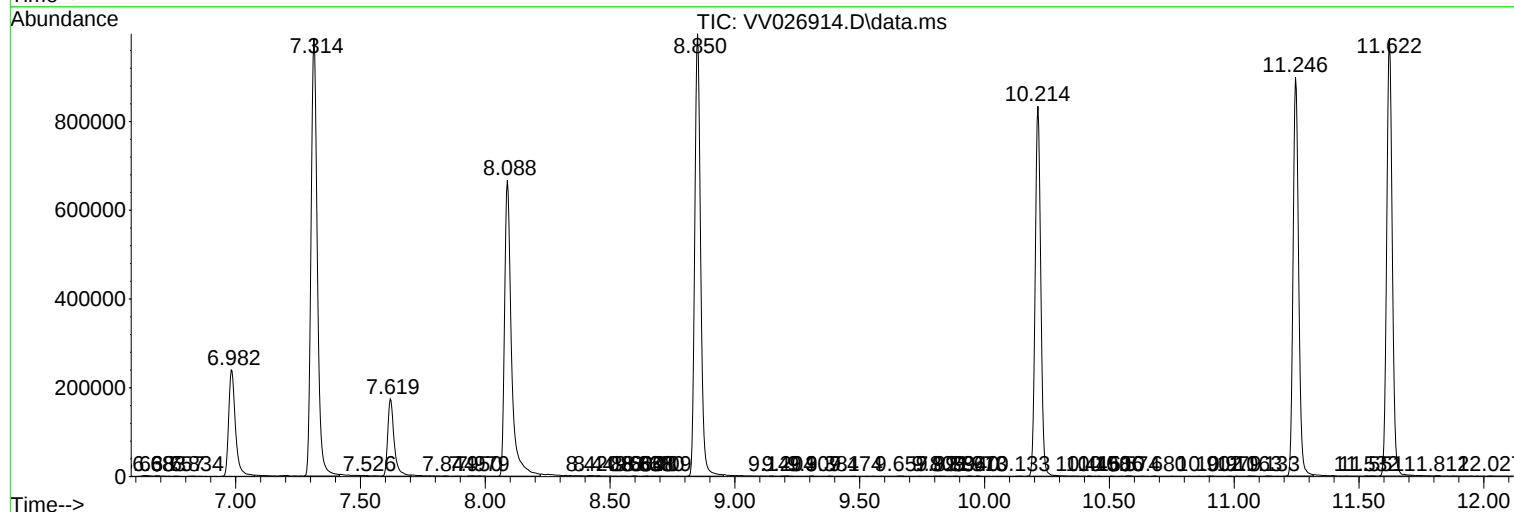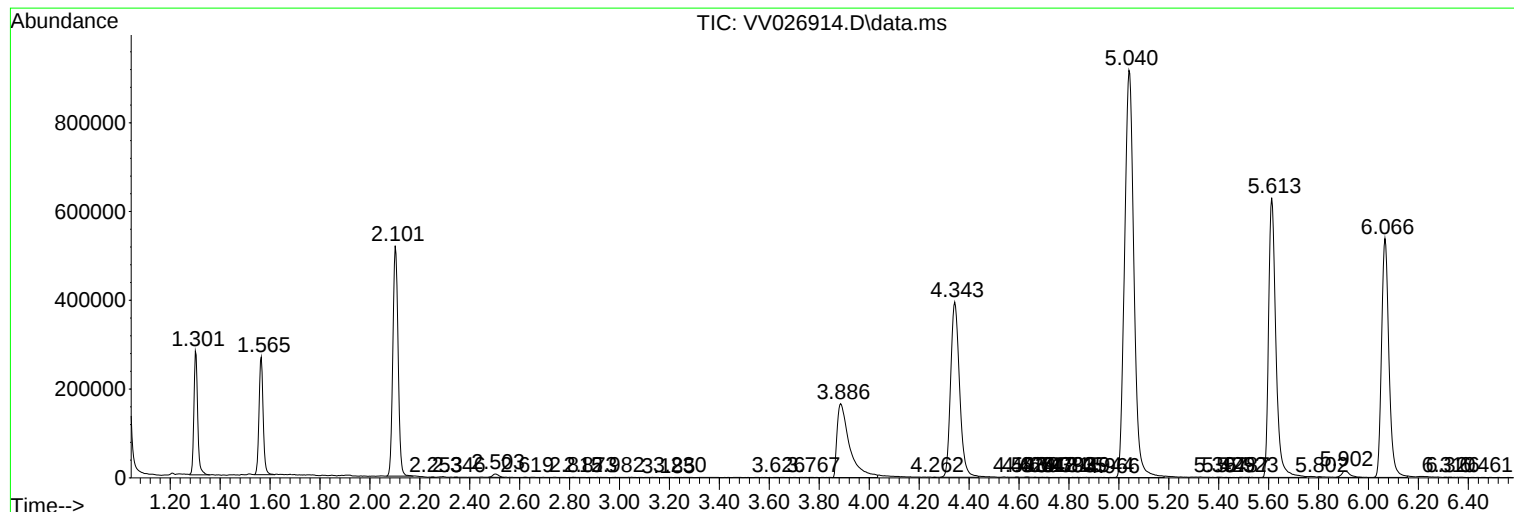

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026914.D
Acq On : 23 Jul 2022 11:50
Operator : SY/MD
Sample : VV0723MBL01
Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK226

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026914.D
Acq On : 23 Jul 2022 11:50
Operator : SY/MD
Sample : VV0723MBL01
Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK226

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc