

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026916.D
 Acq On : 23 Jul 2022 12:45
 Operator : SY/MD
 Sample : N3743-01ME
 Misc : 5.30g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5C87ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	87	rBV	79002	89673	4.71%	0.797%
2	2.076	313	322	335	rVB	244727	351500	18.48%	3.126%
3	3.297	699	702	704	rBV	380	217	0.01%	0.002%
4	3.378	720	727	730	rBV3	457	508	0.03%	0.005%
5	3.407	734	736	738	rBV	261	137	0.01%	0.001%
6	3.503	763	766	768	rBV	217	147	0.01%	0.001%
7	3.542	775	778	783	rVB2	356	283	0.01%	0.003%
8	3.571	783	787	792	rVB2	555	461	0.02%	0.004%
9	3.603	792	797	803	rBV3	431	557	0.03%	0.005%
10	3.625	803	804	806	rVB	179	46	0.00%	0.000%
11	3.641	806	809	811	rBV2	234	129	0.01%	0.001%
12	3.654	811	813	816	rVB	276	136	0.01%	0.001%
13	3.680	816	821	822	rBV	294	191	0.01%	0.002%
14	3.748	839	842	845	rBV	189	154	0.01%	0.001%
15	3.815	859	863	866	rVB2	411	251	0.01%	0.002%
16	3.831	866	868	869	rBV	161	77	0.00%	0.001%
17	3.867	876	879	881	rBV2	354	233	0.01%	0.002%
18	3.908	881	892	913	rBV2	68859	246568	12.96%	2.193%
19	4.339	1012	1026	1060	rVB2	182088	483934	25.44%	4.304%
20	4.667	1126	1128	1131	rVB2	396	186	0.01%	0.002%
21	4.722	1142	1145	1147	rBV	392	203	0.01%	0.002%
22	4.741	1147	1151	1155	rVB3	457	409	0.02%	0.004%
23	4.757	1155	1156	1157	rBV3	177	52	0.00%	0.000%
24	4.773	1158	1161	1165	rVB3	493	409	0.02%	0.004%
25	4.796	1165	1168	1172	rBV3	493	465	0.02%	0.004%
26	4.815	1172	1174	1179	rBV	482	315	0.02%	0.003%
27	4.873	1190	1192	1194	rBV	199	104	0.01%	0.001%
28	4.899	1198	1200	1206	rBV2	329	301	0.02%	0.003%
29	4.924	1206	1208	1209	rBV2	242	97	0.01%	0.001%
30	4.966	1219	1221	1225	rVB2	239	126	0.01%	0.001%
31	5.034	1226	1242	1273	rBV2	469966	1179896	62.02%	10.493%
32	5.336	1326	1336	1353	rBV4	12633	33523	1.76%	0.298%
33	5.539	1397	1399	1401	rBV3	617	334	0.02%	0.003%
34	5.555	1401	1404	1406	rVV3	839	612	0.03%	0.005%
35	5.609	1409	1421	1453	rVV	714167	1502835	78.99%	13.365%
36	5.908	1503	1514	1530	rBV9	16779	41654	2.19%	0.370%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072322\
 Data File : VW026916.D
 Acq On : 23 Jul 2022 12:45
 Operator : SY/MD
 Sample : N3743-01ME
 Misc : 5.30g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5C87ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.066	1551	1563	1593	rVB	253152	547766	28.79%	4.871%
38	6.329	1643	1645	1649	rBV4	427	260	0.01%	0.002%
39	6.474	1684	1690	1698	rVB4	596	760	0.04%	0.007%
40	6.506	1698	1700	1702	rBV2	214	106	0.01%	0.001%
41	6.529	1702	1707	1712	rBV4	555	551	0.03%	0.005%
42	6.593	1724	1727	1730	rVB	433	201	0.01%	0.002%
43	6.609	1730	1732	1733	rBV	281	123	0.01%	0.001%
44	6.648	1733	1744	1755	rBV5	5077	11905	0.63%	0.106%
45	6.799	1788	1791	1794	rVB3	1082	634	0.03%	0.006%
46	6.889	1816	1819	1820	rBV	100	57	0.00%	0.001%
47	6.902	1820	1823	1824	rBV2	488	227	0.01%	0.002%
48	6.985	1838	1849	1877	rBV	113376	232165	12.20%	2.065%
49	7.313	1939	1951	1974	rBV	453751	824646	43.35%	7.334%
50	7.622	2037	2047	2075	rBV	76443	155660	8.18%	1.384%
51	7.841	2113	2115	2117	rBV	320	180	0.01%	0.002%
52	7.895	2129	2132	2136	rBV4	372	351	0.02%	0.003%
53	7.940	2142	2146	2148	rBV2	581	352	0.02%	0.003%
54	7.976	2148	2157	2171	rBV2	20351	35999	1.89%	0.320%
55	8.040	2175	2177	2182	rVB3	279	183	0.01%	0.002%
56	8.098	2185	2195	2229	rBV	155951	554430	29.14%	4.931%
57	8.548	2333	2335	2337	rBV	461	211	0.01%	0.002%
58	8.603	2348	2352	2356	rBV3	350	402	0.02%	0.004%
59	8.693	2377	2380	2382	rBV2	277	169	0.01%	0.002%
60	8.773	2403	2405	2407	rBV	361	166	0.01%	0.001%
61	8.850	2416	2429	2456	rBV	1075794	1902502	100.00%	16.920%
62	9.268	2557	2559	2561	rBV2	336	130	0.01%	0.001%
63	9.381	2589	2594	2595	rBV	286	236	0.01%	0.002%
64	9.445	2612	2614	2615	rBV	304	123	0.01%	0.001%
65	9.480	2623	2625	2626	rBV2	418	84	0.00%	0.001%
66	9.587	2656	2658	2659	rBV2	372	142	0.01%	0.001%
67	9.648	2675	2677	2681	rVB	273	155	0.01%	0.001%
68	9.667	2681	2683	2687	rVB2	190	104	0.01%	0.001%
69	9.693	2687	2691	2695	rVB2	379	306	0.02%	0.003%
70	9.715	2695	2698	2700	rBV2	308	237	0.01%	0.002%
71	9.866	2742	2745	2749	rVB2	372	299	0.02%	0.003%
72	9.927	2763	2764	2767	rBV	252	91	0.00%	0.001%
73	10.091	2812	2815	2817	rBV2	459	232	0.01%	0.002%
74	10.172	2837	2840	2842	rBV2	338	211	0.01%	0.002%
75	10.220	2842	2855	2874	rBV	362622	633961	33.32%	5.638%
76	10.419	2915	2917	2920	rBV2	252	172	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026916.D
 Acq On : 23 Jul 2022 12:45
 Operator : SY/MD
 Sample : N3743-01ME
 Misc : 5.30g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5C87ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M

Title : VOC Analysis

77	10.471	2930	2933	2935	rVB2	297	177	0.01%	0.002%
78	10.490	2935	2939	2941	rBV	352	297	0.02%	0.003%
79	10.580	2960	2967	2979	rVB6	3707	5328	0.28%	0.047%
80	10.905	3066	3068	3071	rVB	265	116	0.01%	0.001%
81	10.931	3073	3076	3080	rVB2	431	313	0.02%	0.003%
82	10.953	3080	3083	3084	rBV	197	103	0.01%	0.001%
83	11.059	3113	3116	3118	rBV	319	197	0.01%	0.002%
84	11.252	3164	3176	3199	rBV	1049835	1650779	86.77%	14.681%
85	11.625	3281	3292	3314	rBV	460615	743159	39.06%	6.609%
86	12.496	3560	3563	3564	rBV2	332	178	0.01%	0.002%
87	12.532	3571	3574	3580	rBV3	551	461	0.02%	0.004%




Sum of corrected areas: 11244320

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026916.D
Acq On : 23 Jul 2022 12:45
Operator : SY/MD
Sample : N3743-01ME
Misc : 5.30g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5C87ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

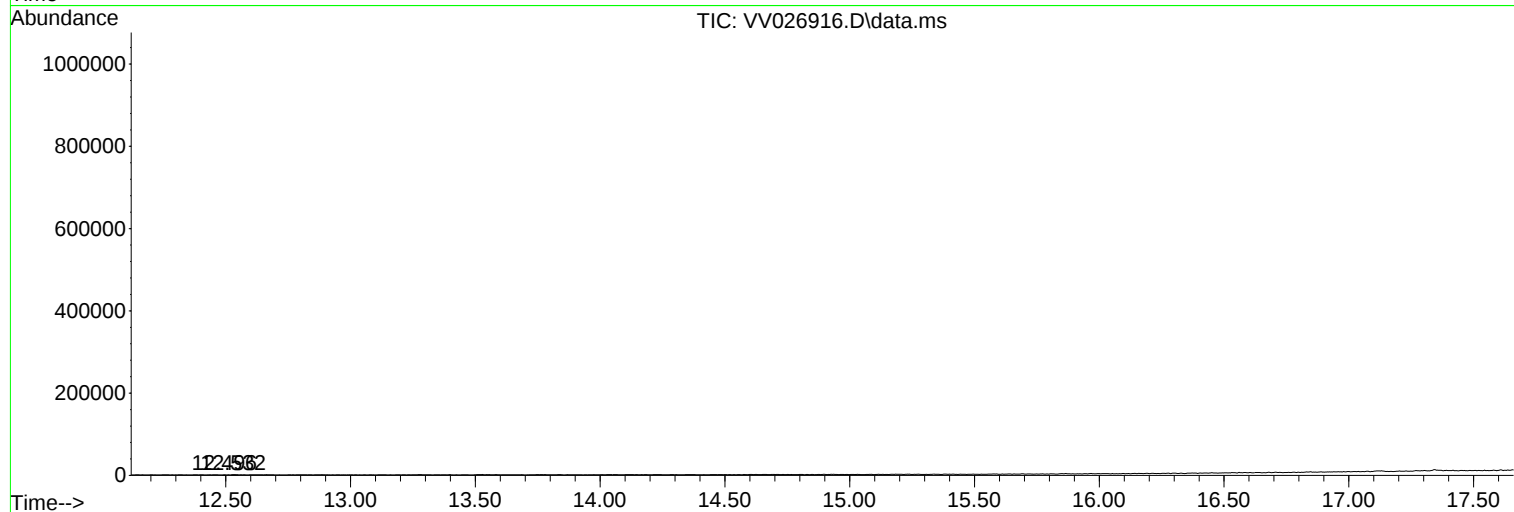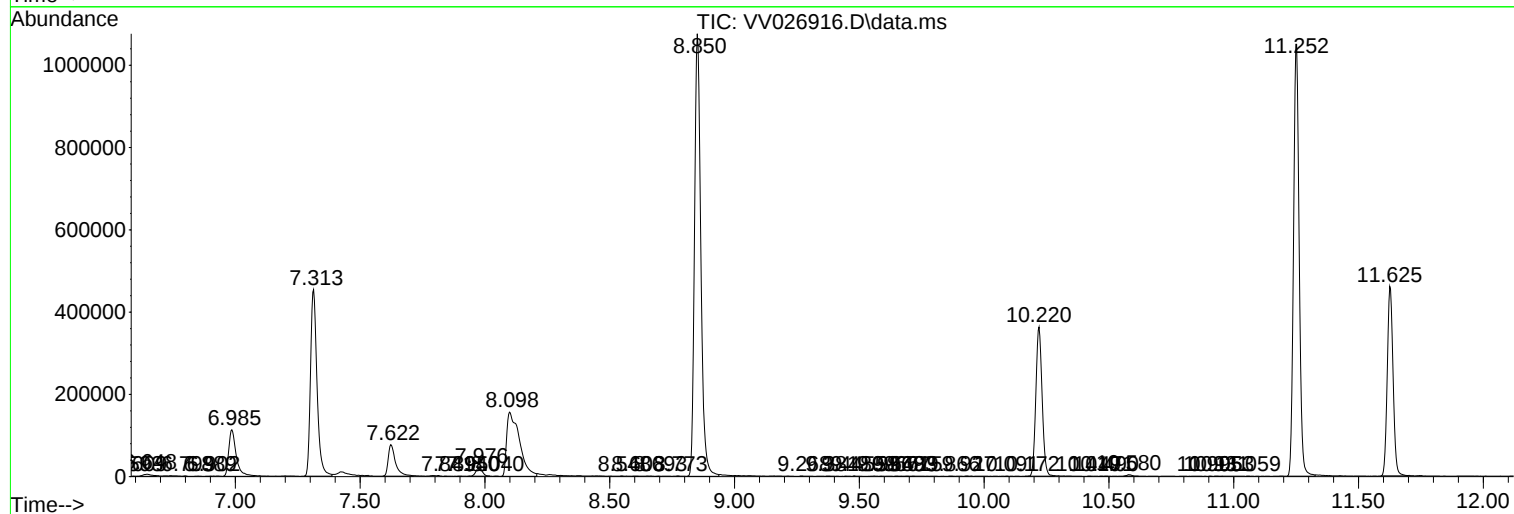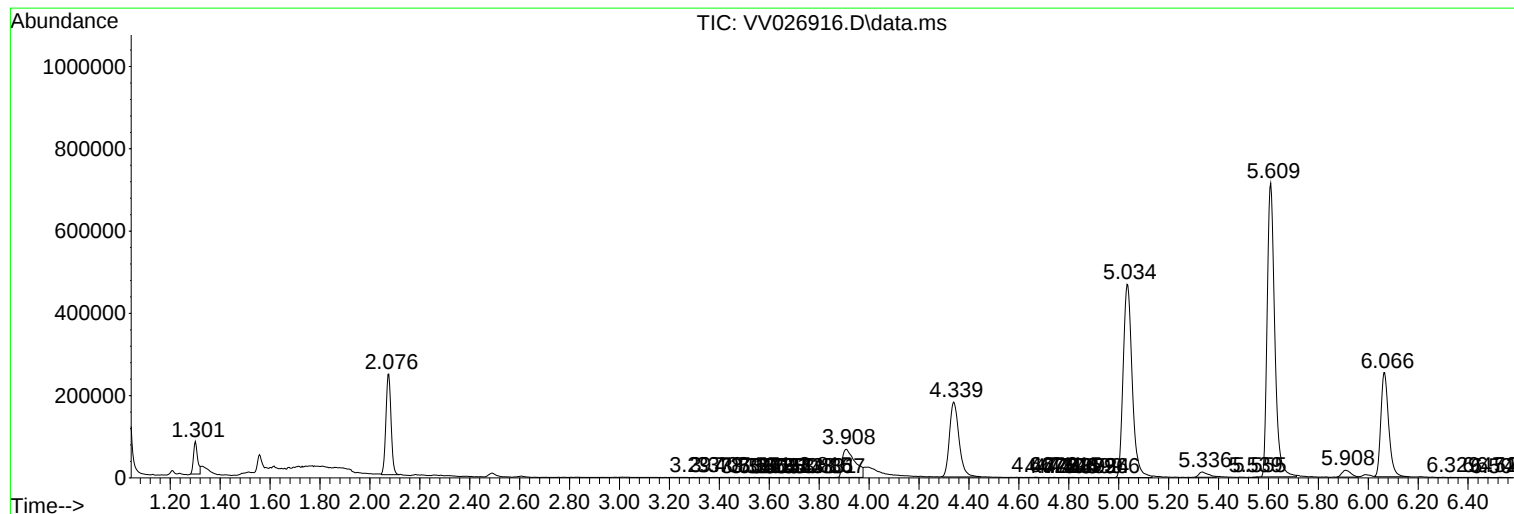

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026916.D
Acq On : 23 Jul 2022 12:45
Operator : SY/MD
Sample : N3743-01ME
Misc : 5.30g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5C87ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026916.D
Acq On : 23 Jul 2022 12:45
Operator : SY/MD
Sample : N3743-01ME
Misc : 5.30g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5C87ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc