

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026919.D
 Acq On : 23 Jul 2022 13:58
 Operator : SY/MD
 Sample : N3741-01ME
 Misc : 5.50g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B12ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M

Title : VOC Analysis

Signal : TIC: VV026919.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	74	80	108	rVB	150739	216980	11.83%	1.588%
2	2.082	314	324	341	rBV	399812	568677	31.00%	4.163%
3	2.433	423	433	444	rBV2	19450	37131	2.02%	0.272%
4	2.838	557	559	560	rBV2	293	117	0.01%	0.001%
5	2.995	605	608	612	rVB2	492	326	0.02%	0.002%
6	3.015	612	614	616	rBV	371	181	0.01%	0.001%
7	3.121	643	647	650	rBV2	326	251	0.01%	0.002%
8	3.156	656	658	662	rBV3	195	125	0.01%	0.001%
9	3.307	701	705	707	rBV2	506	335	0.02%	0.002%
10	3.346	713	717	720	rBV2	400	362	0.02%	0.003%
11	3.388	727	730	735	rVB3	208	178	0.01%	0.001%
12	3.417	735	739	742	rVB2	227	134	0.01%	0.001%
13	3.442	743	747	751	rBV3	384	387	0.02%	0.003%
14	3.494	761	763	768	rVB3	445	240	0.01%	0.002%
15	3.564	782	785	786	rBV	314	198	0.01%	0.001%
16	3.597	793	795	801	rVB3	402	259	0.01%	0.002%
17	3.626	801	804	806	rBV2	184	116	0.01%	0.001%
18	3.748	838	842	845	rBV2	439	344	0.02%	0.003%
19	3.767	845	848	849	rBV	288	169	0.01%	0.001%
20	3.780	849	852	855	rVV2	371	226	0.01%	0.002%
21	3.841	869	871	876	rVB2	368	227	0.01%	0.002%
22	3.892	876	887	929	rBV	108536	408988	22.30%	2.994%
23	4.336	1010	1025	1056	rBV	295182	741097	40.40%	5.425%
24	4.638	1115	1119	1124	rVB3	607	636	0.03%	0.005%
25	4.658	1124	1125	1130	rBV2	310	243	0.01%	0.002%
26	4.751	1150	1154	1157	rBV2	296	259	0.01%	0.002%
27	4.809	1169	1172	1175	rVB2	421	302	0.02%	0.002%
28	4.825	1175	1177	1178	rBV2	142	45	0.00%	0.000%
29	4.886	1194	1196	1198	rBV	200	85	0.00%	0.001%
30	4.970	1218	1222	1224	rBV2	250	222	0.01%	0.002%
31	5.034	1226	1242	1275	rBV2	737181	1834431	100.00%	13.429%
32	5.513	1389	1391	1394	rVB2	323	122	0.01%	0.001%
33	5.561	1400	1406	1408	rBV4	533	480	0.03%	0.004%
34	5.609	1409	1421	1462	rVV	586081	1207460	65.82%	8.839%
35	5.905	1502	1513	1528	rBV2	11402	25302	1.38%	0.185%
36	6.063	1549	1562	1599	rBV	411622	855326	46.63%	6.262%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026919.D
 Acq On : 23 Jul 2022 13:58
 Operator : SY/MD
 Sample : N3741-01ME
 Misc : 5.50g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B12ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.301	1634	1636	1640	rVB	402	288	0.02%	0.002%
38	6.323	1640	1643	1646	rBV	499	292	0.02%	0.002%
39	6.355	1650	1653	1655	rBV2	485	217	0.01%	0.002%
40	6.371	1655	1658	1660	rVB3	497	207	0.01%	0.002%
41	6.384	1660	1662	1664	rBV2	369	192	0.01%	0.001%
42	6.449	1680	1682	1685	rVB3	405	159	0.01%	0.001%
43	6.490	1692	1695	1697	rBV2	203	129	0.01%	0.001%
44	6.503	1697	1699	1702	rBV	224	174	0.01%	0.001%
45	6.551	1712	1714	1715	rBV	196	86	0.00%	0.001%
46	6.587	1723	1725	1726	rVB	146	36	0.00%	0.000%
47	6.600	1726	1729	1732	rBV	265	175	0.01%	0.001%
48	6.642	1734	1742	1747	rBV5	2107	3143	0.17%	0.023%
49	6.796	1787	1790	1791	rBV2	199	121	0.01%	0.001%
50	6.825	1797	1799	1804	rVB3	357	220	0.01%	0.002%
51	6.879	1812	1816	1819	rBV	315	231	0.01%	0.002%
52	6.908	1823	1825	1828	rBV	111	58	0.00%	0.000%
53	6.928	1828	1831	1832	rBV	208	122	0.01%	0.001%
54	6.982	1836	1848	1876	rBV	178007	350126	19.09%	2.563%
55	7.265	1932	1936	1939	rBV5	456	379	0.02%	0.003%
56	7.310	1939	1950	1972	rBV	734227	1300886	70.91%	9.523%
57	7.619	2037	2046	2072	rBV	122543	234141	12.76%	1.714%
58	7.876	2123	2126	2128	rBV3	505	360	0.02%	0.003%
59	7.947	2143	2148	2153	rBV4	537	703	0.04%	0.005%
60	7.979	2153	2158	2165	rVV3	1654	1950	0.11%	0.014%
61	8.018	2168	2170	2173	rBV	194	93	0.01%	0.001%
62	8.053	2180	2181	2182	rVB	124	24	0.00%	0.000%
63	8.095	2182	2194	2231	rBV	299904	878446	47.89%	6.431%
64	8.706	2382	2384	2388	rBV2	351	210	0.01%	0.002%
65	8.722	2388	2389	2392	rVB	357	140	0.01%	0.001%
66	8.741	2393	2395	2396	rBV2	206	85	0.00%	0.001%
67	8.850	2417	2429	2462	rBV	900398	1494435	81.47%	10.940%
68	9.246	2548	2552	2554	rBV	371	248	0.01%	0.002%
69	9.407	2600	2602	2604	rBV2	220	117	0.01%	0.001%
70	9.423	2605	2607	2609	rVB2	306	132	0.01%	0.001%
71	9.564	2649	2651	2653	rVB2	301	130	0.01%	0.001%
72	9.577	2653	2655	2658	rVB2	224	115	0.01%	0.001%
73	9.593	2658	2660	2662	rBV2	327	188	0.01%	0.001%
74	9.674	2681	2685	2686	rBV	322	228	0.01%	0.002%
75	9.821	2728	2731	2733	rBV2	497	337	0.02%	0.002%
76	9.957	2771	2773	2779	rVB3	481	308	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026919.D
 Acq On : 23 Jul 2022 13:58
 Operator : SY/MD
 Sample : N3741-01ME
 Misc : 5.50g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B12ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M

Title : VOC Analysis

77	10.053	2799	2803	2804	rBV	425	228	0.01%	0.002%
78	10.217	2841	2854	2878	rBV	577271	968264	52.78%	7.088%
79	10.580	2962	2967	2971	rBV	1092	953	0.05%	0.007%
80	10.670	2993	2995	2998	rBV2	396	293	0.02%	0.002%
81	10.751	3018	3020	3023	rBV2	372	251	0.01%	0.002%
82	10.780	3026	3029	3031	rVB	377	168	0.01%	0.001%
83	10.863	3051	3055	3058	rBV3	416	328	0.02%	0.002%
84	11.249	3163	3175	3195	rBV	842517	1301104	70.93%	9.525%
85	11.551	3267	3269	3275	rVB3	633	487	0.03%	0.004%
86	11.625	3280	3292	3315	rBV	732872	1159087	63.19%	8.485%
87	12.381	3519	3527	3536	rBV4	4478	7502	0.41%	0.055%
88	14.413	4151	4159	4170	rVB2	35970	49594	2.70%	0.363%




Sum of corrected areas: 13659851

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026919.D
Acq On : 23 Jul 2022 13:58
Operator : SY/MD
Sample : N3741-01ME
Misc : 5.50g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B12ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

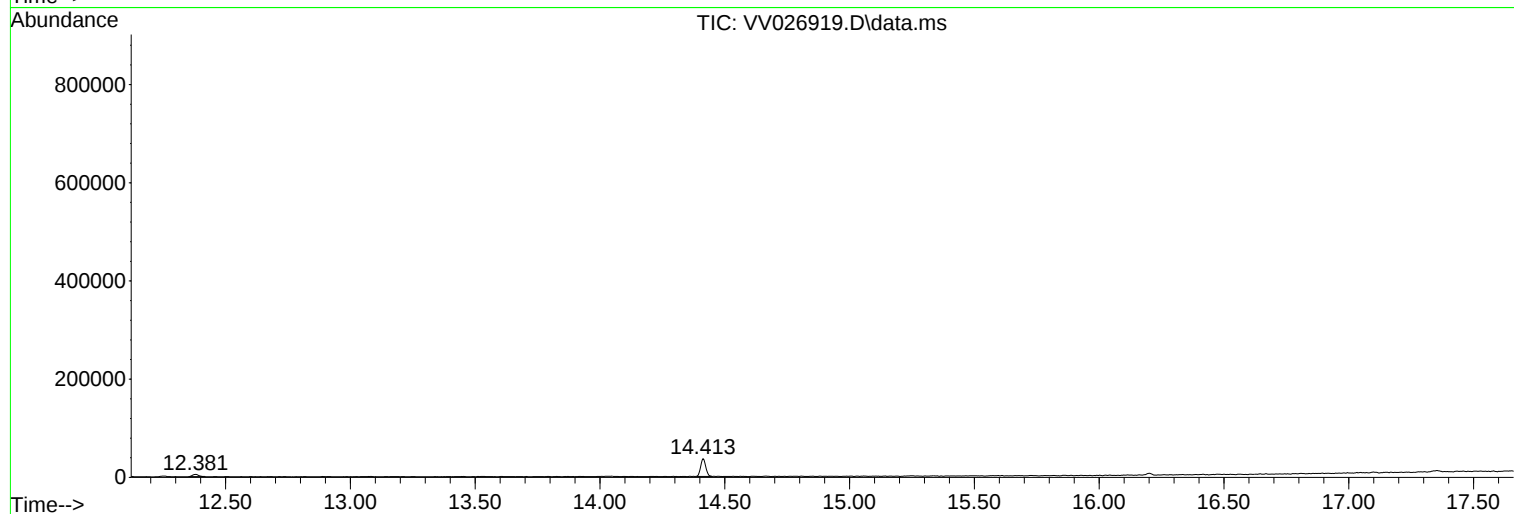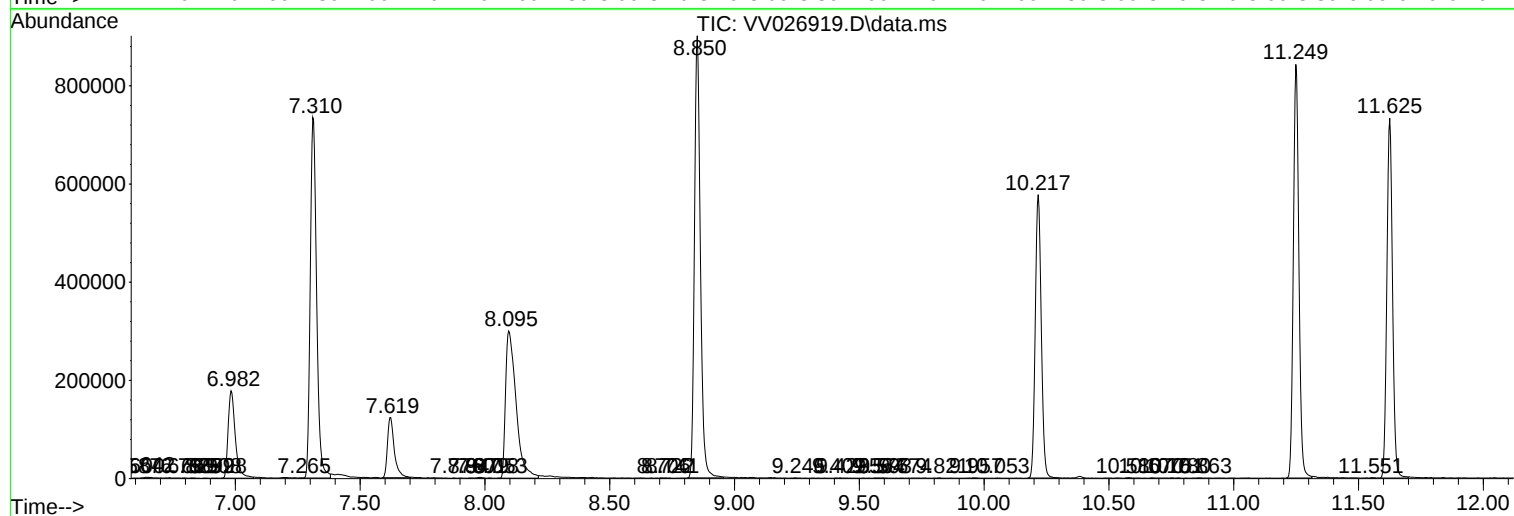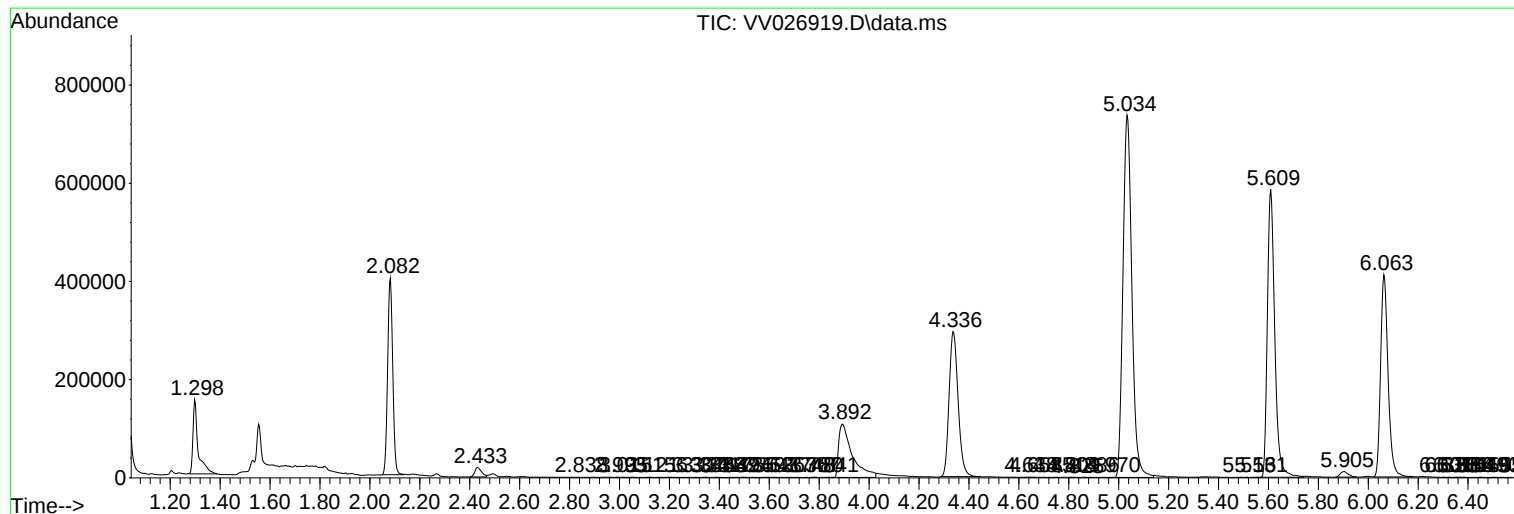

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026919.D
Acq On : 23 Jul 2022 13:58
Operator : SY/MD
Sample : N3741-01ME
Misc : 5.50g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B12ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026919.D
Acq On : 23 Jul 2022 13:58
Operator : SY/MD
Sample : N3741-01ME
Misc : 5.50g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B12ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc