


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026911.D
Acq On : 23 Jul 2022 09:07
Operator : SY/MD
Sample : BFB297
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB297

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Title : VOC Analysis
Last Update : Mon Jul 25 02:02:46 2022

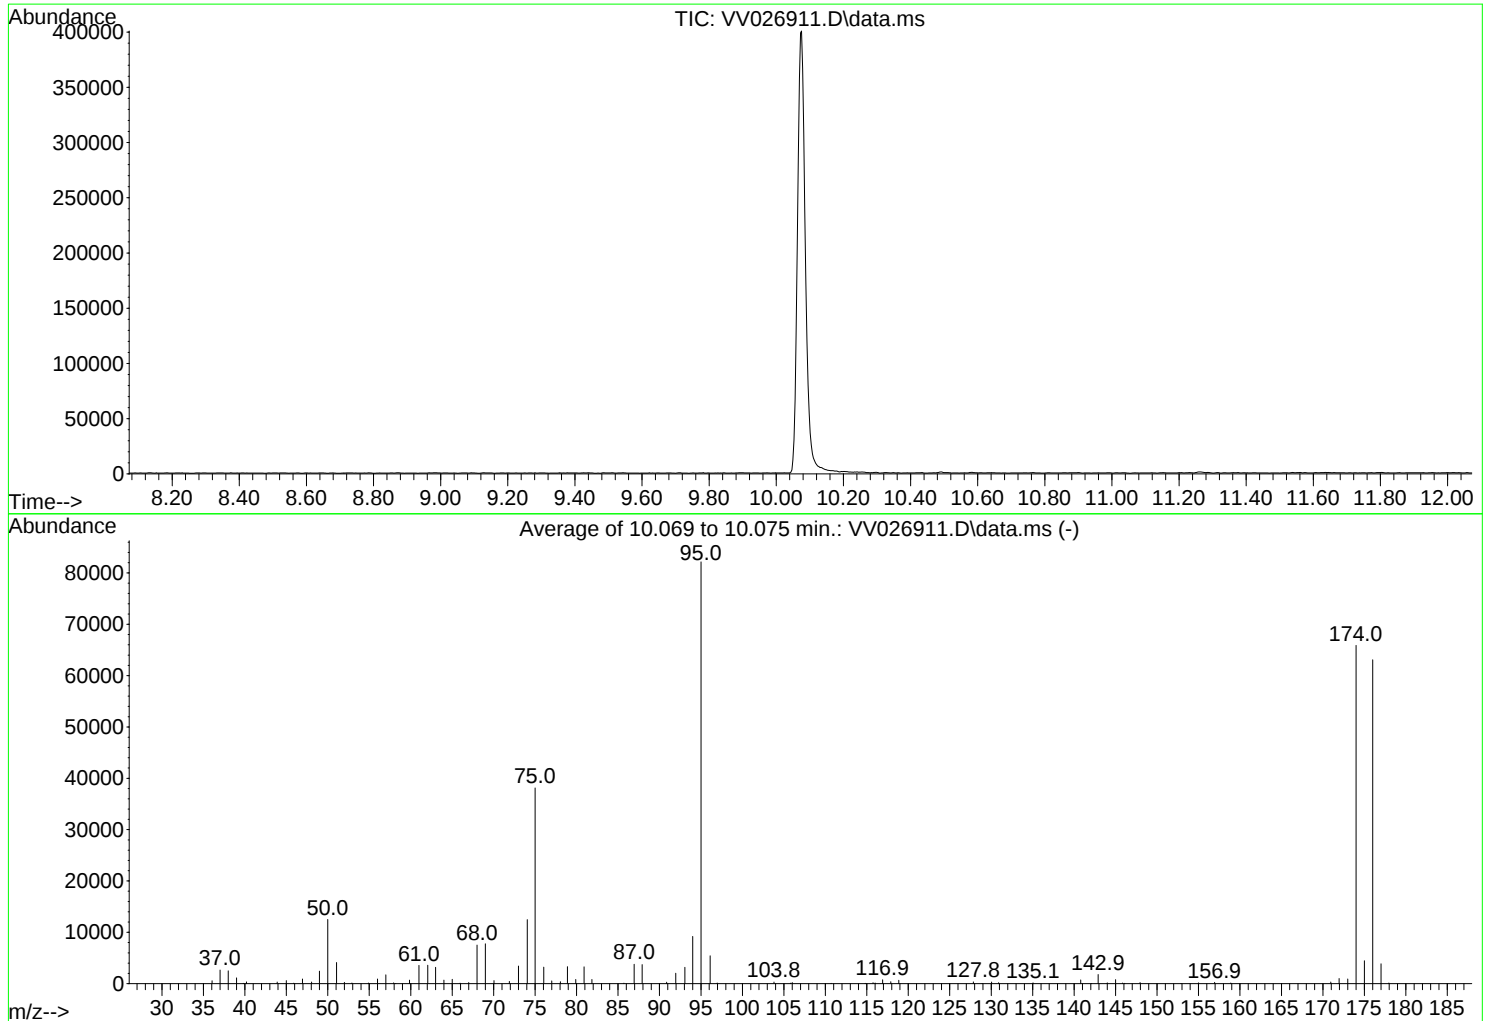

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	12497	PASS
75	95	30	80	46.4	38115	PASS
95	95	100	100	100.0	82160	PASS
96	95	5	9	6.6	5432	PASS
173	174	0.00	2	1.4	908	PASS
174	95	50	120	80.2	65883	PASS
175	174	5	9	6.8	4468	PASS
176	174	95	105	95.8	63096	PASS
177	176	5	10	6.1	3867	PASS

m/z	Abundance
39.90	314.0
43.90	546.0

Instrument :
MSVOA_V
ClientSampleId :
BFB297

m/z	Abundance
36.00	525.0
37.00	2555.0
38.00	2492.0
39.00	1098.0
39.80	345.0
40.20	276.0
44.00	879.0
45.00	645.0
45.90	102.0
47.00	860.0
48.00	357.0
49.00	2270.0
50.00	11829.0
51.10	3875.0
52.00	211.0
52.90	117.0
54.90	134.0
56.00	851.0
57.00	1635.0
57.90	113.0
58.20	104.0
59.90	656.0
61.00	3139.0
62.00	3192.0
63.00	3009.0
64.00	650.0
65.00	719.0
65.90	129.0
67.00	190.0
68.00	6973.0
69.00	7343.0
70.10	548.0
71.90	434.0
73.00	3237.0
74.00	11758.0
75.00	35264.0
76.00	3139.0
77.10	512.0
78.00	315.0
78.90	3004.0
79.90	823.0
80.90	3078.0
81.80	724.0
86.90	3533.0
87.90	3386.0
91.00	244.0
91.90	1942.0
93.10	2965.0
94.00	8710.0
95.00	76968.0
96.10	5143.0
97.00	142.0
103.80	293.0
105.80	318.0
110.70	110.0
115.70	234.0
116.90	654.0
117.90	334.0
118.90	594.0
127.90	348.0
130.10	360.0
130.90	149.0
135.00	173.0
140.80	610.0
142.10	111.0
142.90	1638.0
144.00	200.0
145.00	746.0
145.80	169.0
147.90	206.0
155.00	129.0
156.90	240.0
158.90	135.0
171.00	271.0
172.00	791.0
173.00	909.0
174.00	60136.0
175.00	4171.0
176.00	57208.0
177.00	3591.0
178.00	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB297

m/z	Abundance
36.10	595.0
37.00	2726.0
38.00	2514.0
39.00	1172.0
39.80	369.0
40.20	344.0
44.00	861.0
45.00	619.0
45.90	111.0
46.90	942.0
48.00	323.0
49.00	2535.0
50.00	12966.0
51.00	4246.0
52.00	266.0
52.90	105.0
54.90	126.0
56.00	942.0
57.00	1744.0
57.90	151.0
59.90	716.0
61.00	3714.0
62.00	3669.0
63.00	3275.0
64.00	706.0
65.00	833.0
66.00	113.0
67.00	223.0
68.00	7804.0
69.00	8014.0
70.10	642.0
71.90	465.0
73.00	3601.0
74.00	13034.0
75.00	39216.0
76.10	3274.0
77.00	515.0
78.00	360.0
78.90	3427.0
79.90	826.0
80.90	3361.0
81.90	828.0
85.70	111.0
87.00	3926.0
87.90	3830.0
90.80	298.0
91.90	2103.0
93.00	3228.0
94.00	9560.0
95.00	84952.0
96.10	5585.0
97.00	122.0
103.80	355.0
106.00	327.0
110.70	113.0
114.80	106.0
115.80	298.0
116.90	817.0
117.90	391.0
118.80	675.0
127.90	383.0
130.10	345.0
130.90	190.0
135.10	157.0
140.80	766.0
142.90	1899.0
144.00	171.0
145.00	833.0
145.90	175.0
148.00	220.0
152.90	105.0
155.00	157.0
157.00	270.0
158.90	144.0
170.90	312.0
172.00	1015.0
173.00	917.0
174.00	68040.0
175.00	4576.0
176.00	65448.0
177.00	3962.0
177.90	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB297

m/z	Abundance
36.10	579.0
37.00	2662.0
38.00	2490.0
39.00	1124.0
39.80	427.0
40.20	410.0
43.90	842.0
45.00	534.0
45.90	104.0
46.90	881.0
48.10	299.0
49.00	2537.0
50.00	12696.0
51.00	4192.0
52.00	257.0
52.90	113.0
54.90	163.0
56.00	906.0
57.00	1780.0
58.00	168.0
59.80	679.0
61.00	3811.0
62.10	3884.0
63.00	3269.0
64.00	724.0
65.00	936.0
67.00	207.0
68.00	7773.0
69.00	7890.0
70.00	637.0
71.90	440.0
73.00	3494.0
74.10	12585.0
75.00	39864.0
76.10	3189.0
76.90	530.0
78.10	420.0
78.90	3463.0
79.90	782.0
80.90	3412.0
81.90	854.0
85.70	139.0
87.00	3835.0
87.90	3873.0
90.80	317.0
92.00	2075.0
93.00	3346.0
94.00	9300.0
95.00	84560.0
96.10	5569.0
96.90	125.0
103.80	344.0
106.00	332.0
114.80	116.0
116.00	342.0
116.90	763.0
117.90	381.0
118.80	714.0
127.80	301.0
128.90	124.0
130.00	265.0
130.90	219.0
135.00	144.0
140.80	807.0
142.90	1848.0
144.00	137.0
145.00	798.0
146.10	170.0
148.00	224.0
155.00	174.0
157.00	239.0
158.90	103.0
170.90	325.0
171.90	1156.0
173.00	898.0
174.00	69472.0
175.00	4656.0
176.00	66632.0
177.00	4047.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB297