

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072419\
 Data File : VV012006.D
 Acq On : 24 Jul 2019 13:06
 Operator : SY/MD
 Sample : K3890-06
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A52J2

Quant Time: Jul 25 05:00:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 25 04:12:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	132588	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	127551	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	62844	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	31451	4.56	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.20%
7) Chloroethane-d5	1.59	69	26199	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.60%
11) 1,1-Dichloroethene-d2	2.13	63	53220	3.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.60%
20) 2-Butanone-d5	3.94	46	98458	48.88	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.76%
24) Chloroform-d	4.40	84	88562	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
26) 1,2-Dichloroethane-d4	5.08	65	50216	5.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.80%
32) Benzene-d6	5.10	84	175145	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.12	67	51694	5.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.60%
41) Toluene-d8	7.36	98	159641	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
43) trans-1,3-Dichloropropene-	7.66	79	19961	4.83	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.60%
46) 2-Hexanone-d5	8.13	63	80691	48.64	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.28%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35932	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	65735	5.43	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.60%


Target Compounds					Ovalue
13) Acetone	2.20	43	4028	3.710 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072419\
Data File : VV012006.D
Acq On : 24 Jul 2019 13:06
Operator : SY/MD
Sample : K3890-06
Misc : 25ML/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A52J2

Quant Time: Jul 25 05:00:04 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 25 04:12:02 2019
Response via : Initial Calibration

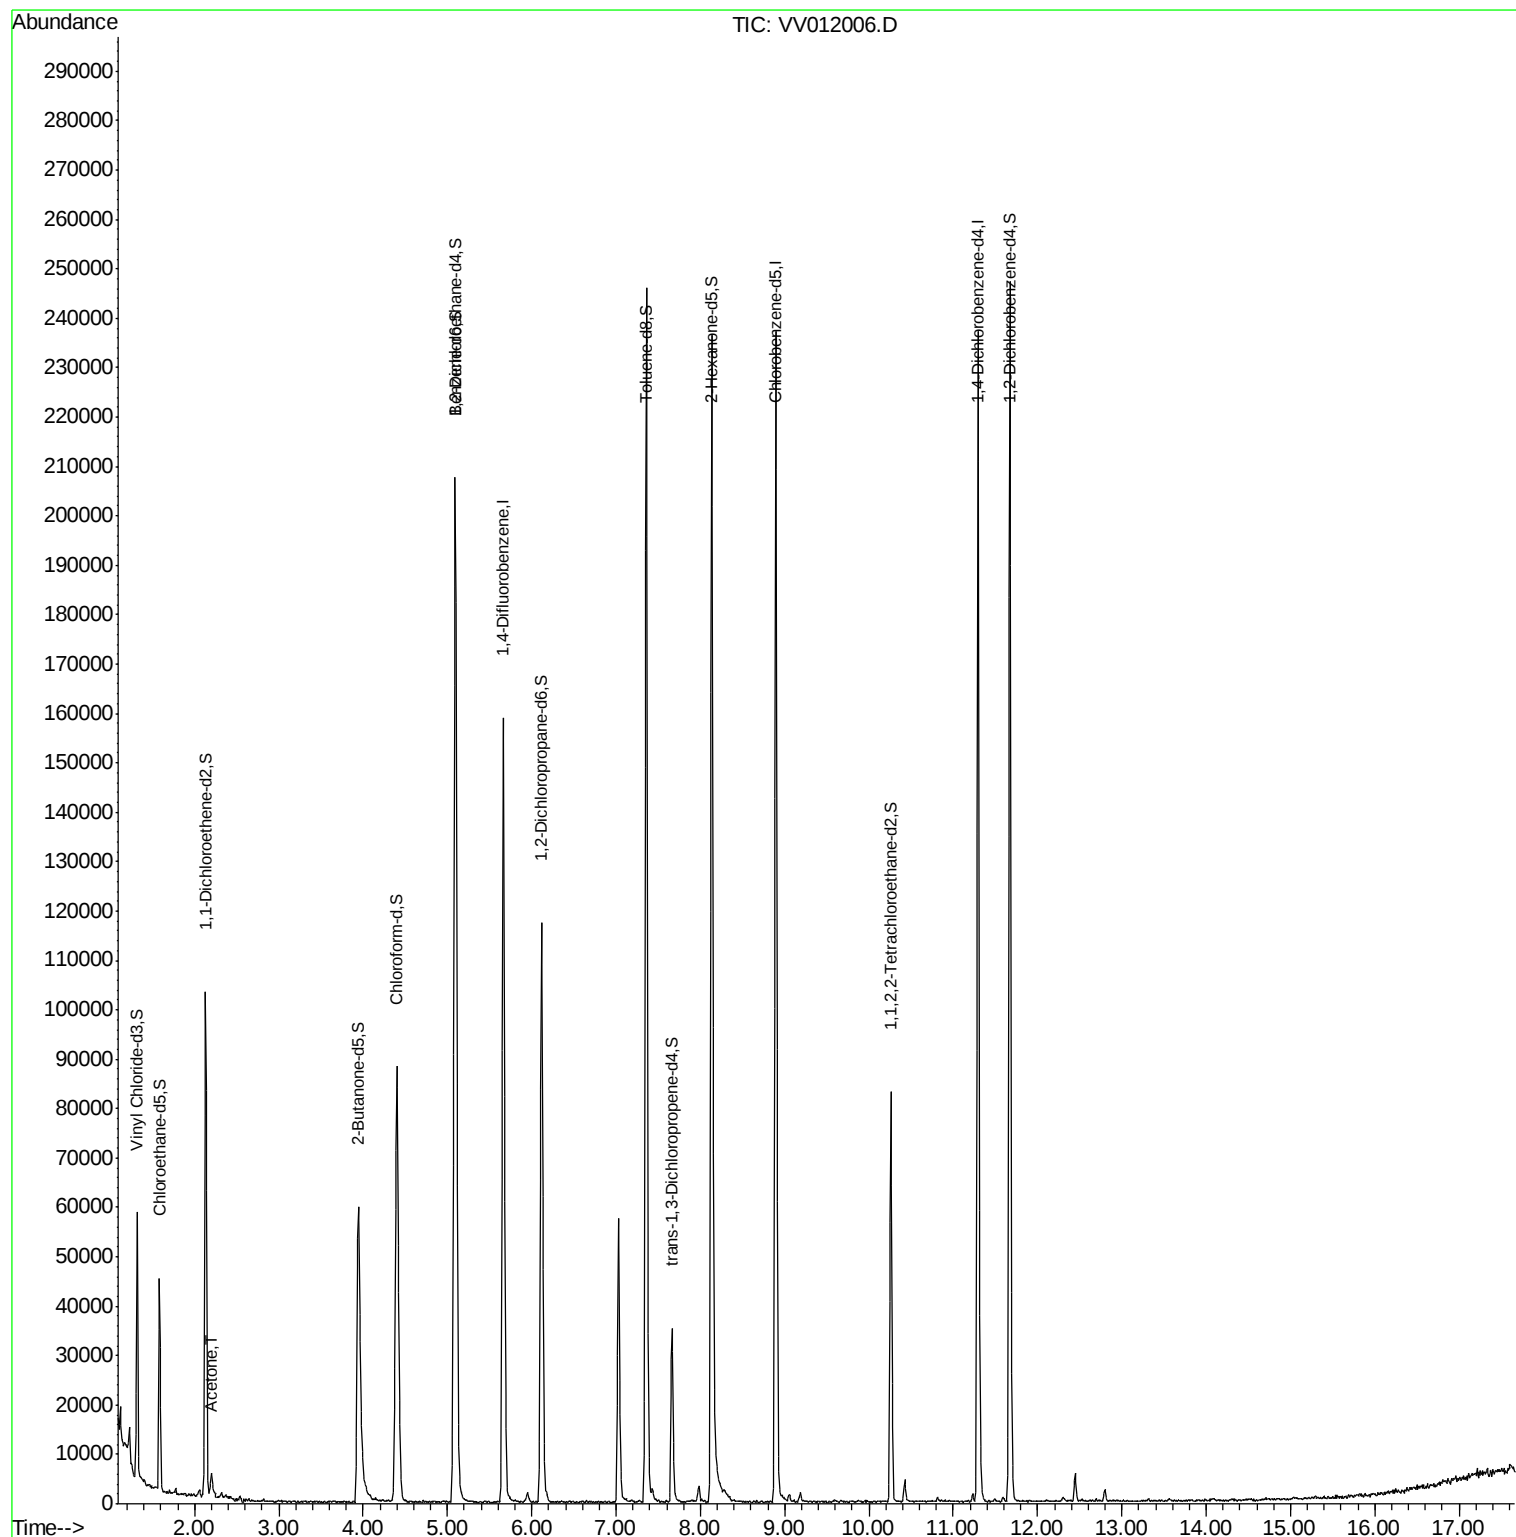

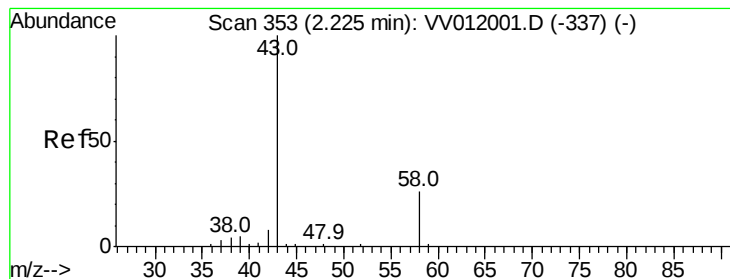

#13

Acetone

Concen: 3.710 ug/L

RT: 2.20 min Scan# 345

Delta R.T. -0.03 min

Lab File: VV012006.D

Acq: 24 Jul 2019 13:06

Instrument :
MSVOA_V
ClientSampleId :
A52J2

Tot Ion: 43 Resp: 4028

Ion Ratio Lower Upper

43 100

58 23.6 0.0 51.8

