

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072419\
 Data File : VV012011.D
 Acq On : 24 Jul 2019 15:11
 Operator : SY/MD
 Sample : K3958-12
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2A01

Quant Time: Jul 25 05:45:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 25 04:12:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	136790	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	128201	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	63649	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	30191	4.25	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.00%
7) Chloroethane-d5	1.59	69	25274	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.14	63	50803	3.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.80%
20) 2-Butanone-d5	3.95	46	99543	47.90	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.80%
24) Chloroform-d	4.40	84	87749	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
26) 1,2-Dichloroethane-d4	5.09	65	49420	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.80%
32) Benzene-d6	5.10	84	171033	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
36) 1,2-Dichloropropane-d6	6.12	67	50203	4.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.20%
41) Toluene-d8	7.36	98	155720	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
43) trans-1,3-Dichloropropene-	7.67	79	18750	4.52	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.40%
46) 2-Hexanone-d5	8.14	63	80882	48.50	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.00%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	34935	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	64587	5.27	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	11829	10.560 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072419\
Data File : VV012011.D
Acq On : 24 Jul 2019 15:11
Operator : SY/MD
Sample : K3958-12
Misc : 25ML/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2A01

Quant Time: Jul 25 05:45:28 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 25 04:12:02 2019
Response via : Initial Calibration

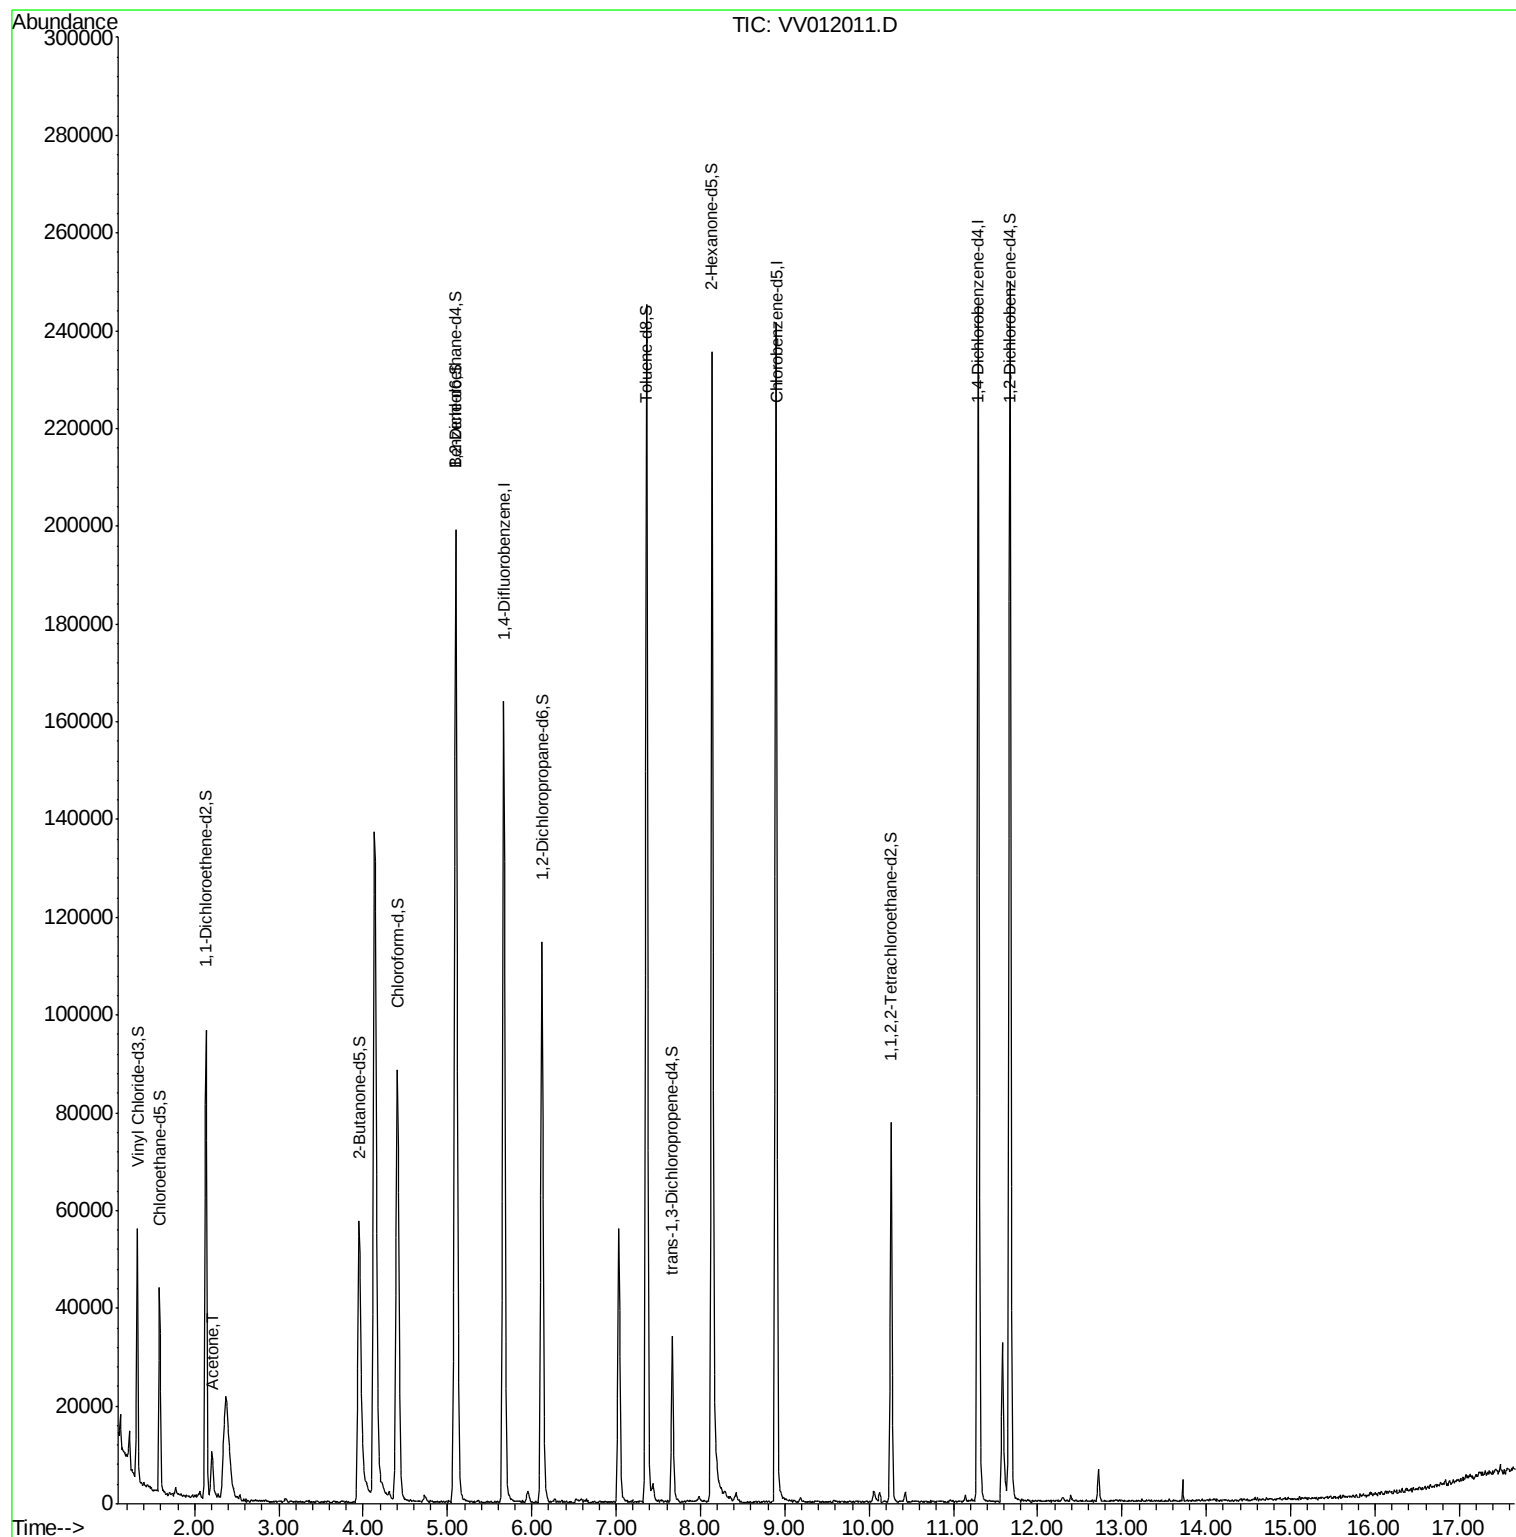

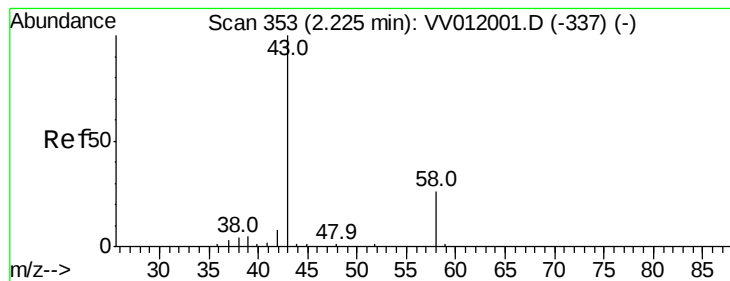

#13

Acetone

Concen: 10.560 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.02 min

Lab File: VV012011.D

Acq: 24 Jul 2019 15:11

Instrument :
MSVOA_V
ClientSampleId :
F2A01

Tot Ion: 43 Resp: 11829

Ion Ratio Lower Upper

43 100

58 25.5 0.0 51.8

