


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072419\
Data File : VV012000.D
Acq On : 24 Jul 2019 09:42
Operator : SY/MD
Sample : BFB37
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB37

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jul 25 04:12:02 2019

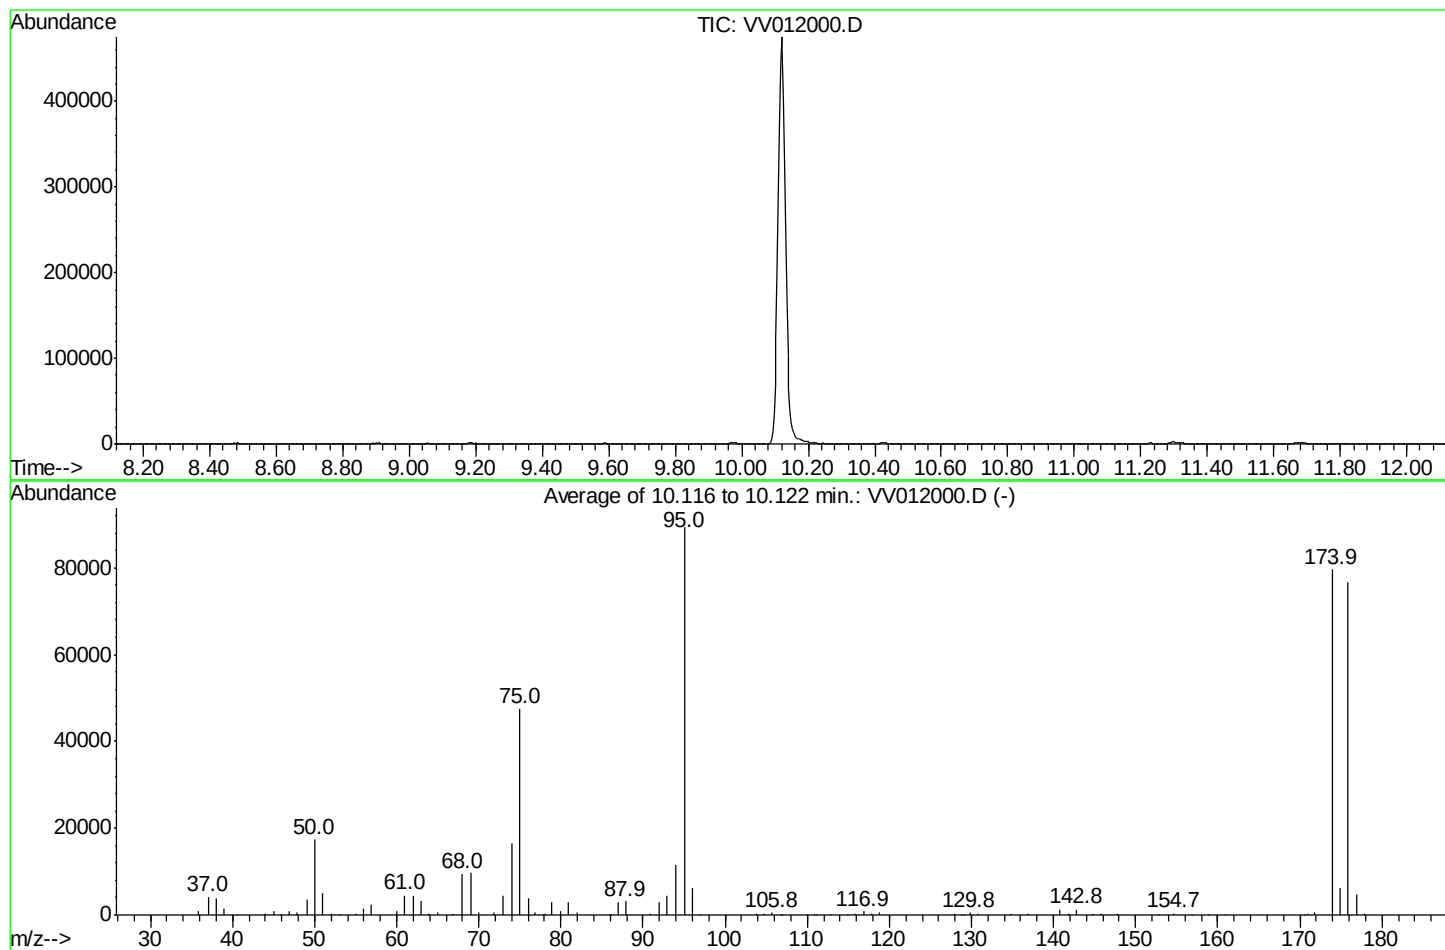

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	17306	PASS
75	95	30	80	53.3	47616	PASS
95	95	100	100	100.0	89330	PASS
96	95	5	9	7.0	6219	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.0	79533	PASS
175	174	5	9	7.9	6298	PASS
176	174	95	101	96.6	76840	PASS
177	176	5	9	6.1	4698	PASS

Scan 2794 (10.074 min): VV012000.D
BFB37

m/z	Abundance
39.90	186.0
44.00	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
35.90	735.0
37.00	4106.0
38.00	3942.0
38.90	1548.0
39.90	284.0
43.90	613.0
45.00	780.0
45.90	120.0
46.80	811.0
47.90	737.0
49.00	3696.0
50.00	16712.0
51.00	5057.0
52.00	325.0
53.00	124.0
54.90	256.0
56.00	1506.0
57.00	2394.0
60.00	889.0
61.00	4279.0
62.00	4385.0
62.90	3140.0
63.90	414.0
65.00	532.0
66.90	297.0
68.00	9580.0
69.00	9556.0
69.90	639.0
71.80	524.0
73.00	4438.0
74.00	16145.0
75.00	46048.0
76.00	4028.0
76.90	556.0
77.70	256.0
78.10	273.0
78.80	2785.0
80.00	853.0
80.90	2919.0
81.90	644.0
85.80	148.0
86.90	2982.0
87.90	2945.0
90.80	403.0
91.90	2820.0
92.90	4406.0
94.00	11151.0
95.00	85568.0
96.00	6044.0
97.00	119.0
103.80	439.0
104.70	206.0
105.80	448.0
107.00	143.0
112.90	150.0
114.90	143.0
115.80	387.0
116.90	734.0
117.80	426.0
118.80	600.0
127.80	319.0
128.70	104.0
129.80	415.0
130.80	226.0
134.90	192.0
136.80	174.0
140.80	1077.0
141.80	232.0
142.80	1194.0
144.90	240.0
145.70	199.0
147.70	207.0
154.70	360.0
156.80	178.0
160.90	150.0
170.40	121.0
171.00	198.0
171.90	686.0
173.90	75296.0
174.90	5914.0
175.90	72656.0
176.90	4507.0
177.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
35.90	791.0
37.00	4401.0
38.00	4139.0
38.90	1601.0
39.90	283.0
40.50	102.0
43.90	634.0
44.90	810.0
45.80	118.0
46.80	793.0
47.90	777.0
49.00	3618.0
50.00	17928.0
51.00	5191.0
52.00	309.0
52.90	120.0
54.90	231.0
55.90	1572.0
57.00	2516.0
59.90	963.0
60.90	4621.0
62.00	4542.0
62.90	3305.0
63.90	472.0
65.00	554.0
66.90	306.0
68.00	9866.0
69.00	10013.0
70.00	721.0
71.90	570.0
73.00	4724.0
74.00	16984.0
75.00	49312.0
76.00	4009.0
76.90	552.0
78.00	294.0
78.90	3011.0
80.00	905.0
80.90	3194.0
81.90	710.0
86.10	178.0
86.90	3130.0
87.90	3204.0
90.80	432.0
91.90	2945.0
92.90	4566.0
94.00	12026.0
95.00	92392.0
96.00	6451.0
97.00	140.0
103.80	457.0
104.70	186.0
105.80	481.0
106.90	120.0
109.90	108.0
111.10	108.0
112.90	157.0
114.90	131.0
115.80	421.0
116.90	796.0
117.80	470.0
118.80	688.0
128.00	354.0
129.00	123.0
129.80	465.0
130.80	191.0
134.80	223.0
136.80	196.0
140.80	1181.0
141.80	261.0
142.90	1201.0
144.90	259.0
145.70	172.0
147.70	273.0
154.70	362.0
156.90	154.0
158.90	106.0
160.90	135.0
170.50	125.0
171.10	215.0
171.80	672.0
173.90	82272.0
174.90	6500.0
175.90	79584.0
176.90	4805.0
177.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
35.90	744.0
37.00	4308.0
38.00	3889.0
38.90	1539.0
39.90	271.0
40.50	117.0
43.90	655.0
44.90	784.0
46.90	754.0
47.90	725.0
49.00	3335.0
50.00	17280.0
51.00	4869.0
52.00	249.0
52.90	107.0
55.00	192.0
55.90	1477.0
56.90	2387.0
59.90	903.0
60.90	4450.0
62.00	4359.0
62.90	3324.0
63.90	426.0
65.10	497.0
66.90	318.0
67.90	9283.0
69.00	9649.0
70.00	797.0
71.90	561.0
72.90	4523.0
74.00	16163.0
75.00	47488.0
76.00	3832.0
76.80	529.0
78.00	287.0
78.90	2908.0
80.00	844.0
80.90	3035.0
81.90	710.0
86.10	191.0
86.90	3046.0
87.90	3284.0
90.80	383.0
91.90	2843.0
92.90	4238.0
94.00	11685.0
95.00	90032.0
96.00	6164.0
97.00	178.0
103.80	408.0
104.70	165.0
105.70	478.0
106.70	105.0
109.90	105.0
110.80	107.0
112.90	157.0
114.90	104.0
115.80	412.0
116.90	788.0
117.80	410.0
118.80	643.0
128.00	395.0
129.00	172.0
129.80	478.0
130.80	152.0
134.80	206.0
136.80	199.0
140.80	1174.0
141.90	215.0
142.90	1162.0
144.80	212.0
145.70	129.0
147.70	316.0
152.80	105.0
154.70	315.0
156.90	106.0
158.90	129.0
160.90	122.0
170.60	133.0
171.10	189.0
171.80	591.0
173.90	81032.0
174.90	6480.0
175.90	78280.0
176.90	4782.0
177.80	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37