


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072420\
Data File : VV017645.D
Acq On : 24 Jul 2020 13:39
Operator : SY/MD
Sample : L3395-12
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAY20

Manual Integrations
APPROVED

MMDadoda
7/29/2020 11:24:57 AM

Quant Time: Jul 25 00:43:09 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 25 00:05:26 2020
Response via : Initial Calibration

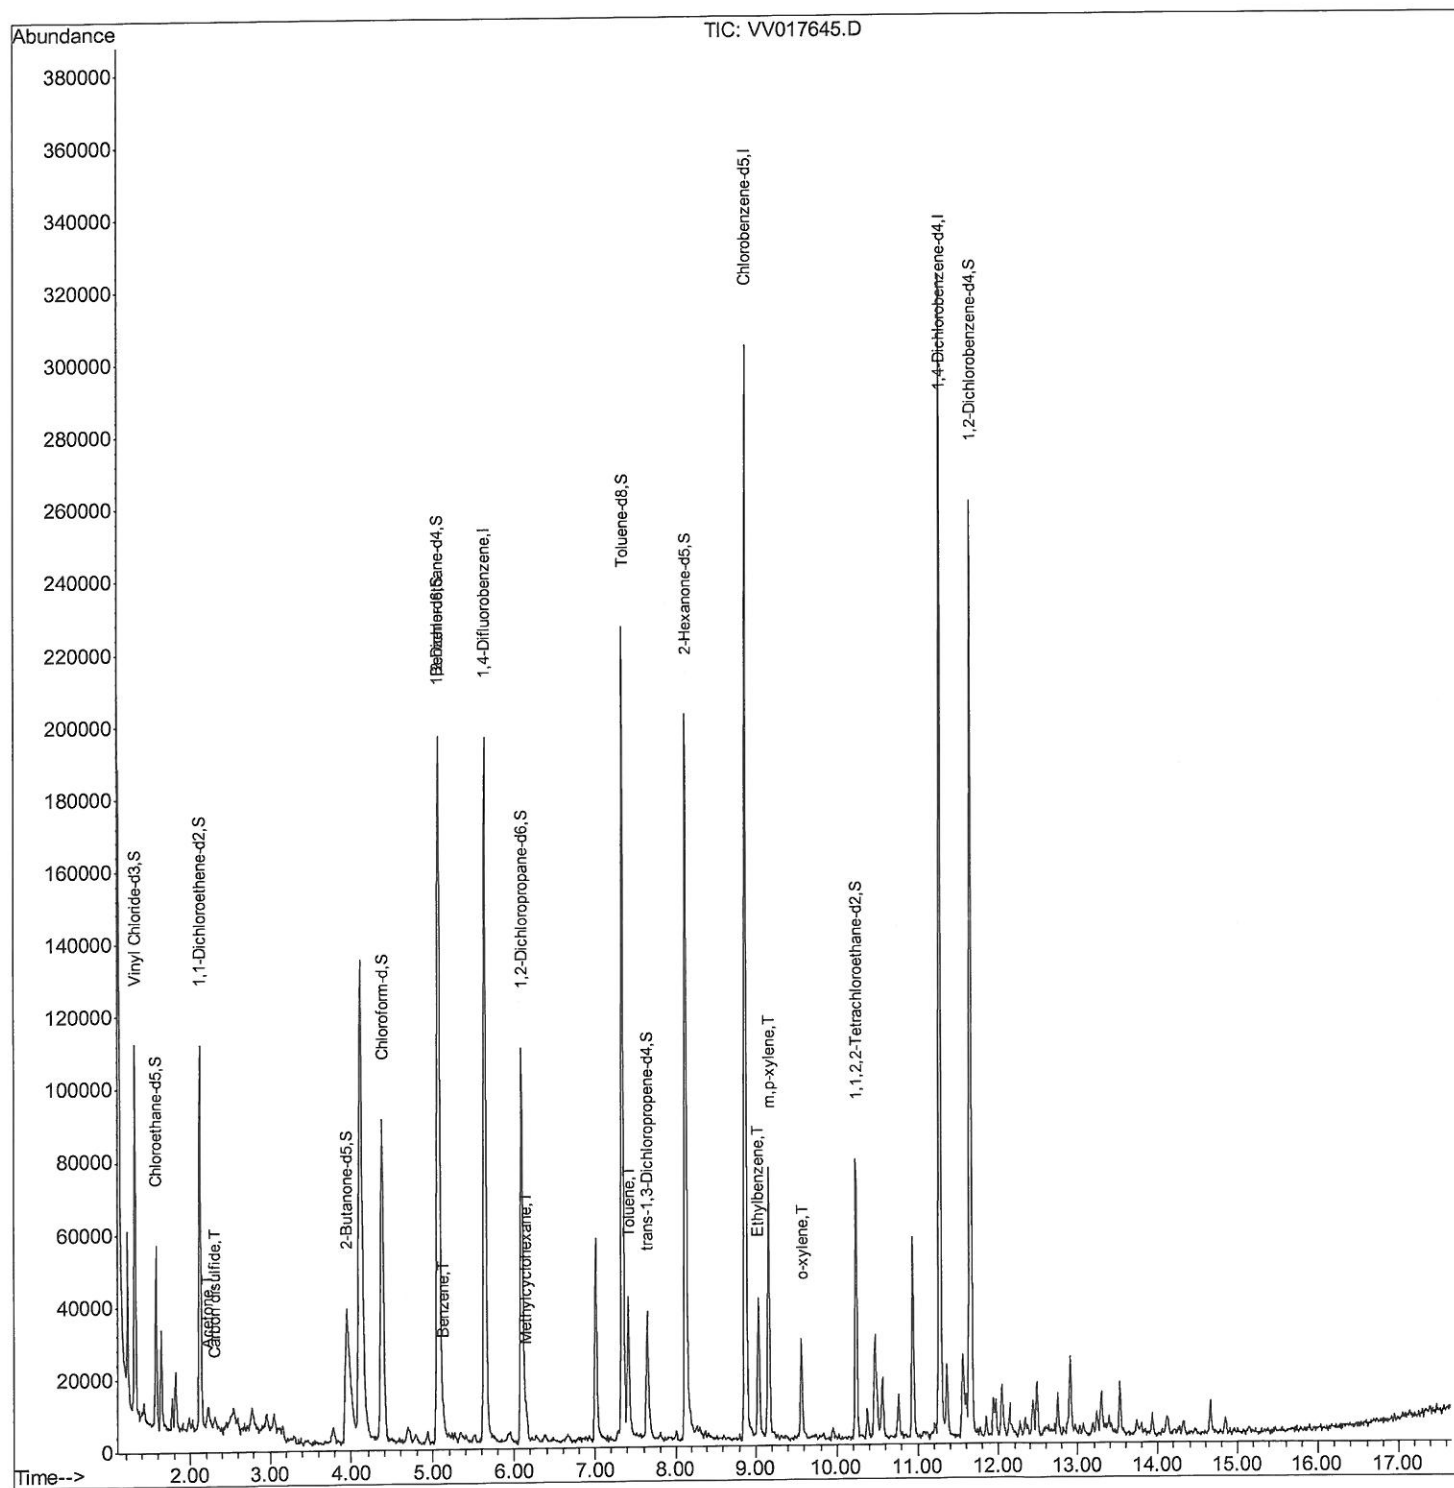

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072420\
 Data File : VV017645.D
 Acq On : 24 Jul 2020 13:39
 Operator : SY/MD
 Sample : L3395-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAY20

Manual Integrations
 APPROVED

MMDadoda
 7/29/2020 11:24:57 AM

Quant Time: Jul 25 00:08:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 25 00:05:26 2020
 Response via : Initial Calibration

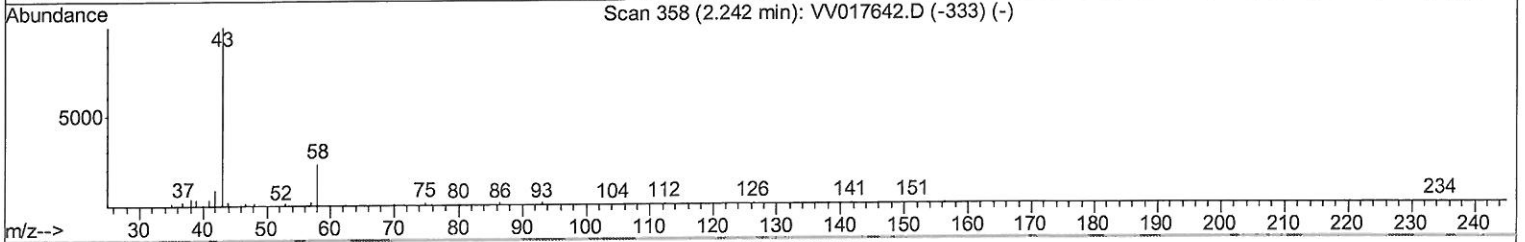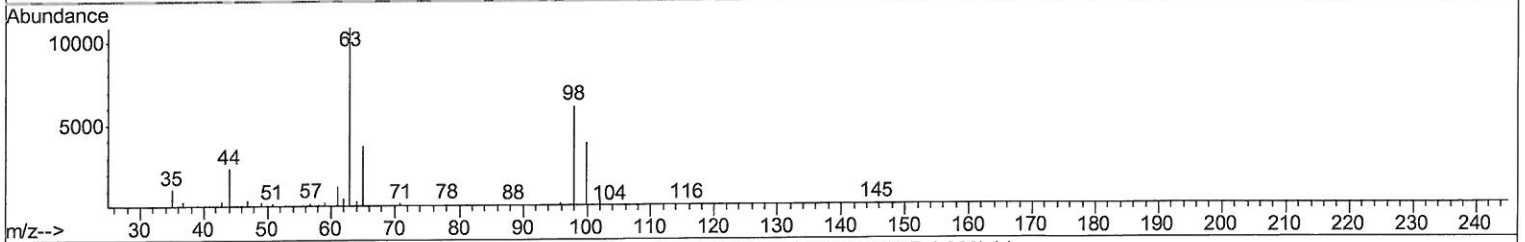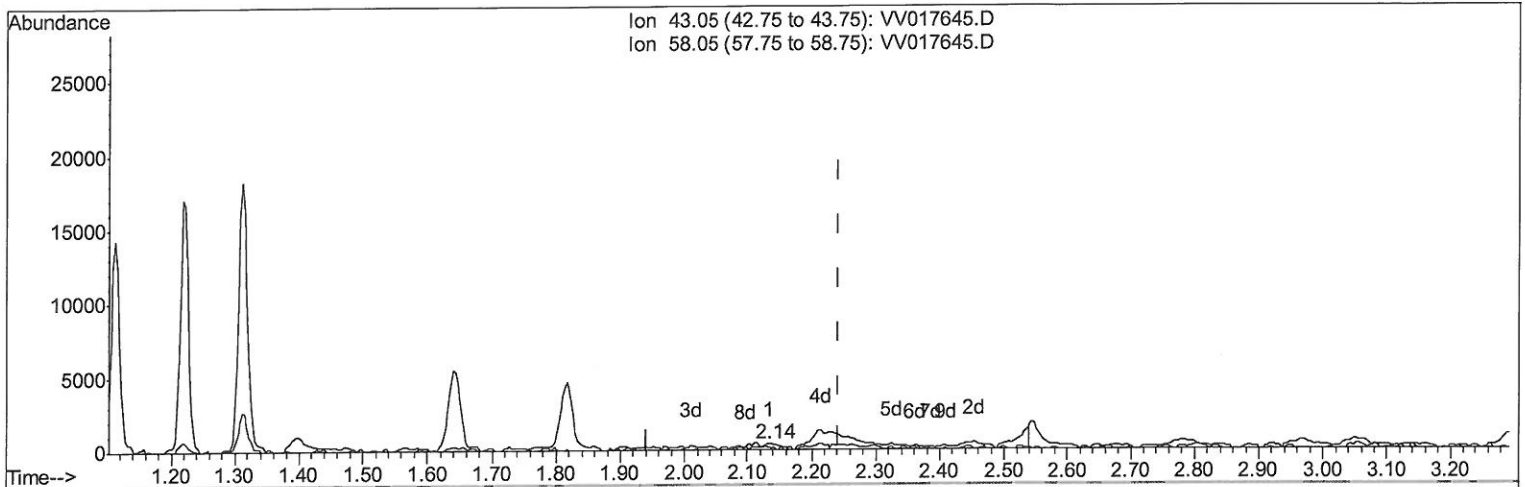

TIC: VV017645.D

(13) Acetone (T)

2.135min (-0.106) 0.57ug/L

response 807

Ion	Exp%	Act%
43.05	100	100
58.05	9.30	13.01
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072420\
 Data File : VV017645.D
 Acq On : 24 Jul 2020 13:39
 Operator : SY/MD
 Sample : L3395-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 GAY20

Manual Integrations
APPROVED

MMDadoda
 7/29/2020 11:24:57 AM

Quant Time: Jul 25 00:08:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 25 00:05:26 2020
 Response via : Initial Calibration

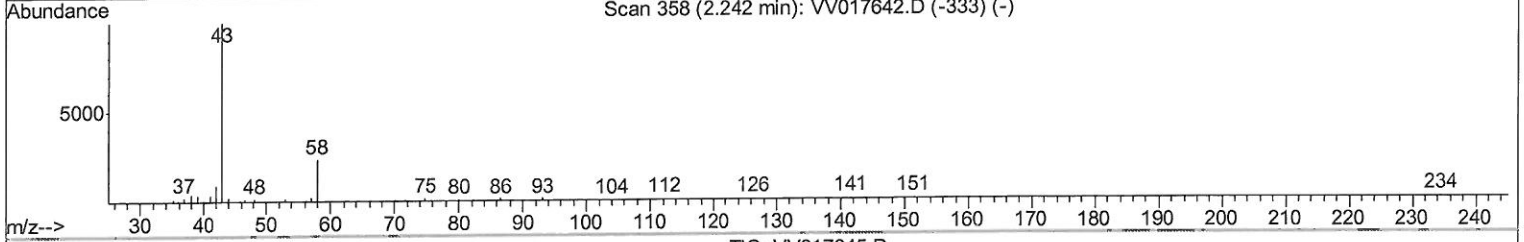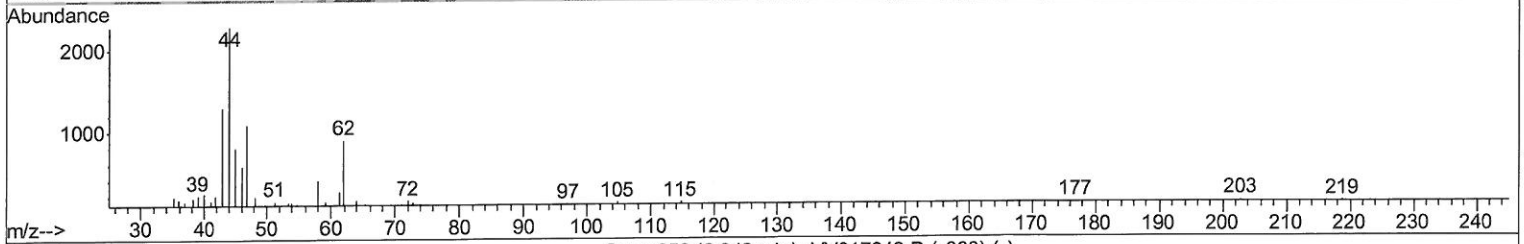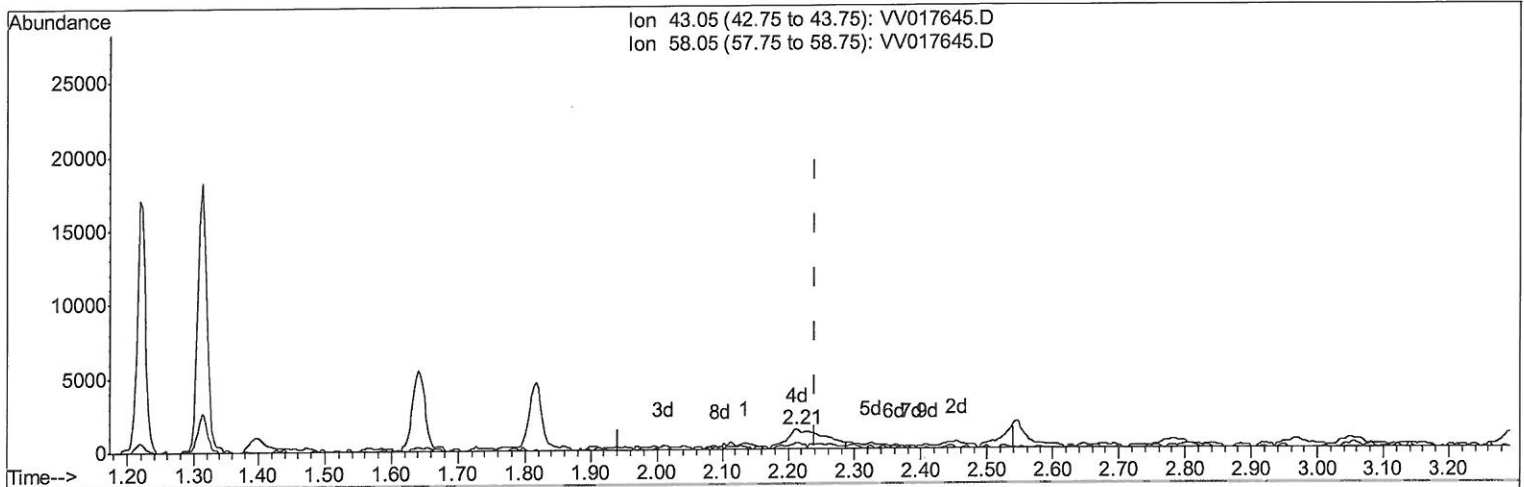

TIC: VV017645.D

(13) Acetone (T)

2.212min (-0.029) 3.71ug/L m

response 5280

Ion	Exp%	Act%
43.05	100	100
58.05	9.30	1.99
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten signature: MD
 7/29/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072420\
 Data File : VV017645.D
 Acq On : 24 Jul 2020 13:39
 Operator : SY/MD
 Sample : L3395-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAY20

Manual Integrations
 APPROVED

MMDadoda
 7/29/2020 11:24:57 AM

Quant Time: Jul 25 00:43:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 25 00:05:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	159246	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	160819	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	79750	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	34262	4.51	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.20%
7) Chloroethane-d5	1.58	69	28420	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.60%
11) 1,1-Dichloroethene-d2	2.12	63	57738	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	3.94	46	88917	48.88	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.76%
24) Chloroform-d	4.37	84	90391	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
26) 1,2-Dichloroethane-d4	5.06	65	53120	5.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.00%
32) Benzene-d6	5.07	84	160504	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.60%
36) 1,2-Dichloropropane-d6	6.09	67	45204	4.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.80%
41) Toluene-d8	7.34	98	142126	4.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.60%
45) trans-1,3-Dichloropropene-	7.65	79	20291	4.54	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.80%
48) 2-Hexanone-d5	8.11	63	64019	46.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.52%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	33397	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.40%
65) 1,2-Dichlorobenzene-d4	11.65	152	62762	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%

Target Compounds

					Ovalue	
13) Acetone	2.21	43	5280m	3.708	ug/L	
14) Carbon disulfide	2.31	76	2987	0.115	ug/L #	65
33) Benzene	5.13	78	6600	0.145	ug/L	100
35) Methylcyclohexane	6.15	83	2018	0.105	ug/L #	61
42) Toluene	7.41	91	27517	0.554	ug/L	99
54) Ethylbenzene	9.03	91	25120	0.452	ug/L	100
55) m,p-xylene	9.16	106	20919	0.999	ug/L	93
56) o-xylene	9.57	106	6799	0.335	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed