

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072420\
 Data File : VV017656.D
 Acq On : 24 Jul 2020 19:24
 Operator : SY/MD
 Sample : L3446-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4C65

Quant Time: Jul 25 02:47:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 25 00:05:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	152732	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	147804	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	75160	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	32383	4.44	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.80%
7) Chloroethane-d5	1.58	69	26780	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.00%
11) 1,1-Dichloroethene-d2	2.12	63	57234	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	3.94	46	74997	42.99	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.98%
24) Chloroform-d	4.38	84	87164	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	5.06	65	45173	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.20%
32) Benzene-d6	5.07	84	155000	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
36) 1,2-Dichloropropane-d6	6.10	67	42347	4.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.40%
41) Toluene-d8	7.34	98	139674	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
45) trans-1,3-Dichloropropene-	7.65	79	17323	4.22	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.40%
48) 2-Hexanone-d5	8.11	63	46442	36.51	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.02%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	25923	4.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.20%
65) 1,2-Dichlorobenzene-d4	11.65	152	57290	5.04	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.80%


Target Compounds					Ovalue
13) Acetone	2.21	43	11340	8.303 ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072420\
Data File : VV017656.D
Acq On : 24 Jul 2020 19:24
Operator : SY/MD
Sample : L3446-07
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4C65

Quant Time: Jul 25 02:47:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 25 00:05:26 2020
Response via : Initial Calibration

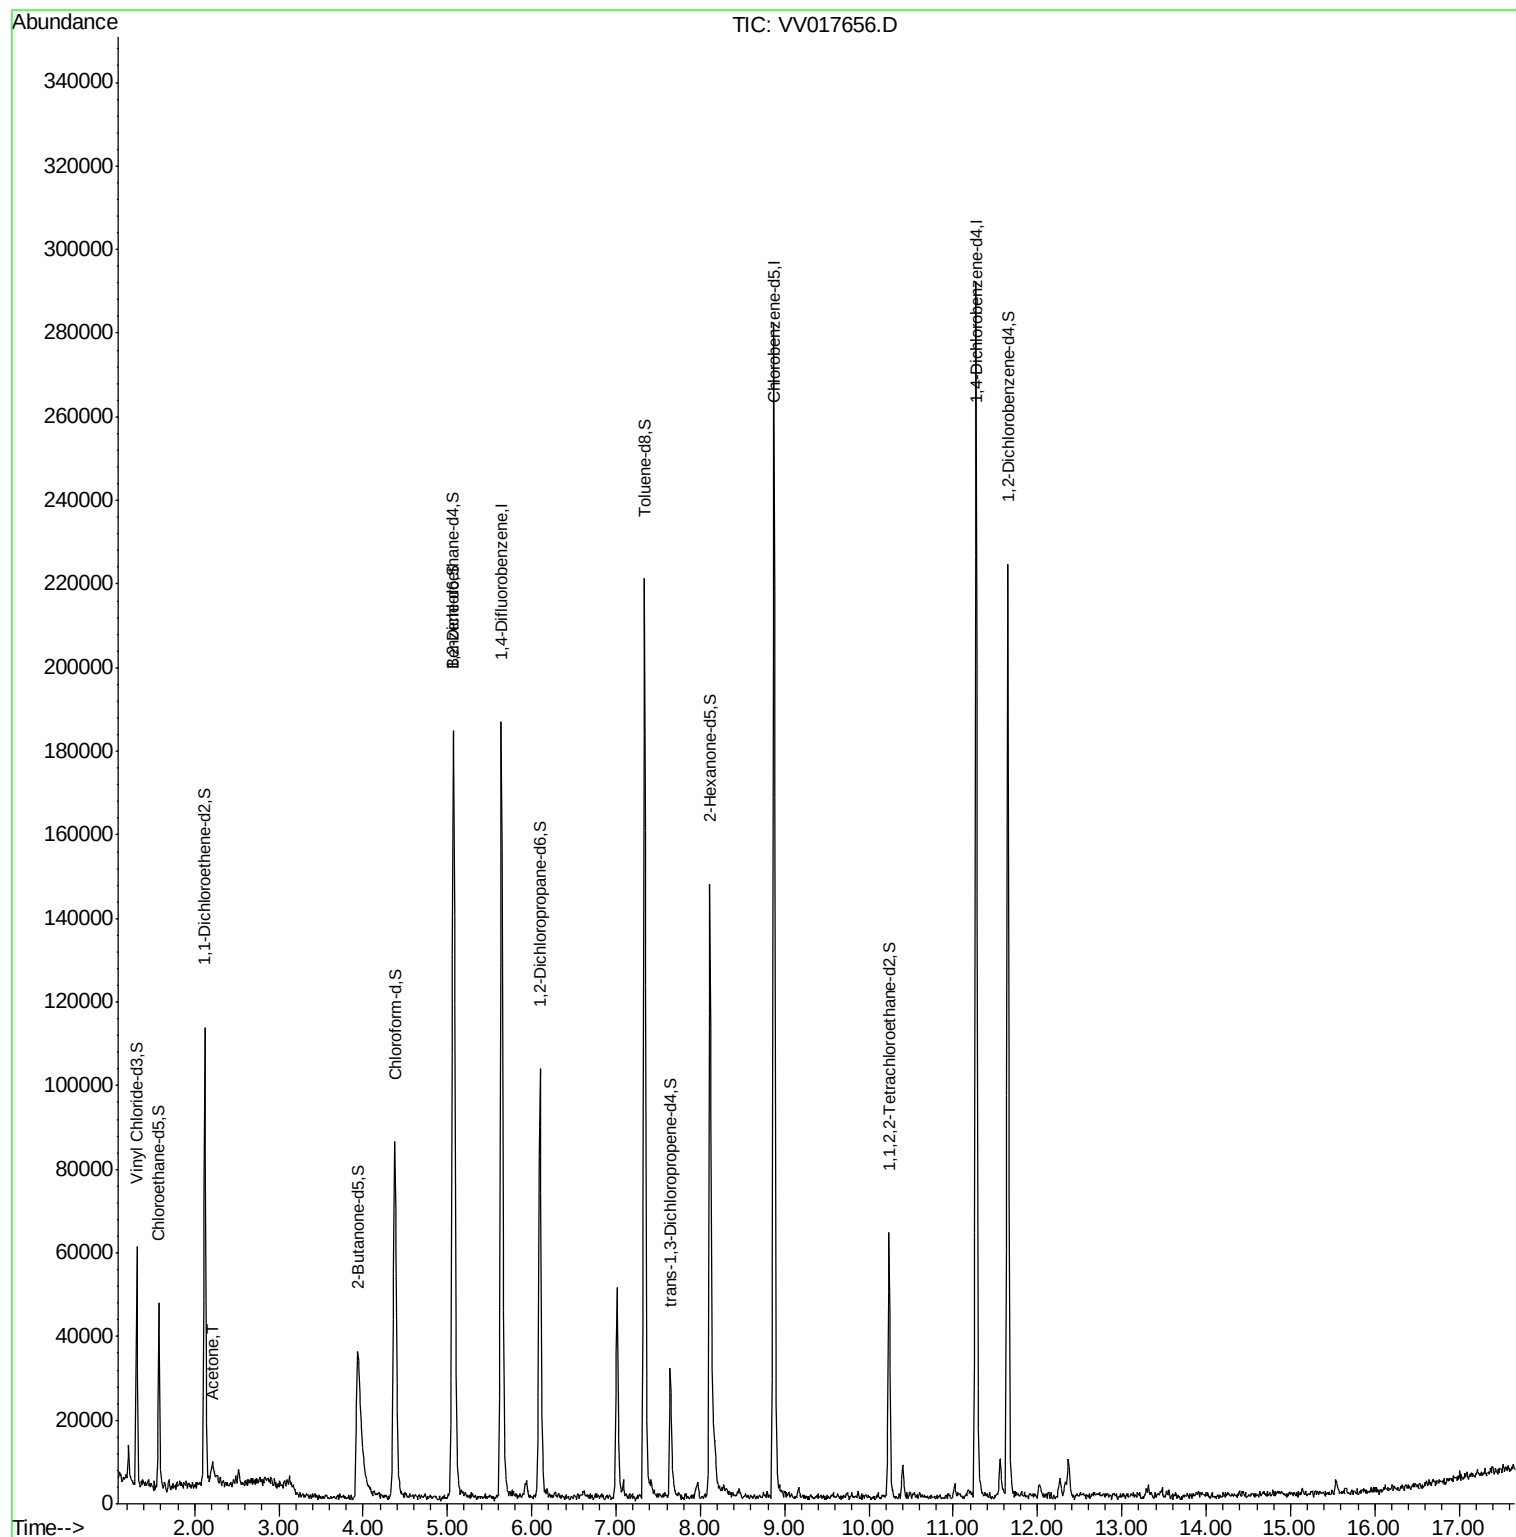

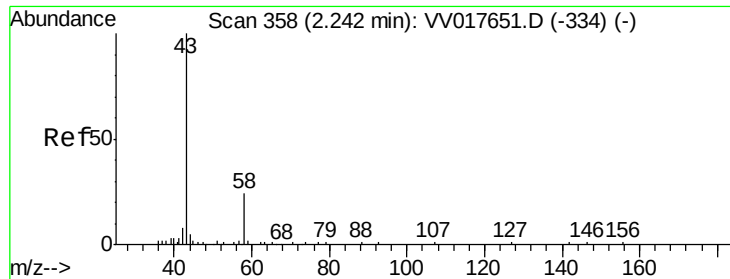

#13

Acetone

Concen: 8.303 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.03 min

Lab File: VV017656.D

Acq: 24 Jul 2020 19:24

Instrument :

MSVOA_V

ClientSampleId :


F4C65

Tot Ion: 43 Resp: 11340

Ion Ratio Lower Upper

43 100

58 17.7 0.0 18.6

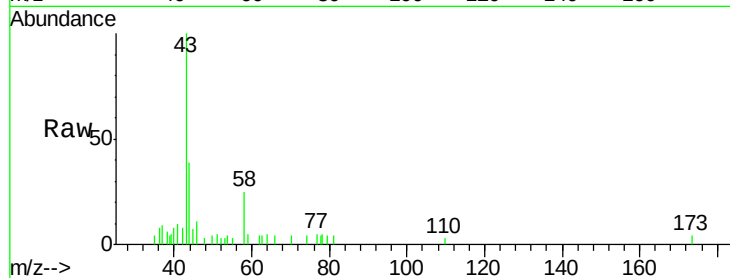

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

