

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072420\
 Data File : VV017657.D
 Acq On : 24 Jul 2020 19:48
 Operator : SY/MD
 Sample : L3446-09
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4C81

Quant Time: Jul 25 02:50:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 25 00:05:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	152751	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	149394	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	72907	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	34857	4.78	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.60%
7) Chloroethane-d5	1.58	69	29620	5.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.20%
11) 1,1-Dichloroethene-d2	2.12	63	58736	3.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.80%
20) 2-Butanone-d5	3.94	46	77180	44.23	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.46%
24) Chloroform-d	4.38	84	88281	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
26) 1,2-Dichloroethane-d4	5.06	65	47385	5.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.00%
32) Benzene-d6	5.07	84	160628	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
36) 1,2-Dichloropropane-d6	6.09	67	43353	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	7.34	98	146788	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
45) trans-1,3-Dichloropropene-	7.65	79	17545	4.23	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.60%
48) 2-Hexanone-d5	8.11	63	46778	36.38	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	72.76%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	27858	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.40%
65) 1,2-Dichlorobenzene-d4	11.65	152	60799	5.51	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	10981	8.039 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072420\
Data File : VV017657.D
Acq On : 24 Jul 2020 19:48
Operator : SY/MD
Sample : L3446-09
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4C81

Quant Time: Jul 25 02:50:50 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 25 00:05:26 2020
Response via : Initial Calibration

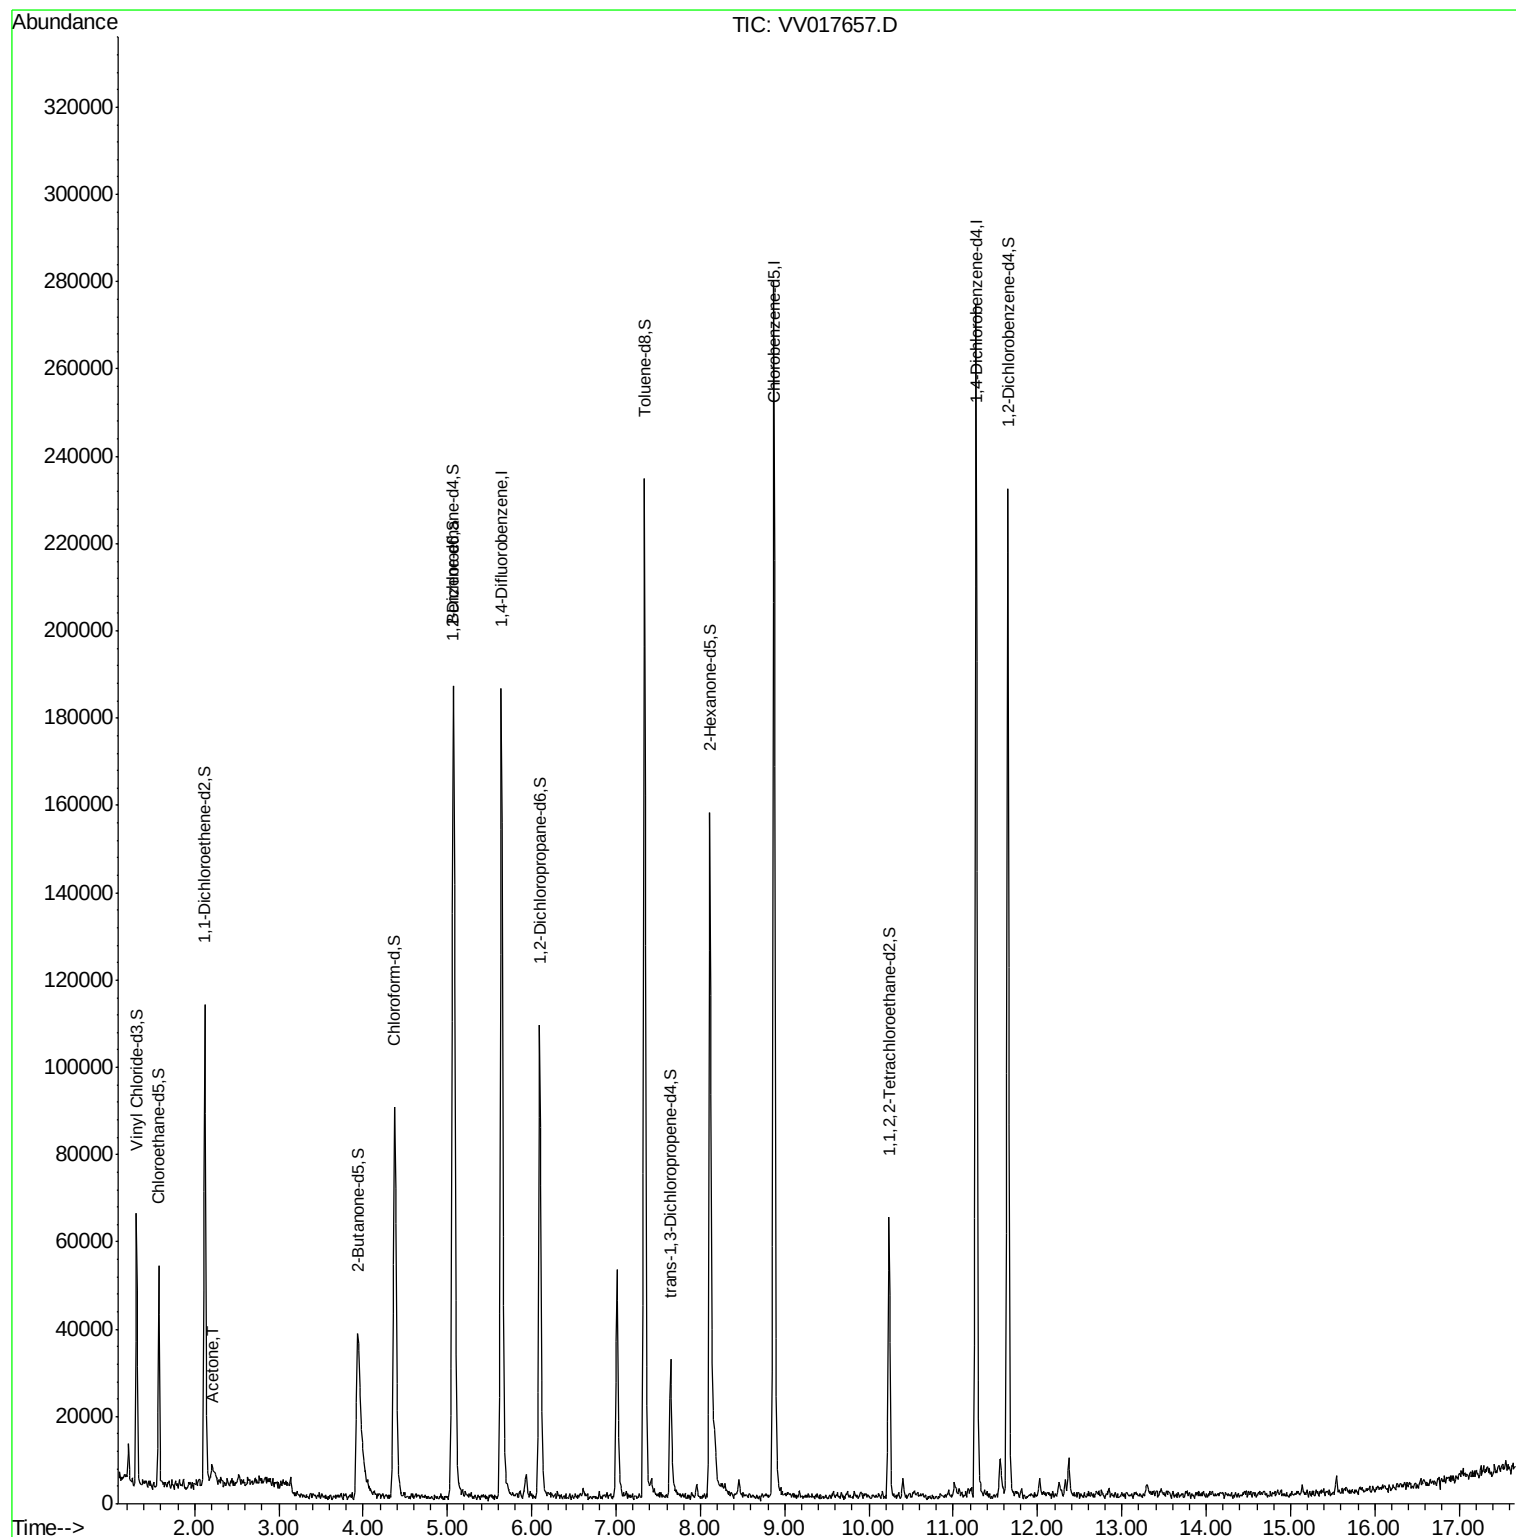

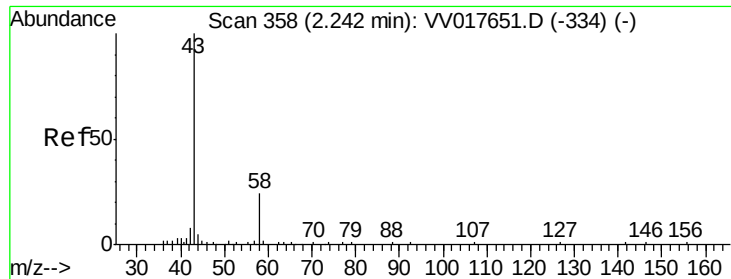

#13

Acetone

Concen: 8.039 ug/L

RT: 2.21 min Scan# 349

Delta R.T. -0.03 min

Lab File: VV017657.D

Acq: 24 Jul 2020 19:48

Instrument :
MSVOA_V
ClientSampleId :
F4C81

Tot Ion: 43 Resp: 10981

Ion Ratio Lower Upper

43 100

58 10.3 0.0 18.6

