


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072424\
Data File : VV036660.D
Acq On : 24 Jul 2024 08:40
Operator : SY/MD
Sample : BFB348
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB348

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072224SMA.M
Title : VOC Analysis
Last Update : Thu Jul 25 00:49:57 2024

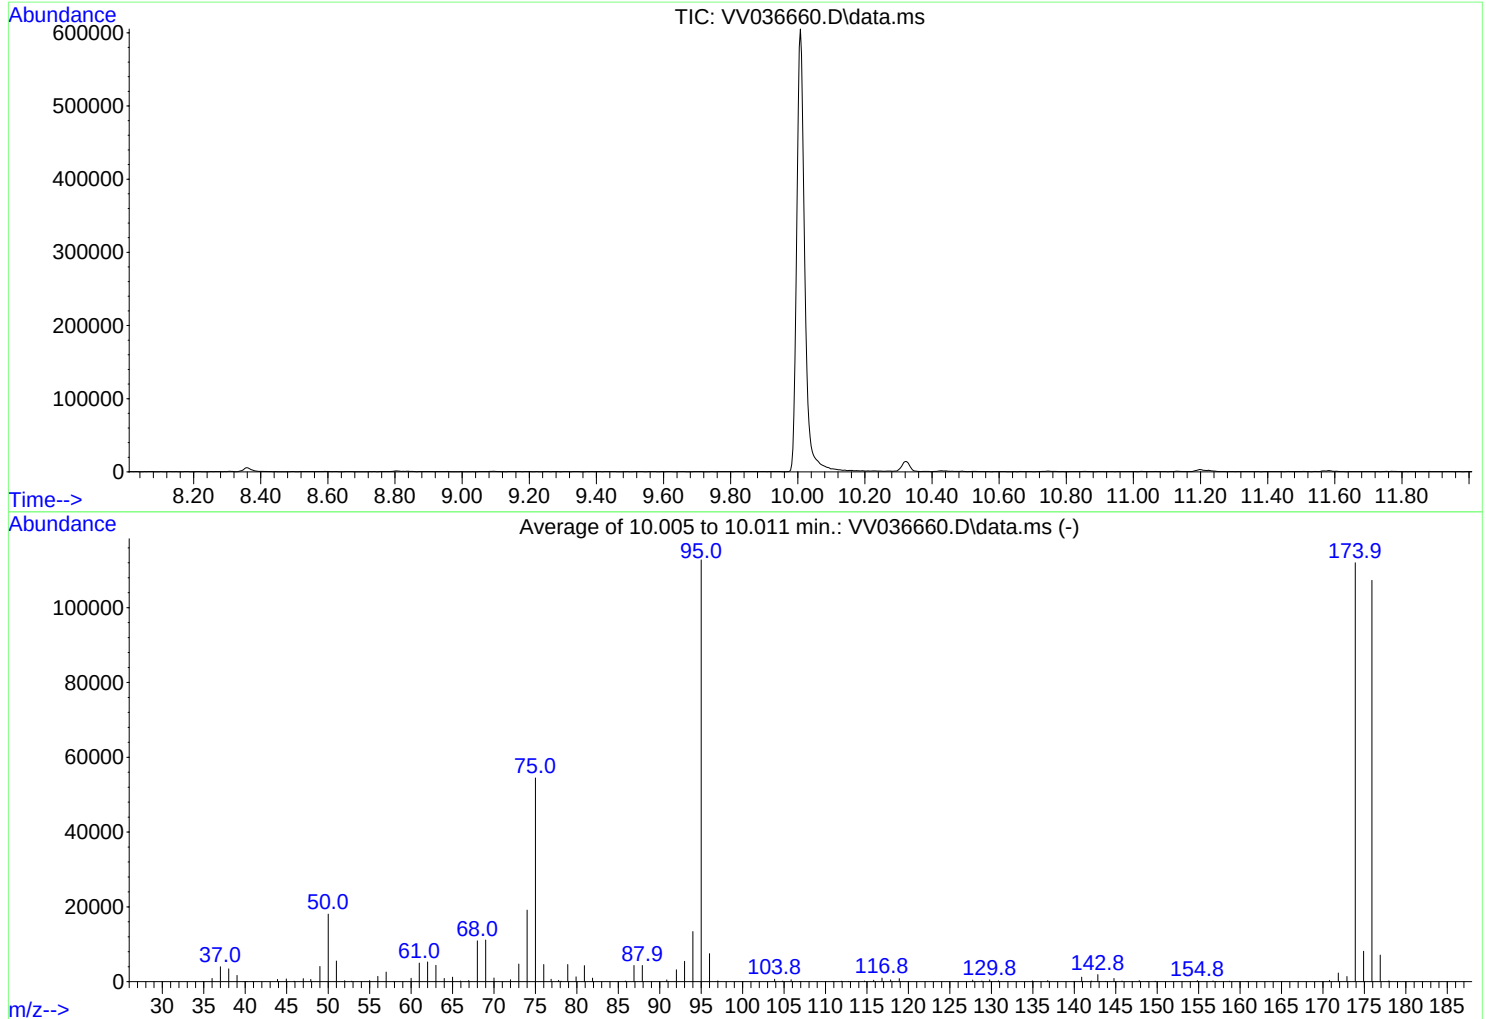

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	18069	PASS
75	95	30	80	48.3	54464	PASS
95	95	100	100	100.0	112795	PASS
96	95	5	9	6.7	7501	PASS
173	174	0.00	2	1.2	1360	PASS
174	95	50	120	99.3	112035	PASS
175	174	5	9	7.2	8122	PASS
176	174	95	101	95.8	107325	PASS
177	176	5	9	6.6	7112	PASS

m/z	Abundance
39.80	110.0
43.80	321.0

Instrument :
MSVOA_V
ClientSampleId :
BFB348

m/z	Abundance
36.00	897.0
37.00	4066.0
38.00	3510.0
39.00	1703.0
39.90	155.0
40.20	168.0
40.90	106.0
44.00	910.0
45.00	722.0
45.90	143.0
47.00	867.0
47.90	595.0
49.00	4143.0
50.00	18376.0
51.00	5549.0
52.00	287.0
52.80	137.0
55.00	287.0
56.00	1390.0
57.00	2682.0
58.00	105.0
60.00	889.0
61.00	5147.0
62.00	5399.0
63.00	4320.0
64.00	819.0
65.00	1219.0
65.90	149.0
66.90	330.0
68.00	11170.0
69.00	11412.0
70.00	1030.0
72.00	503.0
73.00	4611.0
74.00	19464.0
75.00	54664.0
76.00	4527.0
76.90	605.0
77.80	332.0
78.10	352.0
78.90	4758.0
79.90	1321.0
80.90	4457.0
81.90	965.0
85.90	183.0
86.90	4397.0
87.90	4418.0
90.80	438.0
92.00	3123.0
93.00	5219.0
94.00	13524.0
95.00	111864.0
96.00	7596.0
97.00	268.0
103.90	603.0
104.80	193.0
105.90	504.0
106.90	115.0
110.90	113.0
111.90	125.0
112.80	125.0
114.70	165.0
115.80	343.0
116.80	1037.0
117.90	464.0
118.90	854.0
127.80	420.0
128.90	185.0
129.80	420.0
130.90	209.0
135.00	233.0
136.80	290.0
140.10	101.0
140.90	1207.0
142.00	162.0
142.90	1961.0
144.80	909.0
145.80	189.0
147.80	314.0
149.70	138.0
154.90	323.0
156.70	193.0
158.70	121.0
160.80	142.0
170.80	338.0
171.90	2274.0
172.90	1401.0
173.90	108800.0
174.90	7974.0
175.90	104088.0
176.90	7025.0
178.00	237.0

Instrument :
MSVOA_V
ClientSampleId :
BFB348

m/z	Abundance
36.00	876.0
37.00	4056.0
38.00	3476.0
39.00	1751.0
39.90	172.0
44.00	932.0
45.00	736.0
45.90	157.0
47.00	836.0
47.90	625.0
49.00	4164.0
50.00	18712.0
51.00	5711.0
52.00	285.0
52.90	135.0
55.00	299.0
56.00	1451.0
57.00	2590.0
57.90	111.0
60.00	913.0
61.00	5069.0
62.00	5482.0
63.00	4571.0
64.00	881.0
65.00	1213.0
66.00	170.0
67.00	294.0
68.00	11263.0
69.00	11438.0
70.00	1003.0
72.00	521.0
73.00	4847.0
74.00	19840.0
75.00	56376.0
76.00	4721.0
76.90	648.0
77.80	387.0
78.90	4744.0
79.90	1338.0
80.90	4423.0
81.90	966.0
85.80	187.0
86.90	4482.0
87.90	4444.0
90.90	477.0
92.00	3270.0
93.00	5616.0
94.00	13861.0
95.00	116512.0
96.00	7763.0
97.00	229.0
103.90	654.0
104.80	202.0
105.90	557.0
106.90	102.0
110.90	108.0
111.90	125.0
112.80	112.0
114.70	192.0
115.80	366.0
116.80	1019.0
117.90	518.0
118.90	871.0
127.80	468.0
128.80	201.0
129.80	459.0
130.80	218.0
134.90	256.0
136.80	311.0
140.00	121.0
140.90	1236.0
142.00	164.0
142.90	1946.0
143.80	110.0
144.80	918.0
145.80	190.0
147.80	304.0
148.80	104.0
149.70	141.0
154.90	323.0
156.70	209.0
157.10	153.0
158.70	137.0
160.90	122.0
170.80	361.0
171.90	2354.0
172.90	1400.0
173.90	116112.0
174.90	8345.0
175.90	111112.0
176.90	7340.0
177.90	252.0

Instrument :
MSVOA_V
ClientSampleId :
BFB348

m/z	Abundance
36.00	759.0
37.00	3828.0
38.00	3284.0
39.00	1588.0
40.00	198.0
44.00	877.0
44.90	727.0
45.90	154.0
47.00	780.0
47.90	549.0
49.00	3871.0
50.00	17120.0
51.00	5263.0
52.00	228.0
52.90	147.0
55.00	308.0
56.00	1354.0
57.00	2432.0
57.90	101.0
60.00	882.0
61.00	4628.0
62.00	4948.0
63.00	4211.0
64.00	849.0
65.00	1186.0
66.00	179.0
67.00	252.0
68.00	10256.0
69.00	10573.0
70.00	883.0
72.00	525.0
73.00	4685.0
74.00	18128.0
75.00	52352.0
76.00	4531.0
76.90	630.0
77.80	362.0
78.90	4267.0
79.90	1169.0
80.90	3974.0
81.90	899.0
85.90	179.0
86.90	4051.0
87.90	4109.0
90.90	472.0
92.00	3168.0
93.00	5517.0
94.00	12832.0
95.00	110008.0
96.00	7143.0
97.00	175.0
103.80	614.0
104.90	189.0
105.80	536.0
106.90	111.0
111.90	118.0
114.70	177.0
115.80	409.0
116.80	845.0
117.80	490.0
118.90	763.0
127.70	466.0
128.80	200.0
129.80	531.0
130.80	222.0
134.90	212.0
136.80	251.0
139.90	110.0
140.90	1107.0
142.10	149.0
142.80	1695.0
143.80	127.0
144.80	793.0
145.70	193.0
147.90	260.0
149.80	115.0
154.80	317.0
156.80	204.0
158.80	134.0
170.80	324.0
171.80	2333.0
172.90	1279.0
173.90	111192.0
174.90	8046.0
175.90	106776.0
176.90	6972.0
177.90	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB348