

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072519\
 Data File : VV012038.D
 Acq On : 25 Jul 2019 19:47
 Operator : SY/MD
 Sample : K4004-01
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2A27

Quant Time: Aug 10 22:58:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 26 23:19:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	128254	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	123457	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	60235	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	26743	4.01	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.20%
7) Chloroethane-d5	1.59	69	24057	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.13	63	42593	3.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.20%
20) 2-Butanone-d5	3.96	46	105738	54.27	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.54%
24) Chloroform-d	4.40	84	80163	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
26) 1,2-Dichloroethane-d4	5.09	65	48079	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.80%
32) Benzene-d6	5.10	84	163156	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
36) 1,2-Dichloropropane-d6	6.12	67	48971	4.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.40%
41) Toluene-d8	7.36	98	143928	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.20%
43) trans-1,3-Dichloropropene-	7.67	79	18547	4.64	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.80%
46) 2-Hexanone-d5	8.14	63	85873	53.48	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.96%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35270	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	60472	5.21	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.20%


Target Compounds					Ovalue
22) cis-1,2-Dichloroethene	3.96	96	2857	0.292 ug/L	89
34) Trichloroethene	5.96	95	59460	5.896 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072519\
Data File : VV012038.D
Acq On : 25 Jul 2019 19:47
Operator : SY/MD
Sample : K4004-01
Misc : 25ML/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2A27

Quant Time: Aug 10 22:58:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 26 23:19:45 2019
Response via : Initial Calibration

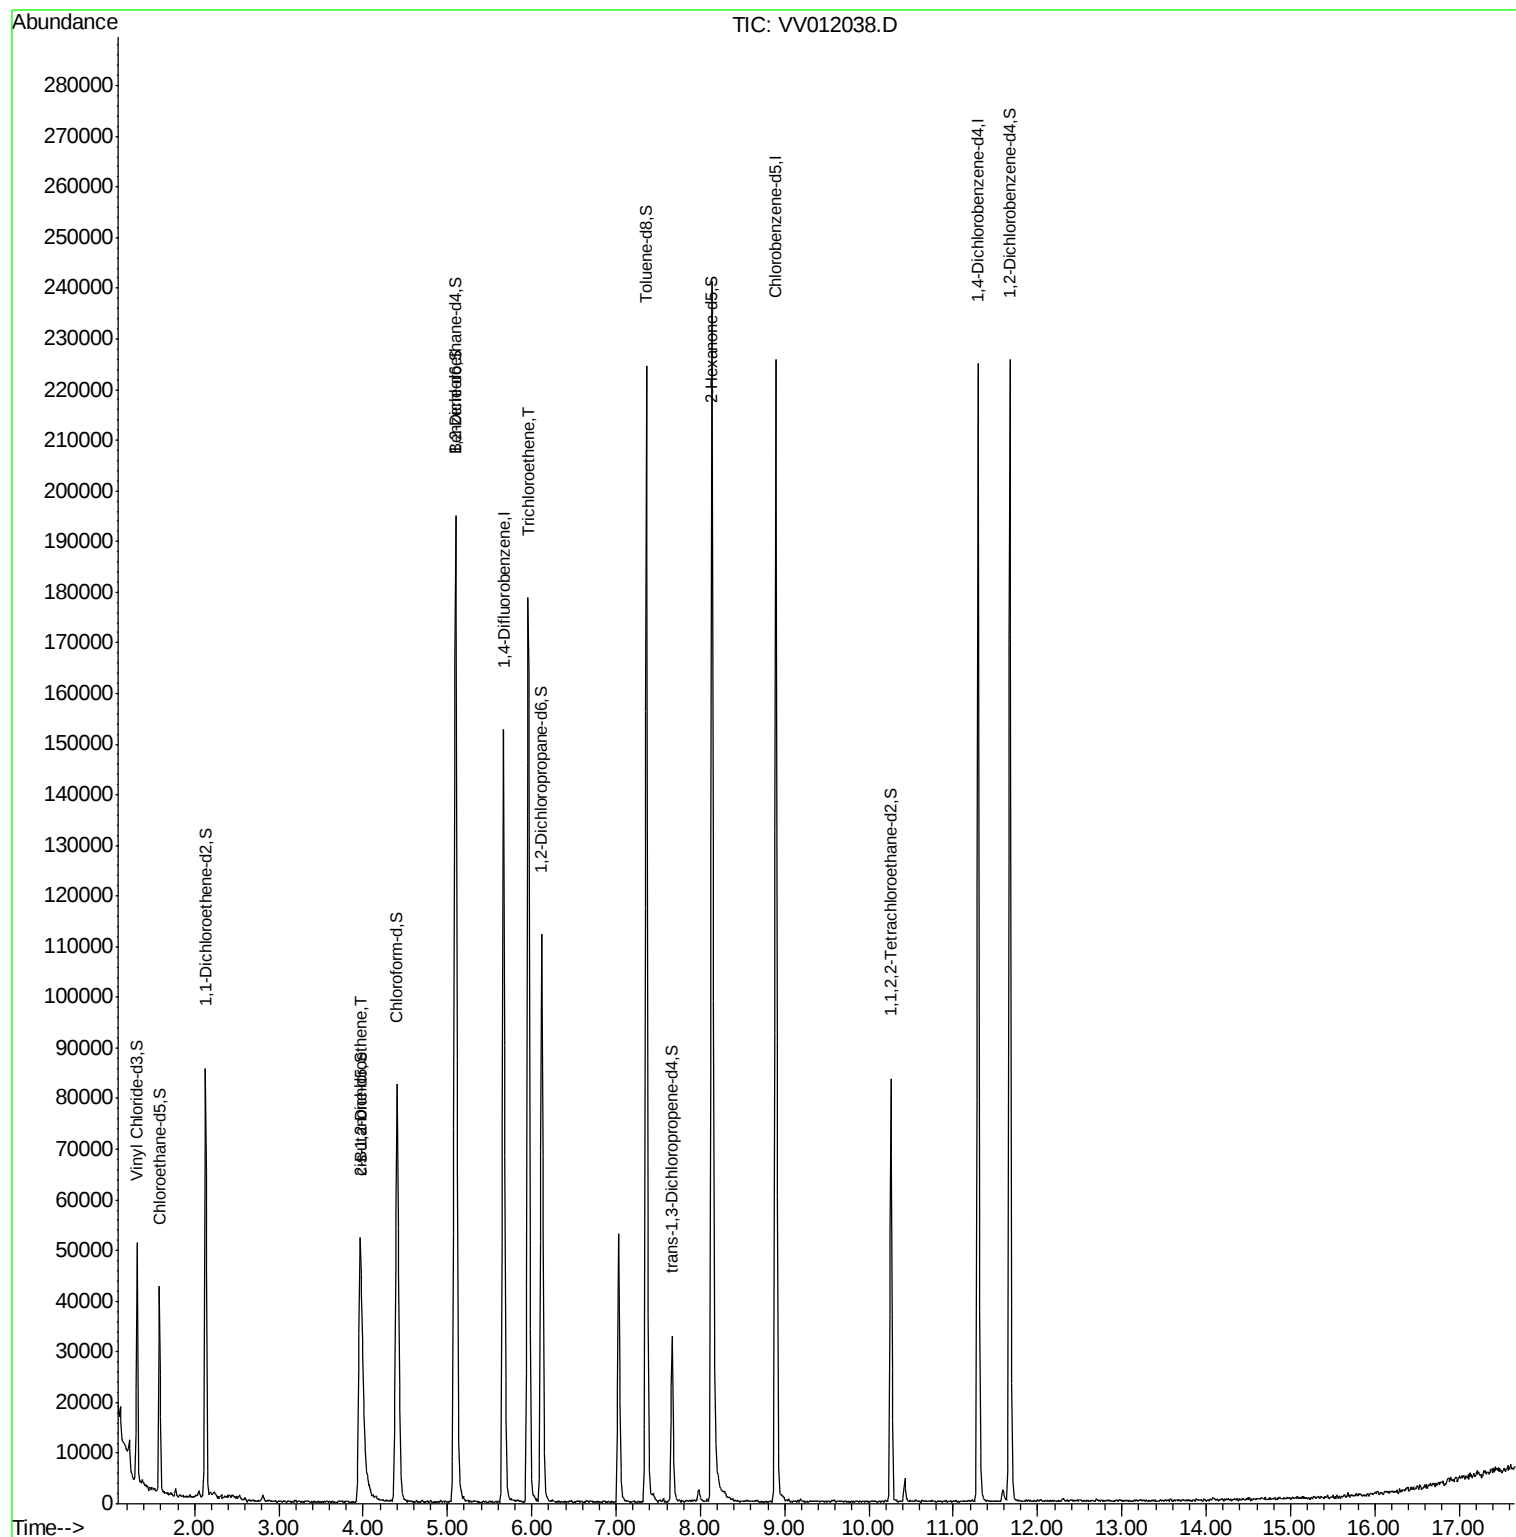

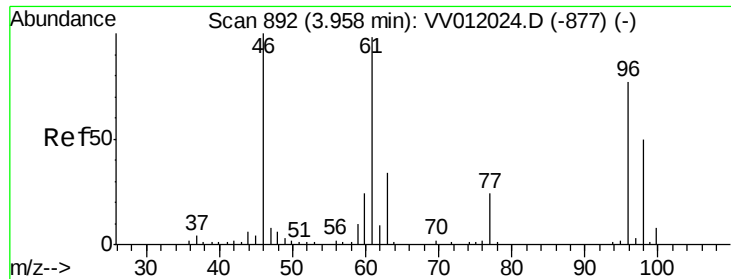


#22




cis-1,2-Dichloroethene
Concen: 0.292 ug/L
RT: 3.96 min Scan# 893
Delta R.T. -0.00 min
Lab File: VV012038.D
Acq: 25 Jul 2019 19:47

Instrument :
MSVOA_V
ClientSampleId :
F2A27

Tot Ion: 96 Resp: 2857
Ion Ratio Lower Upper
96 100
61 114.8 89.0 165.2
68 0.0 0.0 0.0

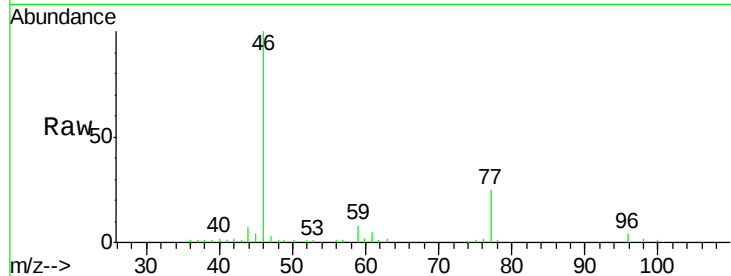


Abundance Ion 96.00 (95.70 to 96.70): VV0
Ion 61.05 (60.75 to 61.75): VV0
Ion 68.15 (67.85 to 68.85): VV0

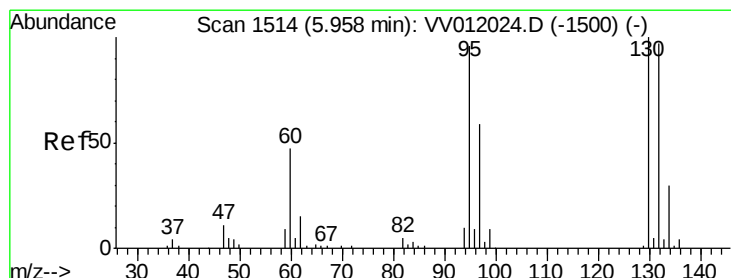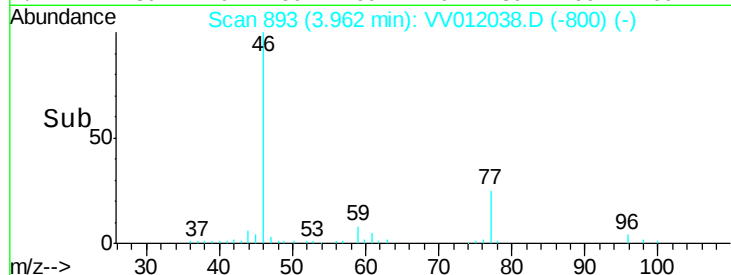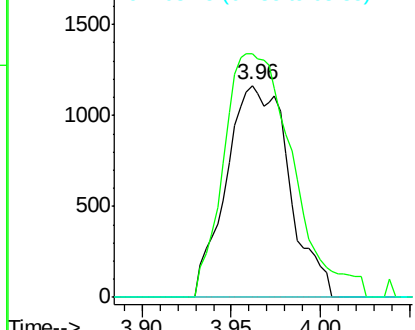

#34

Trichloroethene
Concen: 5.896 ug/L
RT: 5.96 min Scan# 1514
Delta R.T. -0.00 min
Lab File: VV012038.D
Acq: 25 Jul 2019 19:47

Tgt Ion: 95 Resp: 59460
Ion Ratio Lower Upper
95 100
97 63.4 45.6 84.6
132 99.7 71.3 132.3
130 103.9 72.8 135.2

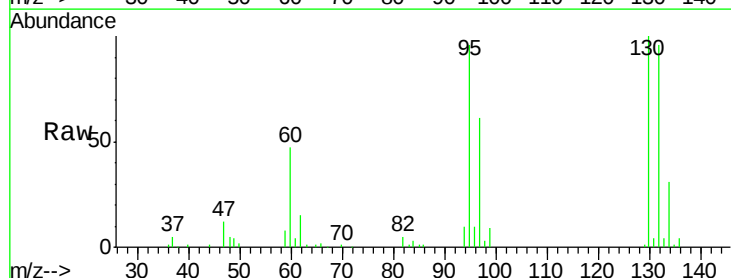

Abundance Ion 95.00 (94.70 to 95.70): VV0
Ion 96.95 (96.65 to 97.65): VV0
Ion 131.95 (131.65 to 132.65): VV0
Ion 129.95 (129.65 to 130.65): VV0

