


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072519\
 Data File : VV012023.D
 Acq On : 25 Jul 2019 08:58
 Operator : SY/MD
 Sample : BFB38
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB38

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jul 26 02:35:49 2019

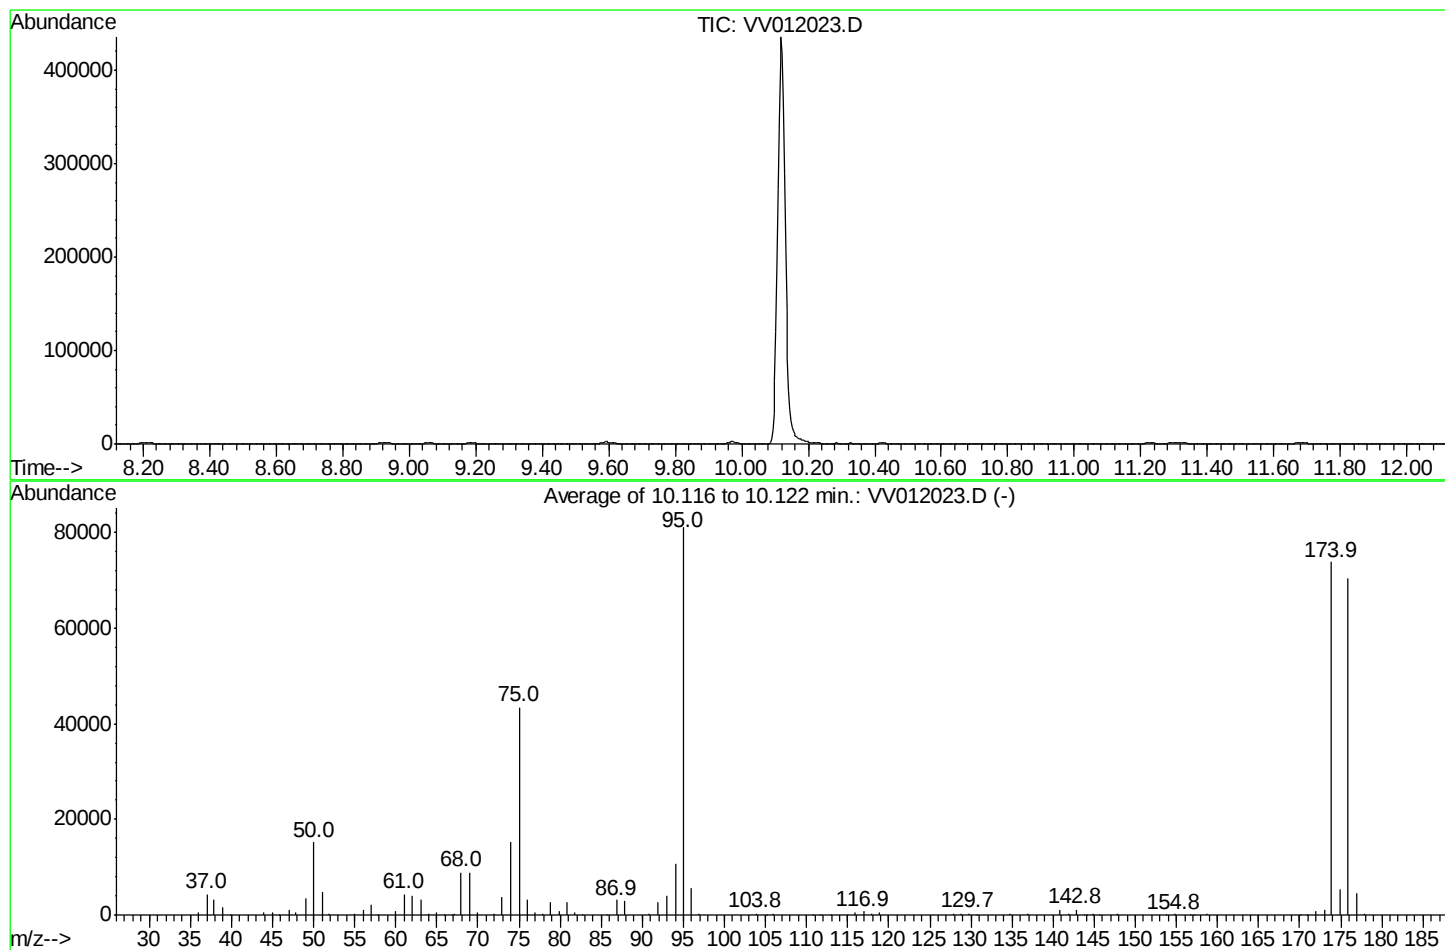

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	15180	PASS
75	95	30	80	53.7	43512	PASS
95	95	100	100	100.0	81085	PASS
96	95	5	9	6.9	5617	PASS
173	174	0.00	2	1.4	1063	PASS
174	95	50	120	91.1	73850	PASS
175	174	5	9	7.4	5499	PASS
176	174	95	101	95.2	70290	PASS
177	176	5	9	6.5	4559	PASS

Scan 2794 (10.074 min): VV012023.D
BFB38

m/z	Abundance
39.80	158.0
43.80	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
36.00	590.0
37.00	4176.0
37.90	3300.0
38.90	1634.0
39.90	199.0
44.00	676.0
45.00	645.0
45.80	116.0
46.90	853.0
47.90	618.0
49.00	3427.0
50.00	15137.0
51.00	4769.0
51.90	331.0
55.00	285.0
56.00	1215.0
57.00	2284.0
57.80	123.0
59.90	816.0
61.00	4448.0
61.90	3938.0
63.00	3339.0
64.10	392.0
65.00	589.0
65.90	154.0
66.80	222.0
67.90	8408.0
69.00	8932.0
69.90	654.0
72.10	413.0
73.00	4038.0
74.00	15033.0
75.00	43272.0
76.00	3213.0
76.90	522.0
78.00	301.0
78.80	2503.0
79.90	844.0
80.90	2785.0
81.80	597.0
85.70	101.0
86.90	3004.0
87.90	2955.0
90.70	334.0
92.00	2606.0
92.90	3804.0
94.00	10266.0
95.00	79616.0
96.00	5535.0
96.90	202.0
103.80	448.0
105.20	104.0
105.80	374.0
110.80	109.0
111.70	124.0
112.80	110.0
114.90	115.0
115.80	436.0
116.90	739.0
117.90	314.0
118.80	507.0
127.90	288.0
128.90	116.0
129.70	360.0
130.70	116.0
134.90	153.0
136.80	190.0
140.80	1048.0
141.80	125.0
142.80	1162.0
143.80	111.0
144.00	114.0
144.90	247.0
145.80	137.0
147.80	204.0
154.80	245.0
156.70	155.0
157.10	107.0
158.80	146.0
170.80	147.0
171.90	785.0
173.00	1008.0
173.90	70160.0
174.90	5420.0
175.90	66648.0
176.90	4441.0
177.80	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
36.00	623.0
37.00	4587.0
37.90	3346.0
38.90	1775.0
39.90	222.0
44.00	743.0
45.00	673.0
45.80	123.0
47.00	1002.0
47.90	585.0
49.00	3663.0
50.00	15639.0
51.00	4897.0
51.90	291.0
55.00	250.0
56.00	1243.0
57.00	2254.0
57.90	128.0
59.90	883.0
61.00	4541.0
62.00	4143.0
63.00	3385.0
64.00	395.0
65.00	547.0
65.90	129.0
67.10	243.0
67.90	9141.0
69.00	9103.0
69.90	646.0
72.00	391.0
72.90	3831.0
73.90	15598.0
75.00	44984.0
76.00	3401.0
76.90	463.0
77.80	323.0
78.80	2741.0
79.90	806.0
80.90	2887.0
81.80	686.0
85.70	101.0
86.90	3227.0
87.80	3130.0
90.80	336.0
92.00	2668.0
93.00	4037.0
94.00	11073.0
95.00	83360.0
96.00	5801.0
96.90	273.0
103.80	422.0
105.90	418.0
110.80	117.0
111.70	138.0
112.90	138.0
114.90	153.0
115.80	475.0
116.90	709.0
117.90	320.0
118.80	496.0
127.90	328.0
128.80	186.0
129.70	364.0
130.70	112.0
134.80	174.0
136.80	206.0
140.80	1045.0
141.80	178.0
142.80	1202.0
143.80	131.0
144.90	216.0
145.70	140.0
147.80	245.0
154.80	256.0
156.70	123.0
157.20	158.0
158.80	174.0
170.10	125.0
171.90	857.0
173.00	1100.0
173.90	76312.0
174.90	5723.0
175.90	72600.0
176.90	4771.0
177.90	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
36.00	635.0
37.00	4435.0
37.90	3217.0
38.90	1621.0
39.90	212.0
43.90	765.0
44.90	615.0
45.80	103.0
47.00	1041.0
47.80	545.0
49.00	3350.0
50.00	14765.0
51.00	4740.0
51.90	263.0
55.00	202.0
56.00	1073.0
57.00	2092.0
60.00	811.0
61.00	4195.0
62.00	4018.0
63.00	3343.0
64.00	393.0
65.00	509.0
67.10	210.0
68.00	8981.0
69.00	8314.0
70.00	526.0
71.90	375.0
72.90	3542.0
73.90	14792.0
75.00	42280.0
76.00	3349.0
77.00	375.0
77.80	319.0
78.80	2808.0
79.90	734.0
80.90	2703.0
81.80	689.0
82.70	117.0
86.90	3104.0
87.80	3007.0
90.80	325.0
91.90	2553.0
93.00	3874.0
94.00	10577.0
95.00	80280.0
96.00	5516.0
96.90	296.0
103.90	349.0
105.90	401.0
110.80	112.0
111.70	120.0
112.90	120.0
114.90	155.0
115.90	439.0
116.90	629.0
117.90	345.0
118.80	463.0
127.90	329.0
128.80	246.0
129.70	329.0
130.70	123.0
134.70	183.0
136.90	174.0
140.80	946.0
141.90	214.0
142.80	1158.0
143.80	111.0
144.80	212.0
145.60	141.0
147.80	232.0
153.70	106.0
154.80	216.0
157.20	162.0
158.70	153.0
170.10	178.0
171.90	920.0
173.00	1083.0
173.90	75080.0
174.90	5355.0
175.90	71624.0
176.90	4466.0
177.90	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38