

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072523\
 Data File : VW031744.D
 Acq On : 25 Jul 2023 16:27
 Operator : SY/MD
 Sample : 03712-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W6

Quant Time: Jul 26 02:57:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 26 02:25:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	262424	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	300631	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	136568	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	116067	43.386	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.780%
7) Chloroethane-d5	1.532	69	111369	45.426	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.860%
11) 1,1-Dichloroethene-d2	2.059	65	53939	43.558	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.120%
21) 2-Butanone-d5	3.793	46	210485	113.704	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	113.700%
24) Chloroform-d	4.256	84	275434	50.077	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.160%
26) 1,2-Dichloroethane-d4	4.947	65	173360	50.657	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.320%
32) Benzene-d6	4.966	84	412008	43.279	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.560%
36) 1,2-Dichloropropane-d6	5.995	67	161260	45.096	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.200%
41) Toluene-d8	7.249	98	309891	38.836	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	77.680%#
43) trans-1,3-Dichloroprop...	7.558	79	62939	40.948	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.900%
47) 2-Hexanone-d5	8.030	63	132560	98.853	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.850%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	245535	49.834	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.660%
66) 1,2-Dichlorobenzene-d4	11.567	152	140820	50.928	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.860%
Target Compounds					Qvalue	
13) Acetone	2.117	43	11177	6.308	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031744.D
Acq On : 25 Jul 2023 16:27
Operator : SY/MD
Sample : 03712-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W6

Quant Time: Jul 26 02:57:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 26 02:25:02 2023
Response via : Initial Calibration

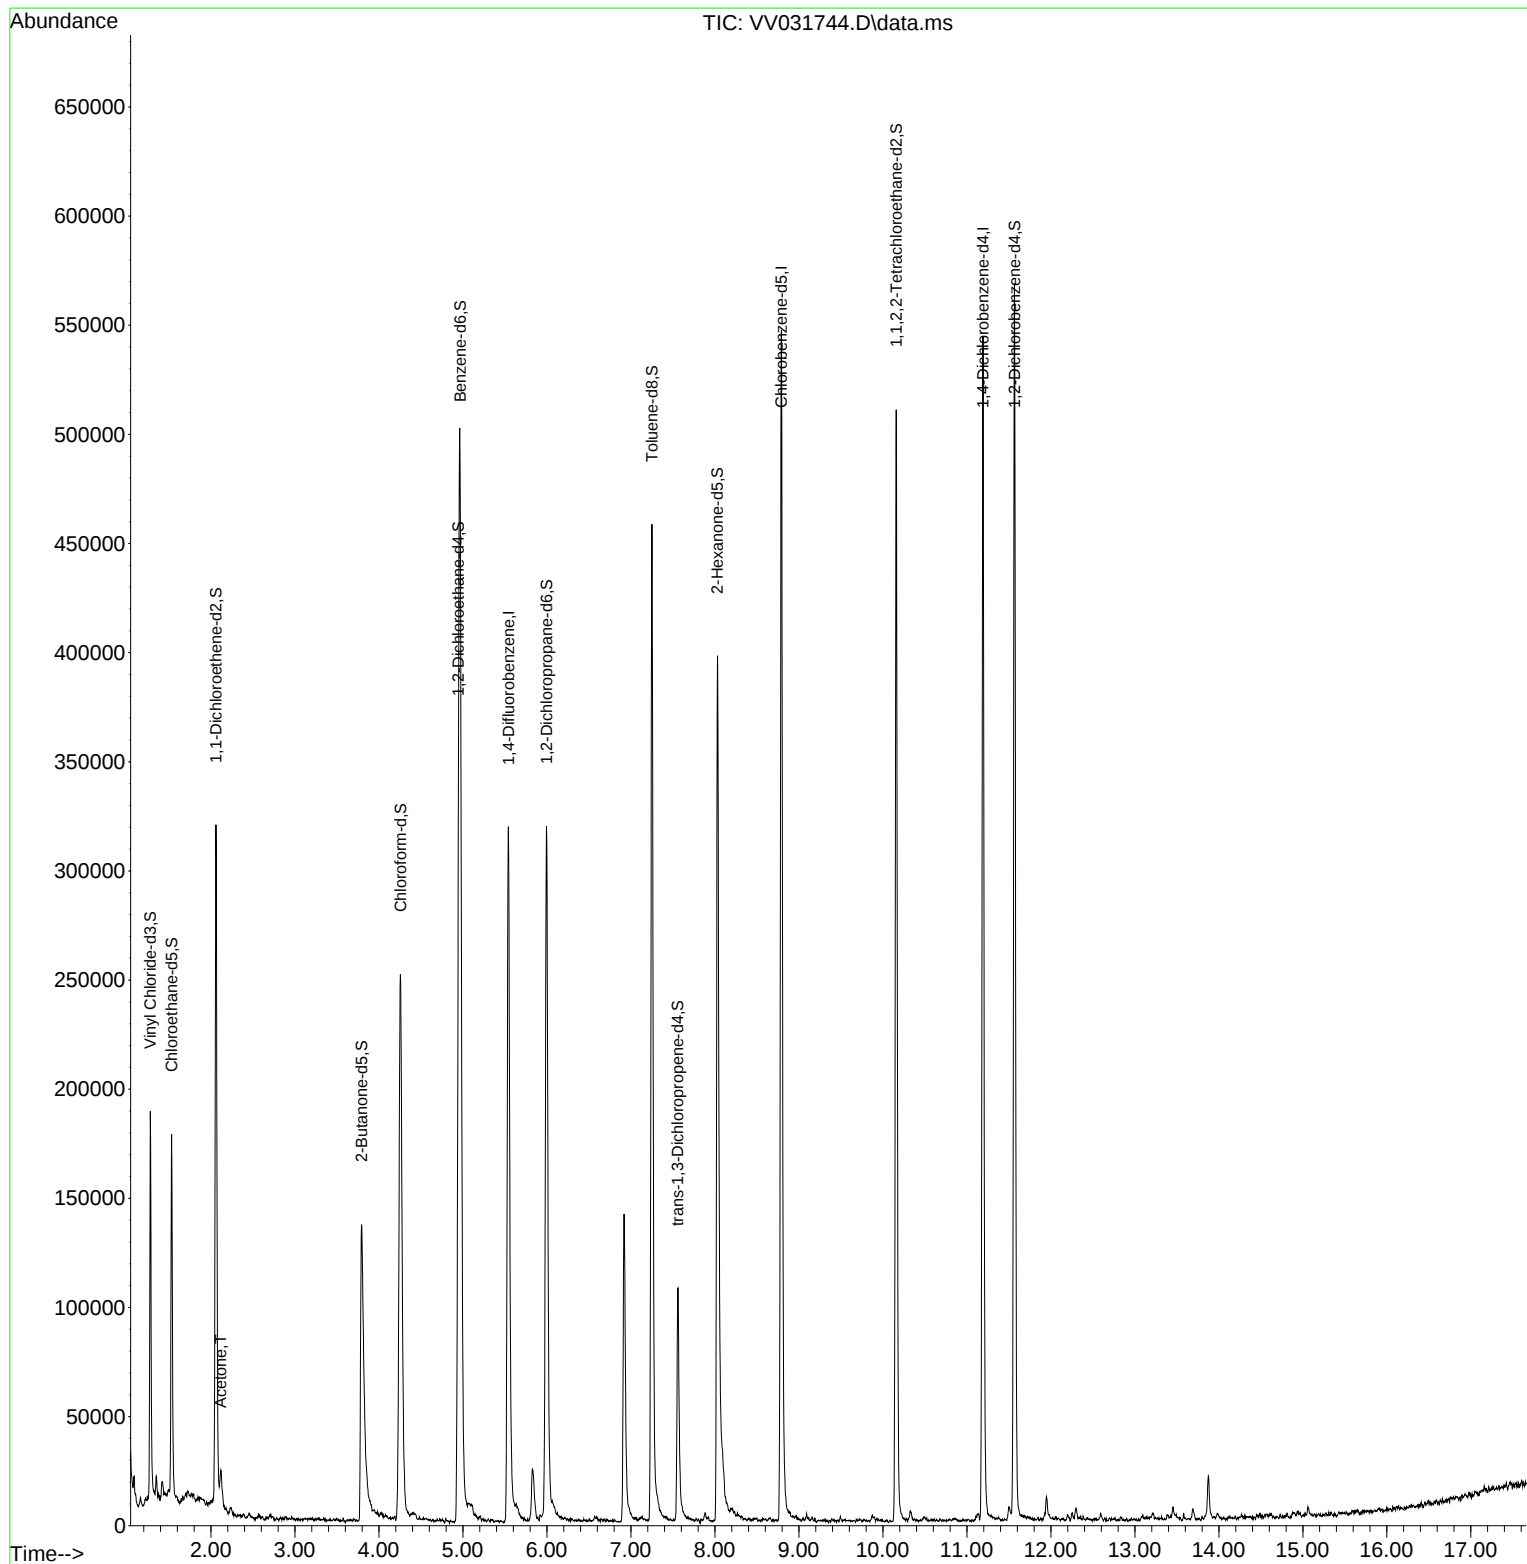

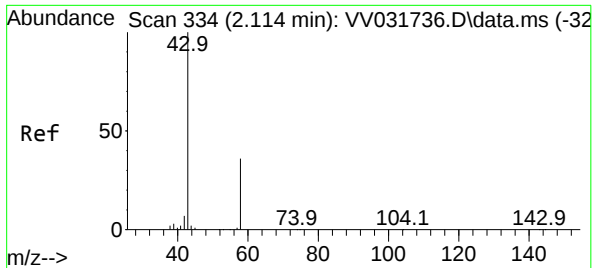

#13
 Acetone
 Concen: 6.308 ug/L
 RT: 2.117 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV031744.D
 Acq: 25 Jul 2023 16:27

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W6

Tgt Ion: 43 Resp: 11177
 Ion Ratio Lower Upper
 43 100
 58 34.7 0.0 72.0

