

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072523\
 Data File : VW031749.D
 Acq On : 25 Jul 2023 18:25
 Operator : SY/MD
 Sample : 03712-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2Y5

Quant Time: Jul 26 02:57:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 26 02:25:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	335546	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	358559	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	170114	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	158085	46.215	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	92.420%	
7) Chloroethane-d5	1.532	69	142853	45.571	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	91.140%	
11) 1,1-Dichloroethene-d2	2.060	65	72079	45.522	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.040%	
21) 2-Butanone-d5	3.793	46	224492	94.843	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	94.840%	
24) Chloroform-d	4.256	84	327191	46.524	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.040%	
26) 1,2-Dichloroethane-d4	4.947	65	211417	48.315	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.640%	
32) Benzene-d6	4.966	84	524042	46.154	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.300%	
36) 1,2-Dichloropropane-d6	5.995	67	202946	47.584	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	95.160%	
41) Toluene-d8	7.249	98	417701	43.890	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	87.780%	
43) trans-1,3-Dichloroprop...	7.558	79	80672	44.006	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	88.020%	
47) 2-Hexanone-d5	8.030	63	139466	87.200	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	87.200%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	271756	46.245	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	92.480%	
66) 1,2-Dichlorobenzene-d4	11.567	152	182781	53.068	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	106.140%	
Target Compounds						
13) Acetone	2.117	43	47786	21.092	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031749.D
Acq On : 25 Jul 2023 18:25
Operator : SY/MD
Sample : 03712-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2Y5

Quant Time: Jul 26 02:57:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 26 02:25:02 2023
Response via : Initial Calibration

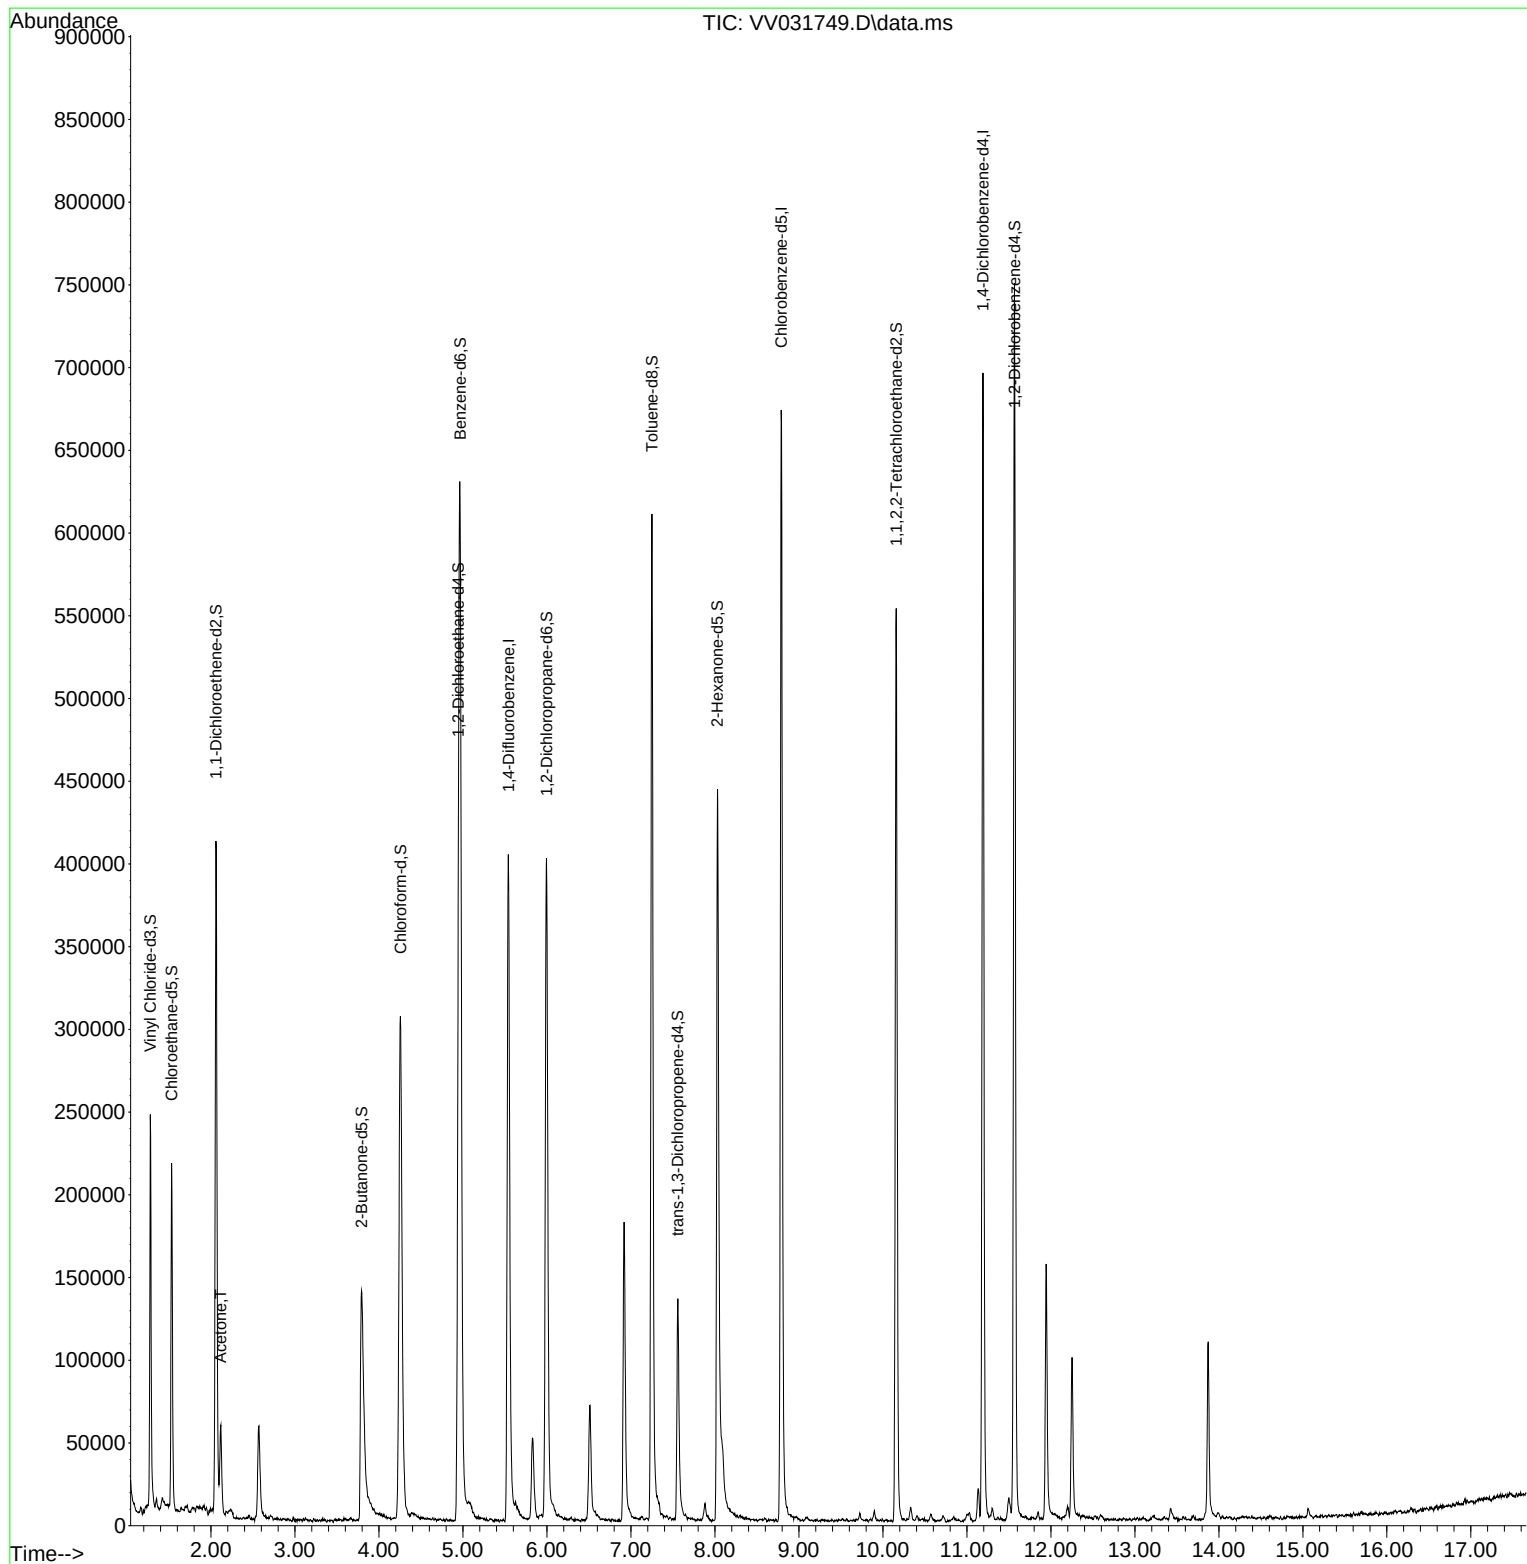

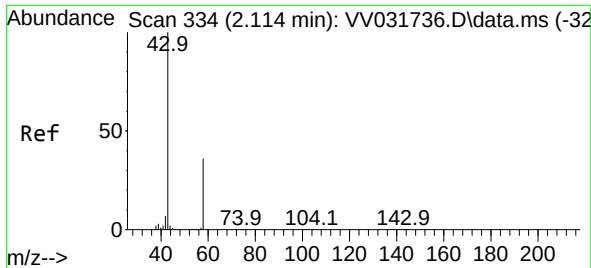

#13

Acetone

Concen: 21.092 ug/L

RT: 2.117 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV031749.D


Acq: 25 Jul 2023 18:25

Instrument :

MSVOA_V

ClientSampleId :

BH2Y5

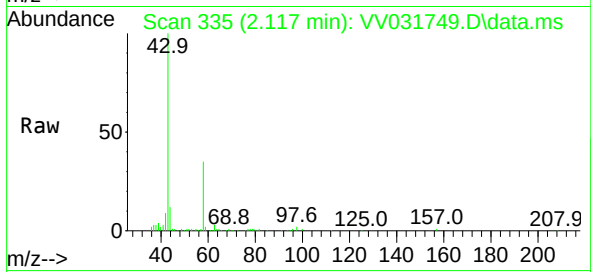

Tgt Ion: 43 Resp: 47786

Ion Ratio Lower Upper

43 100

58 34.4 0.0 72.0

