

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
 Data File : VV031744.D
 Acq On : 25 Jul 2023 16:27
 Operator : SY/MD
 Sample : 03712-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031744.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	175458	185974	13.79%	1.831%
2	1.532	147	153	168	rVB	166346	195560	14.50%	1.926%
3	2.059	309	317	329	rBV	305323	429671	31.86%	4.231%
4	3.040	620	622	625	rBV4	1265	819	0.06%	0.008%
5	3.378	725	727	731	rBV5	985	765	0.06%	0.008%
6	3.542	776	778	779	rBV2	789	241	0.02%	0.002%
7	3.619	797	802	804	rBV5	1285	1294	0.10%	0.013%
8	3.793	847	856	887	rBV	135370	396770	29.42%	3.907%
9	4.256	984	1000	1027	rBV2	249431	645665	47.88%	6.358%
10	4.693	1134	1136	1138	rBV3	1056	510	0.04%	0.005%
11	4.744	1150	1152	1154	rBV2	667	383	0.03%	0.004%
12	4.796	1164	1168	1172	rBV5	2092	2043	0.15%	0.020%
13	4.850	1182	1185	1187	rBV3	1400	964	0.07%	0.009%
14	4.883	1192	1195	1199	rVB3	533	495	0.04%	0.005%
15	4.902	1199	1201	1203	rBV2	844	517	0.04%	0.005%
16	4.963	1203	1220	1248	rBV2	500881	1348442	100.00%	13.279%
17	5.249	1307	1309	1312	rVB2	1032	460	0.03%	0.005%
18	5.329	1332	1334	1335	rBV	1070	563	0.04%	0.006%
19	5.445	1366	1370	1372	rBV4	840	638	0.05%	0.006%
20	5.490	1382	1384	1385	rBV2	618	258	0.02%	0.003%
21	5.542	1385	1400	1424	rBV	318615	679738	50.41%	6.694%
22	5.918	1514	1517	1522	rBV7	2551	2997	0.22%	0.030%
23	5.995	1529	1541	1561	rBV	313881	648865	48.12%	6.390%
24	6.284	1629	1631	1634	rBV2	1468	973	0.07%	0.010%
25	6.673	1750	1752	1754	rBV3	1118	576	0.04%	0.006%
26	6.709	1761	1763	1764	rBV	802	278	0.02%	0.003%
27	6.783	1784	1786	1788	rVB3	1195	487	0.04%	0.005%
28	6.796	1788	1790	1791	rBV2	740	267	0.02%	0.003%
29	6.918	1817	1828	1852	rBV	140662	273474	20.28%	2.693%
30	7.204	1915	1917	1919	rBV2	862	388	0.03%	0.004%
31	7.249	1920	1931	1960	rBV	456268	829854	61.54%	8.172%
32	7.561	2019	2028	2047	rBV	104708	186148	13.80%	1.833%
33	7.821	2107	2109	2110	rVB	626	240	0.02%	0.002%
34	7.834	2110	2113	2117	rBV5	1718	1682	0.12%	0.017%
35	7.979	2156	2158	2161	rBV3	714	368	0.03%	0.004%
36	8.030	2165	2174	2203	rBV	395579	811230	60.16%	7.989%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
 Data File : VV031744.D
 Acq On : 25 Jul 2023 16:27
 Operator : SY/MD
 Sample : 03712-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	8.792	2400	2411	2436	rBV	545259	923015	68.45%	9.089%
38	9.043	2485	2489	2490	rBV2	1246	787	0.06%	0.008%
39	9.188	2532	2534	2539	rVB3	1847	1215	0.09%	0.012%
40	9.294	2565	2567	2570	rBV3	762	410	0.03%	0.004%
41	9.313	2570	2573	2575	rVB2	1144	665	0.05%	0.007%
42	9.345	2581	2583	2586	rVB2	1107	486	0.04%	0.005%
43	9.361	2586	2588	2589	rBV	1131	553	0.04%	0.005%
44	9.390	2593	2597	2601	rBV4	1657	1515	0.11%	0.015%
45	9.464	2615	2620	2623	rBV7	1193	1287	0.10%	0.013%
46	9.493	2623	2629	2636	rBV6	2615	3056	0.23%	0.030%
47	9.683	2686	2688	2689	rBV2	978	338	0.03%	0.003%
48	9.760	2710	2712	2714	rBV2	464	236	0.02%	0.002%
49	9.773	2714	2716	2717	rBV2	807	378	0.03%	0.004%
50	9.943	2767	2769	2773	rVB5	980	565	0.04%	0.006%
51	9.992	2782	2784	2788	rVB4	1004	435	0.03%	0.004%
52	10.053	2801	2803	2808	rVB2	1077	653	0.05%	0.006%
53	10.088	2808	2814	2817	rBV5	1200	1354	0.10%	0.013%
54	10.159	2823	2836	2862	rBV	509249	808557	59.96%	7.962%
55	10.300	2878	2880	2881	rBV2	1372	589	0.04%	0.006%
56	10.950	3080	3082	3083	rBV	789	256	0.02%	0.003%
57	11.050	3111	3113	3114	rBV2	600	266	0.02%	0.003%
58	11.191	3146	3157	3176	rBV	541345	844542	62.63%	8.317%
59	11.567	3263	3274	3296	rVB	564502	896148	66.46%	8.825%
60	11.802	3344	3347	3349	rBV3	1144	705	0.05%	0.007%
61	12.255	3480	3488	3491	rBV6	3886	4986	0.37%	0.049%
62	12.300	3495	3502	3509	rVV6	4834	7927	0.59%	0.078%
63	12.384	3526	3528	3535	rBV7	1595	951	0.07%	0.009%
64	12.657	3611	3613	3615	rBV3	1171	494	0.04%	0.005%
65	12.721	3630	3633	3636	rBV3	1395	984	0.07%	0.010%
66	12.828	3663	3666	3670	rBV4	1739	1637	0.12%	0.016%
67	12.921	3694	3695	3696	rBV4	529	172	0.01%	0.002%




Sum of corrected areas: 10154759

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031744.D
Acq On : 25 Jul 2023 16:27
Operator : SY/MD
Sample : 03712-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

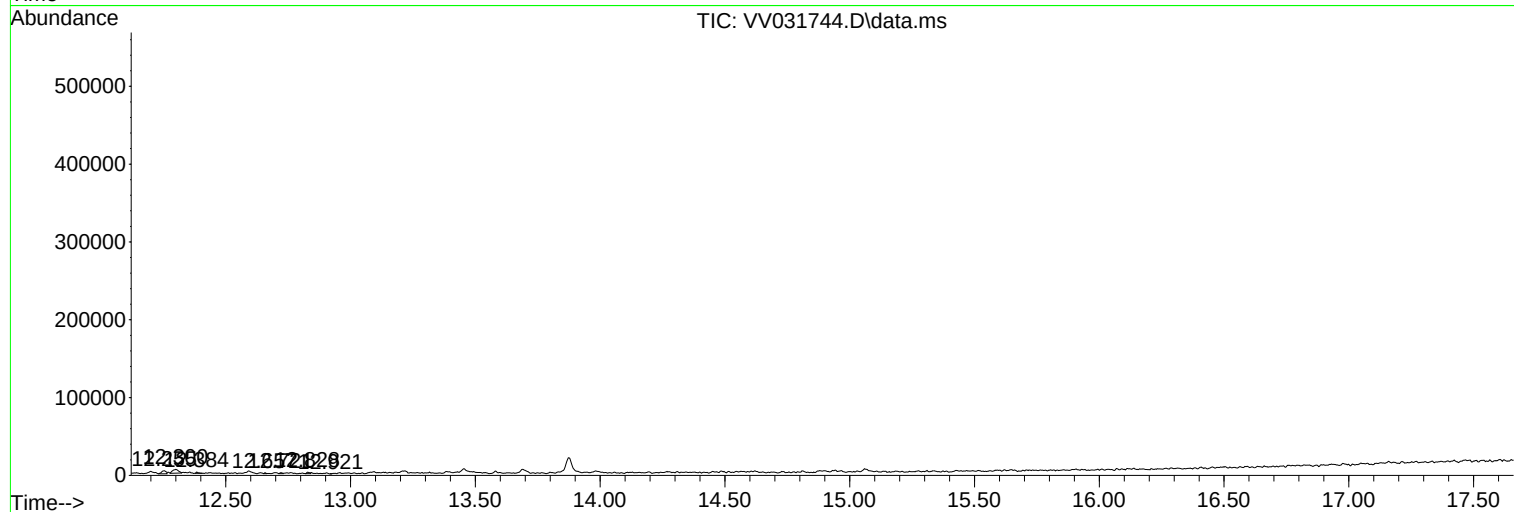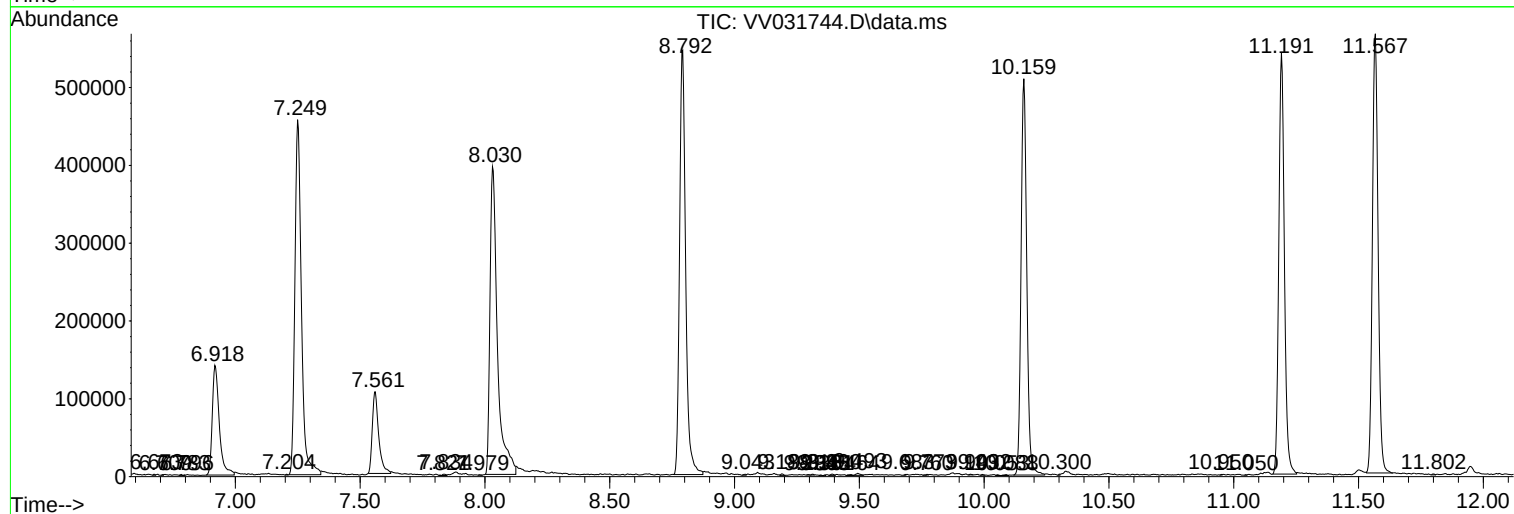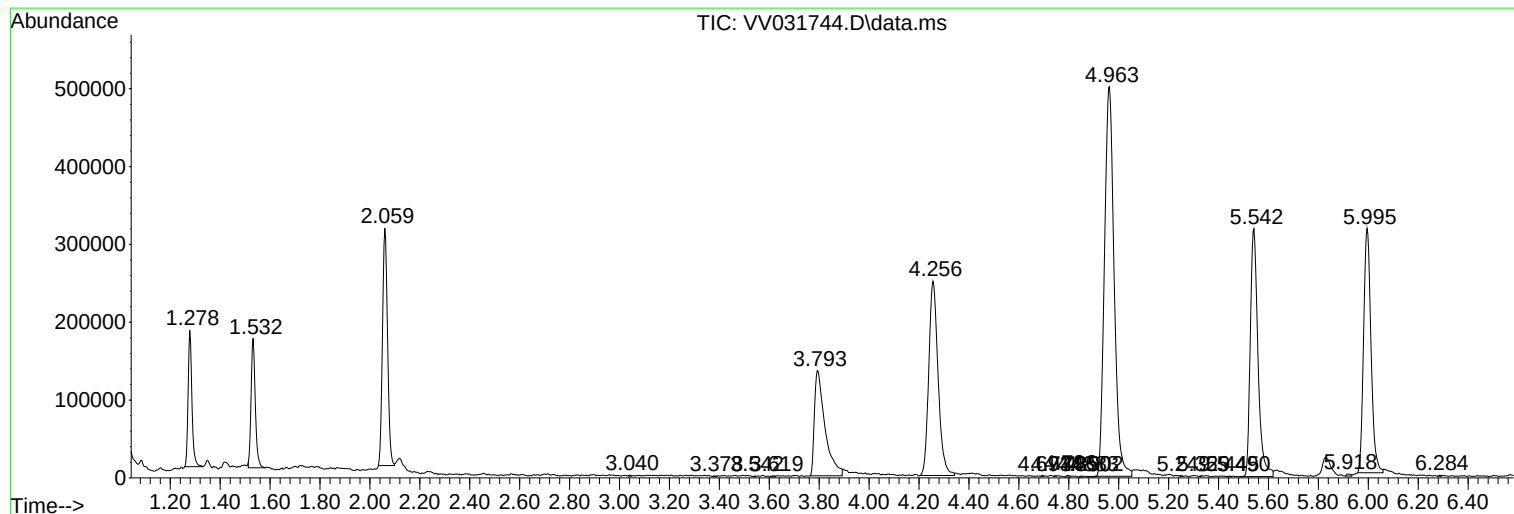

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031744.D
Acq On : 25 Jul 2023 16:27
Operator : SY/MD
Sample : 03712-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031744.D
Acq On : 25 Jul 2023 16:27
Operator : SY/MD
Sample : 03712-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------