

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
 Data File : VV031745.D
 Acq On : 25 Jul 2023 16:51
 Operator : SY/MD
 Sample : 03712-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031745.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	89	rVB	160189	178515	8.82%	1.499%
2	1.532	147	153	168	rVB	152641	188474	9.31%	1.583%
3	2.060	309	317	329	rBV	269367	382010	18.88%	3.209%
4	2.664	503	505	506	rBV2	1425	625	0.03%	0.005%
5	2.699	507	516	530	rVB	25986	46702	2.31%	0.392%
6	2.931	585	588	590	rBV2	1788	1132	0.06%	0.010%
7	2.944	590	592	595	rVB4	1382	510	0.03%	0.004%
8	2.963	596	598	602	rBV4	1547	875	0.04%	0.007%
9	3.195	668	670	674	rVB6	989	499	0.02%	0.004%
10	3.220	674	678	680	rBV4	1669	912	0.05%	0.008%
11	3.288	695	699	700	rBV4	1332	924	0.05%	0.008%
12	3.352	717	719	720	rBV	1197	547	0.03%	0.005%
13	3.513	765	769	772	rBV5	1703	1439	0.07%	0.012%
14	3.625	799	804	805	rBV4	1542	922	0.05%	0.008%
15	3.667	815	817	821	rBV5	1088	786	0.04%	0.007%
16	3.751	841	843	847	rBV5	950	450	0.02%	0.004%
17	3.818	847	864	893	rBV2	392560	1202527	59.43%	10.101%
18	4.256	986	1000	1029	rBV	209363	533707	26.38%	4.483%
19	4.722	1141	1145	1147	rBV4	1154	853	0.04%	0.007%
20	4.757	1153	1156	1157	rBV3	2217	1280	0.06%	0.011%
21	4.963	1203	1220	1248	rBV2	438184	1175789	58.11%	9.876%
22	5.371	1344	1347	1351	rBV7	1684	1490	0.07%	0.013%
23	5.481	1376	1381	1383	rVB5	1443	1198	0.06%	0.010%
24	5.542	1389	1400	1425	rBV	270458	570079	28.17%	4.788%
25	5.841	1480	1493	1511	rBV4	94579	217944	10.77%	1.831%
26	5.995	1530	1541	1561	rBV	283794	571799	28.26%	4.803%
27	6.394	1662	1665	1667	rBV3	1872	1286	0.06%	0.011%
28	6.567	1708	1719	1722	rBV8	2872	4696	0.23%	0.039%
29	6.686	1754	1756	1758	rBV2	1553	774	0.04%	0.007%
30	6.703	1758	1761	1765	rBV4	1770	1438	0.07%	0.012%
31	6.725	1765	1768	1771	rBV4	1367	1040	0.05%	0.009%
32	6.828	1796	1800	1804	rBV7	1222	1287	0.06%	0.011%
33	6.921	1819	1829	1855	rBV	117093	226797	11.21%	1.905%
34	7.204	1914	1917	1919	rBV4	2160	1070	0.05%	0.009%
35	7.249	1919	1931	1960	rBV	374437	702715	34.73%	5.903%
36	7.526	2015	2017	2019	rBV3	1683	1018	0.05%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072523\
 Data File : VW031745.D
 Acq On : 25 Jul 2023 16:51
 Operator : SY/MD
 Sample : 03712-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	7.561	2019	2028	2045	rVV	87672	164757	8.14%	1.384%
38	7.767	2090	2092	2095	rBV4	1202	711	0.04%	0.006%
39	7.911	2123	2137	2165	rBV	1166474	2023516	100.00%	16.997%
40	8.030	2165	2174	2191	rBV	376978	710600	35.12%	5.969%
41	8.677	2373	2375	2378	rBV3	1245	600	0.03%	0.005%
42	8.792	2400	2411	2430	rBV	457313	764049	37.76%	6.418%
43	9.217	2540	2543	2549	rBV5	1986	1843	0.09%	0.015%
44	9.262	2555	2557	2561	rBV3	1346	1060	0.05%	0.009%
45	9.329	2575	2578	2579	rBV2	1382	962	0.05%	0.008%
46	9.358	2585	2587	2590	rBV4	1453	792	0.04%	0.007%
47	9.416	2602	2605	2609	rBV5	1291	929	0.05%	0.008%
48	9.612	2660	2666	2669	rBV6	1793	1684	0.08%	0.014%
49	9.680	2684	2687	2690	rBV4	989	757	0.04%	0.006%
50	9.725	2696	2701	2702	rBV4	1659	1217	0.06%	0.010%
51	9.850	2738	2740	2743	rVB4	1658	855	0.04%	0.007%
52	9.876	2743	2748	2750	rBV6	2408	2169	0.11%	0.018%
53	9.963	2772	2775	2777	rBV5	1186	526	0.03%	0.004%
54	10.037	2795	2798	2801	rVB6	1437	931	0.05%	0.008%
55	10.159	2824	2836	2852	rBV	453841	723462	35.75%	6.077%
56	10.490	2933	2939	2948	rVB	2338	3165	0.16%	0.027%
57	10.654	2987	2990	2992	rBV3	1482	1028	0.05%	0.009%
58	10.757	3015	3022	3023	rVV6	1482	1285	0.06%	0.011%
59	10.789	3029	3032	3033	rBV3	980	448	0.02%	0.004%
60	10.850	3047	3051	3053	rBV4	1197	932	0.05%	0.008%
61	10.898	3062	3066	3069	rBV6	1833	1919	0.09%	0.016%
62	10.960	3083	3085	3087	rBV2	999	525	0.03%	0.004%
63	11.066	3116	3118	3122	rBV4	1152	649	0.03%	0.005%
64	11.098	3122	3128	3131	rBV7	1725	1515	0.07%	0.013%
65	11.191	3146	3157	3175	rBV	436501	682219	33.71%	5.730%
66	11.361	3208	3210	3215	rBV5	1879	1331	0.07%	0.011%
67	11.407	3220	3224	3225	rBV3	652	483	0.02%	0.004%
68	11.567	3263	3274	3290	rBV	463861	742141	36.68%	6.234%
69	11.841	3356	3359	3363	rBV6	1023	823	0.04%	0.007%
70	12.014	3408	3413	3416	rVV6	2362	1980	0.10%	0.017%
71	12.040	3419	3421	3428	rVV8	1069	1136	0.06%	0.010%
72	12.207	3467	3473	3477	rBV6	1547	2017	0.10%	0.017%
73	12.265	3485	3491	3496	rBV7	1395	1751	0.09%	0.015%
74	12.294	3498	3500	3501	rBV	1313	642	0.03%	0.005%
75	12.368	3520	3523	3528	rBV6	1558	1228	0.06%	0.010%
76	12.477	3555	3557	3558	rBV2	1204	513	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
 Data File : VV031745.D
 Acq On : 25 Jul 2023 16:51
 Operator : SY/MD
 Sample : 03712-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	12.561	3581	3583	3586	rBV3	875	619	0.03%	0.005%
78	12.583	3587	3590	3592	rBV4	2370	1790	0.09%	0.015%
79	12.644	3607	3609	3611	rBV3	976	607	0.03%	0.005%
80	12.715	3629	3631	3633	rBV3	1780	780	0.04%	0.007%
81	12.760	3643	3645	3648	rVB4	1702	840	0.04%	0.007%
82	12.776	3648	3650	3655	rVB5	1697	1047	0.05%	0.009%
83	12.802	3655	3658	3663	rBV5	1085	694	0.03%	0.006%
84	12.905	3688	3690	3693	rVB3	1663	867	0.04%	0.007%
85	12.956	3703	3706	3709	rBV4	837	705	0.03%	0.006%
86	13.062	3734	3739	3740	rBV4	1485	1182	0.06%	0.010%
87	13.095	3748	3749	3756	rVB6	1048	931	0.05%	0.008%
88	13.175	3770	3774	3776	rBV3	1625	1019	0.05%	0.009%
89	13.287	3805	3809	3811	rBV4	851	543	0.03%	0.005%
90	13.310	3811	3816	3817	rBV3	1995	1326	0.07%	0.011%
91	13.448	3856	3859	3862	rBV4	2491	2059	0.10%	0.017%
92	13.509	3874	3878	3880	rBV4	1482	1355	0.07%	0.011%
93	13.561	3889	3894	3898	rVB7	1214	1209	0.06%	0.010%
94	13.686	3929	3933	3935	rBV4	4231	3608	0.18%	0.030%
95	13.831	3973	3978	3980	rBV3	1344	1158	0.06%	0.010%
96	13.876	3988	3992	3997	rBV6	4789	4434	0.22%	0.037%
97	13.943	4010	4013	4015	rBV3	1338	957	0.05%	0.008%
98	14.030	4037	4040	4041	rBV2	1001	571	0.03%	0.005%
99	14.095	4055	4060	4062	rBV5	1987	1915	0.09%	0.016%
100	14.349	4135	4139	4142	rBV5	2233	1812	0.09%	0.015%




Sum of corrected areas: 11905287

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031745.D
Acq On : 25 Jul 2023 16:51
Operator : SY/MD
Sample : 03712-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

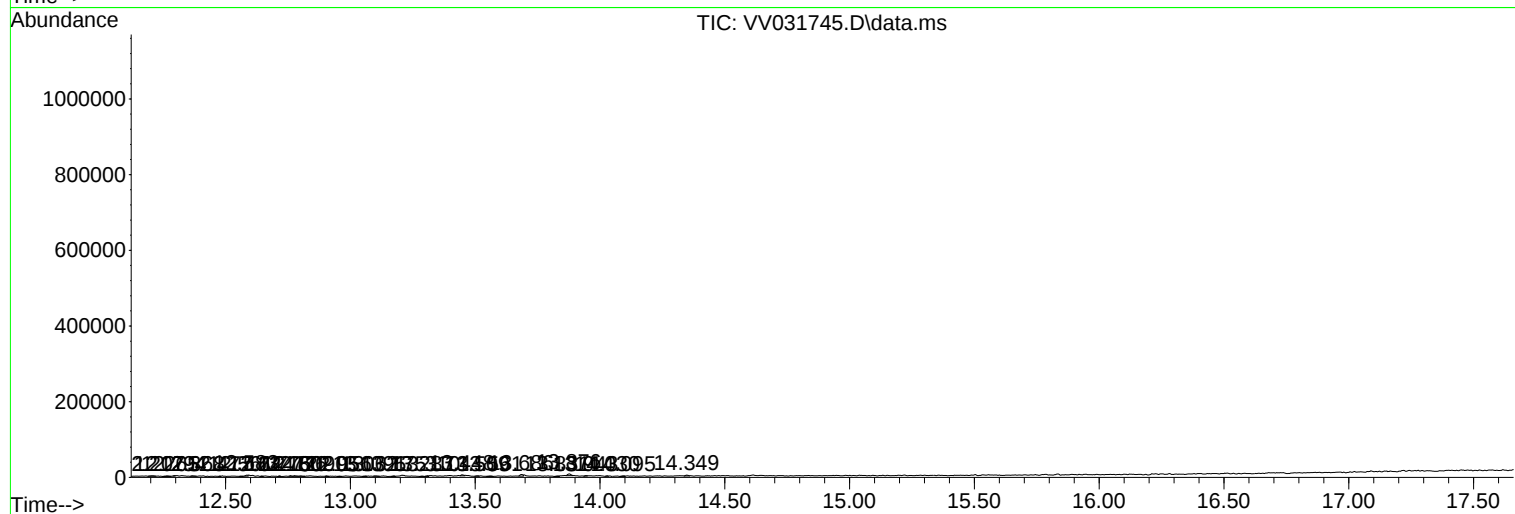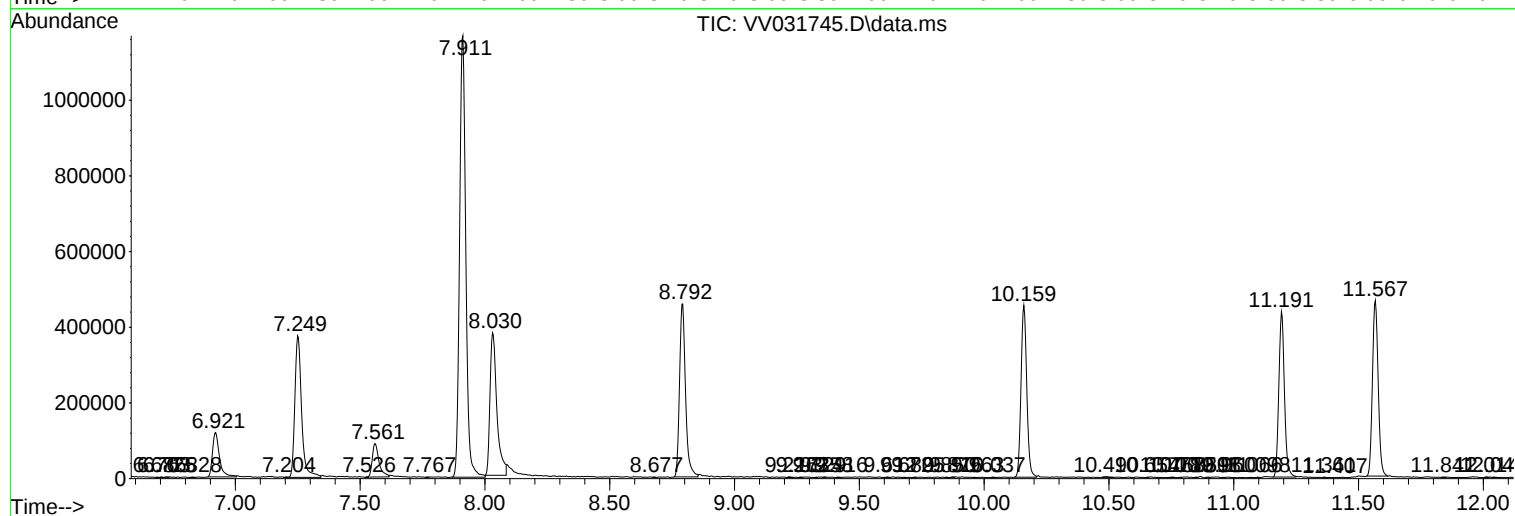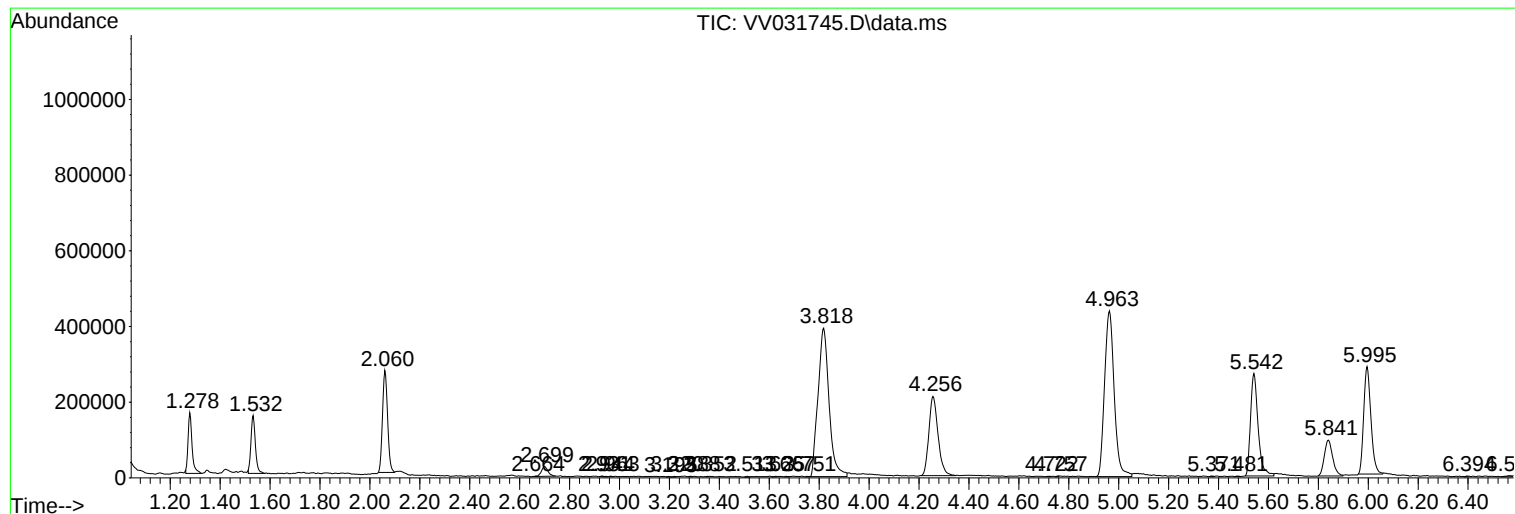

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031745.D
Acq On : 25 Jul 2023 16:51
Operator : SY/MD
Sample : 03712-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031745.D
Acq On : 25 Jul 2023 16:51
Operator : SY/MD
Sample : 03712-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------