

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
 Data File : VV031746.D
 Acq On : 25 Jul 2023 17:15
 Operator : SY/MD
 Sample : 03712-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	239014	255230	15.29%	2.059%
2	1.532	146	153	170	rVB	208689	255906	15.33%	2.064%
3	2.060	308	317	330	rBV	389480	567248	33.98%	4.575%
4	2.658	501	503	504	rBV	1093	407	0.02%	0.003%
5	2.700	513	516	521	rBV6	1795	1781	0.11%	0.014%
6	2.757	532	534	536	rBV	705	333	0.02%	0.003%
7	2.793	544	545	547	rBV2	562	246	0.01%	0.002%
8	2.812	547	551	554	rVV4	1418	1324	0.08%	0.011%
9	2.870	566	569	571	rBV3	1131	629	0.04%	0.005%
10	2.963	596	598	601	rBV3	1281	751	0.04%	0.006%
11	3.011	611	613	615	rBV2	704	367	0.02%	0.003%
12	3.037	618	621	623	rBV3	1078	567	0.03%	0.005%
13	3.111	642	644	646	rBV3	791	358	0.02%	0.003%
14	3.124	646	648	650	rVV3	766	394	0.02%	0.003%
15	3.172	662	663	665	rVB	933	345	0.02%	0.003%
16	3.185	665	667	669	rBV3	815	405	0.02%	0.003%
17	3.298	698	702	705	rBV4	675	658	0.04%	0.005%
18	3.365	720	723	726	rBV3	1212	892	0.05%	0.007%
19	3.465	752	754	757	rBV3	720	508	0.03%	0.004%
20	3.484	757	760	769	rVB6	844	1288	0.08%	0.010%
21	3.523	769	772	773	rBV3	788	261	0.02%	0.002%
22	3.532	773	775	779	rBV3	593	452	0.03%	0.004%
23	3.571	784	787	791	rBV4	1035	754	0.05%	0.006%
24	3.590	791	793	796	rVB3	829	365	0.02%	0.003%
25	3.613	796	800	802	rBV5	996	750	0.04%	0.006%
26	3.648	808	811	814	rBV3	857	523	0.03%	0.004%
27	3.687	821	823	826	rBV3	652	319	0.02%	0.003%
28	3.712	829	831	835	rVB2	929	524	0.03%	0.004%
29	3.728	835	836	837	rBV	678	228	0.01%	0.002%
30	3.796	846	857	888	rBV	138382	411459	24.65%	3.319%
31	4.256	984	1000	1031	rBV	294065	766333	45.91%	6.181%
32	4.651	1121	1123	1127	rVB5	1858	870	0.05%	0.007%
33	4.706	1138	1140	1144	rBV5	1037	659	0.04%	0.005%
34	4.728	1144	1147	1149	rBV2	1372	924	0.06%	0.007%
35	4.777	1160	1162	1164	rBV2	945	297	0.02%	0.002%
36	4.828	1174	1178	1180	rBV4	698	601	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072523\
 Data File : VW031746.D
 Acq On : 25 Jul 2023 17:15
 Operator : SY/MD
 Sample : 03712-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	4.963	1201	1220	1246	rBV2	619361	1669146	100.00%	13.463%
38	5.269	1313	1315	1316	rBV2	1342	612	0.04%	0.005%
39	5.410	1357	1359	1362	rBV4	1128	795	0.05%	0.006%
40	5.542	1388	1400	1426	rBV	393294	834517	50.00%	6.731%
41	5.995	1528	1541	1564	rBV	398662	830230	49.74%	6.696%
42	6.365	1651	1656	1658	rBV4	1580	1412	0.08%	0.011%
43	6.510	1699	1701	1704	rBV4	1012	610	0.04%	0.005%
44	6.680	1752	1754	1760	rVB5	1584	1317	0.08%	0.011%
45	6.706	1760	1762	1767	rBV5	1172	952	0.06%	0.008%
46	6.728	1767	1769	1771	rVV2	794	313	0.02%	0.003%
47	6.767	1779	1781	1782	rBV2	947	462	0.03%	0.004%
48	6.796	1788	1790	1792	rVB	959	439	0.03%	0.004%
49	6.812	1792	1795	1796	rBV2	1076	546	0.03%	0.004%
50	6.844	1802	1805	1810	rBV6	778	553	0.03%	0.004%
51	6.918	1818	1828	1856	rBV	166594	327477	19.62%	2.641%
52	7.249	1919	1931	1966	rBV	586507	1078922	64.64%	8.702%
53	7.558	2018	2027	2050	rBV	129424	239754	14.36%	1.934%
54	7.860	2119	2121	2123	rBV2	1208	636	0.04%	0.005%
55	8.031	2164	2174	2206	rBV	442358	894047	53.56%	7.211%
56	8.497	2317	2319	2322	rBV3	1134	499	0.03%	0.004%
57	8.545	2327	2334	2335	rBV8	1326	1377	0.08%	0.011%
58	8.670	2370	2373	2376	rBV4	1594	1151	0.07%	0.009%
59	8.789	2399	2410	2438	rBV	663885	1115467	66.83%	8.997%
60	9.140	2517	2519	2523	rVB3	1469	908	0.05%	0.007%
61	9.182	2530	2532	2535	rVB4	1198	523	0.03%	0.004%
62	9.204	2535	2539	2541	rBV4	1496	919	0.06%	0.007%
63	9.284	2561	2564	2565	rBV3	1313	718	0.04%	0.006%
64	9.362	2586	2588	2591	rBV4	1121	755	0.05%	0.006%
65	9.442	2610	2613	2614	rBV2	969	536	0.03%	0.004%
66	9.603	2660	2663	2664	rBV3	551	241	0.01%	0.002%
67	9.612	2664	2666	2669	rVV2	709	369	0.02%	0.003%
68	9.629	2669	2671	2675	rVB4	1297	838	0.05%	0.007%
69	9.654	2675	2679	2681	rBV4	843	663	0.04%	0.005%
70	9.667	2681	2683	2684	rBV2	853	352	0.02%	0.003%
71	9.728	2700	2702	2704	rBV2	772	427	0.03%	0.003%
72	9.847	2731	2739	2752	rBV4	10237	15284	0.92%	0.123%
73	9.947	2766	2770	2772	rBV2	1033	783	0.05%	0.006%
74	9.982	2776	2781	2785	rBV6	1438	1639	0.10%	0.013%
75	10.159	2824	2836	2862	rBV	586869	943789	56.54%	7.612%
76	10.297	2878	2879	2881	rBV2	703	305	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072523\
 Data File : VW031746.D
 Acq On : 25 Jul 2023 17:15
 Operator : SY/MD
 Sample : 03712-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	10.368	2898	2901	2903	rBV4	923	585	0.04%	0.005%
78	10.606	2973	2975	2979	rBV4	1188	874	0.05%	0.007%
79	10.683	2997	2999	3002	rVB3	1014	488	0.03%	0.004%
80	10.706	3004	3006	3008	rVV3	753	295	0.02%	0.002%
81	10.796	3031	3034	3036	rBV4	959	622	0.04%	0.005%
82	10.837	3042	3047	3048	rBV3	608	473	0.03%	0.004%
83	10.969	3086	3088	3092	rBV3	1028	863	0.05%	0.007%
84	11.037	3107	3109	3113	rVB4	1188	749	0.04%	0.006%
85	11.059	3113	3116	3117	rBV2	1155	706	0.04%	0.006%
86	11.127	3133	3137	3141	rBV6	2187	2264	0.14%	0.018%
87	11.191	3146	3157	3179	rVV	659077	1013894	60.74%	8.178%
88	11.567	3263	3274	3293	rVB	711607	1122836	67.27%	9.056%
89	11.873	3367	3369	3372	rBV3	1210	845	0.05%	0.007%
90	12.136	3448	3451	3456	rBV2	1243	1353	0.08%	0.011%
91	12.188	3463	3467	3469	rBV4	1912	1532	0.09%	0.012%
92	12.387	3527	3529	3533	rVB2	1475	721	0.04%	0.006%
93	12.445	3545	3547	3551	rVB4	1052	449	0.03%	0.004%
94	12.583	3588	3590	3591	rBV2	1536	626	0.04%	0.005%
95	12.702	3625	3627	3631	rVB4	1158	484	0.03%	0.004%
96	12.818	3659	3663	3664	rBV4	1752	1041	0.06%	0.008%
97	13.043	3731	3733	3734	rBV2	781	399	0.02%	0.003%
98	13.066	3737	3740	3742	rBV2	1176	670	0.04%	0.005%
99	13.361	3831	3832	3833	rBV	710	236	0.01%	0.002%




Sum of corrected areas: 12398244

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031746.D
Acq On : 25 Jul 2023 17:15
Operator : SY/MD
Sample : 03712-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

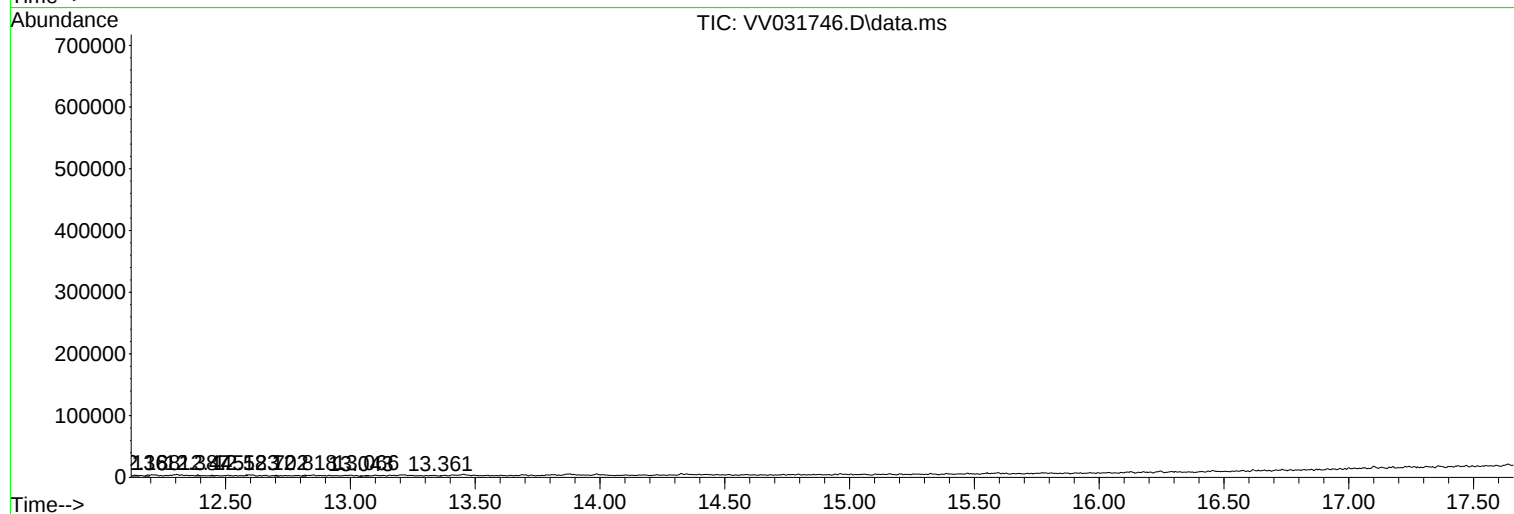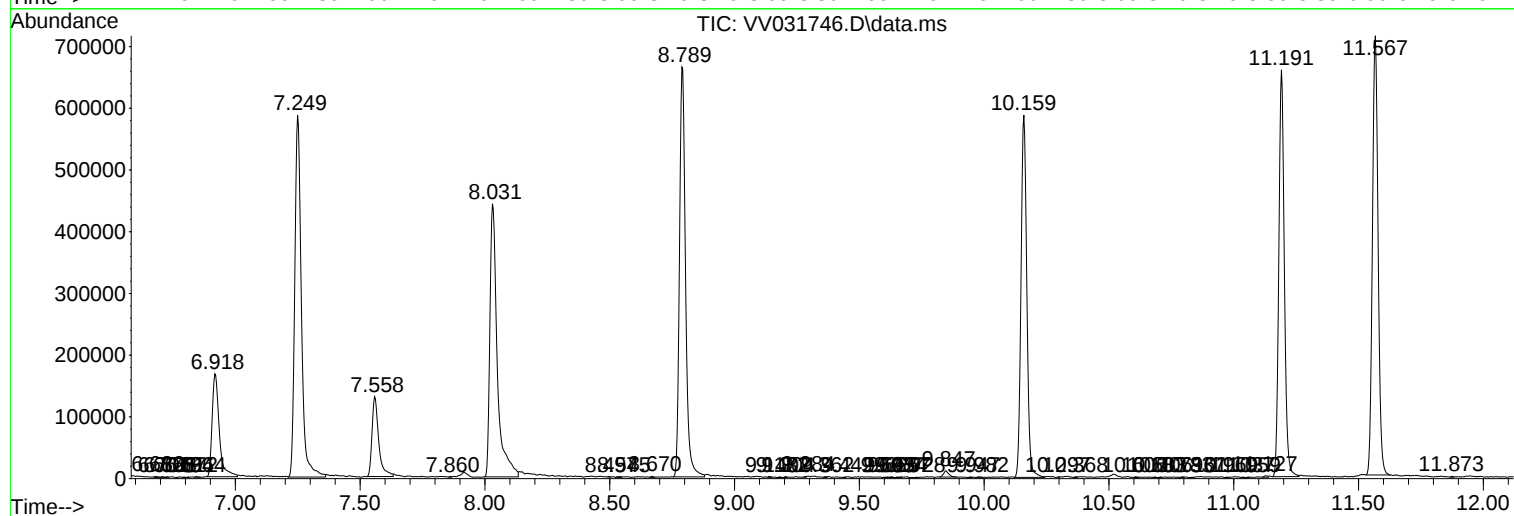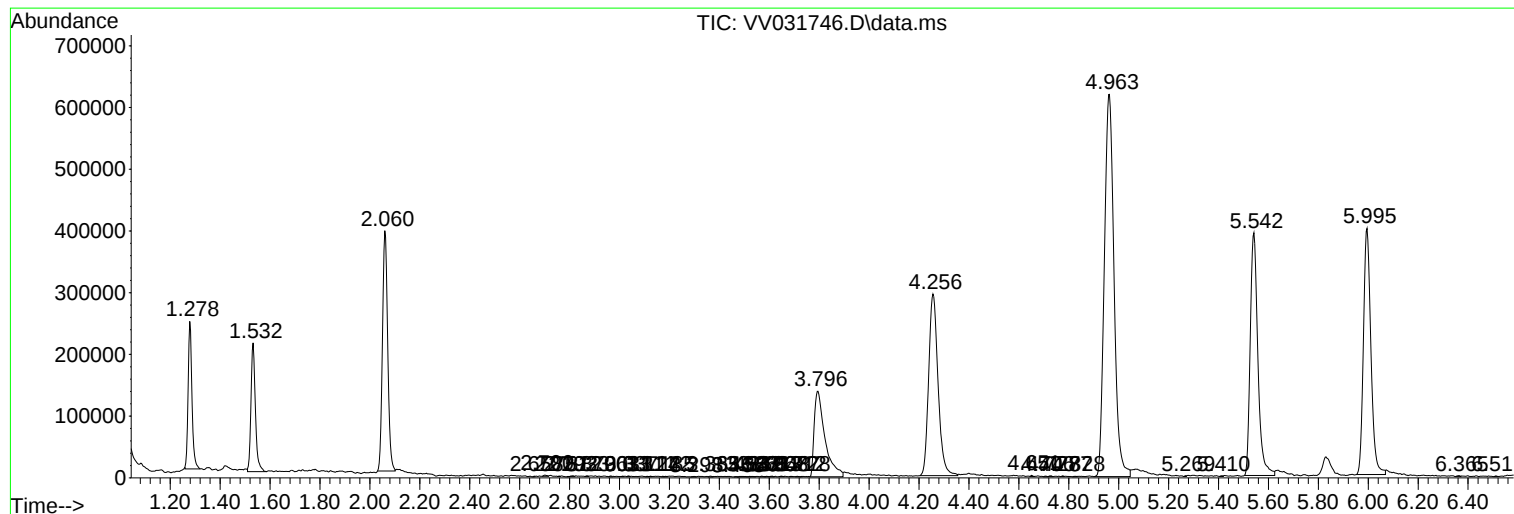

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031746.D
Acq On : 25 Jul 2023 17:15
Operator : SY/MD
Sample : 03712-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031746.D
Acq On : 25 Jul 2023 17:15
Operator : SY/MD
Sample : 03712-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------