

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
 Data File : VV031748.D
 Acq On : 25 Jul 2023 18:02
 Operator : SY/MD
 Sample : 03712-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031748.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	225454	247268	15.69%	2.050%
2	1.532	147	153	170	rVB	211213	253212	16.07%	2.099%
3	2.060	309	317	332	rBV	386832	555662	35.26%	4.607%
4	2.841	558	560	561	rBV2	1661	668	0.04%	0.006%
5	2.986	602	605	610	rVB5	1668	1234	0.08%	0.010%
6	3.333	708	713	715	rBV6	1770	1405	0.09%	0.012%
7	3.429	737	743	745	rBV8	2053	1926	0.12%	0.016%
8	3.461	751	753	757	rBV5	1647	1158	0.07%	0.010%
9	3.551	779	781	786	rVB7	1429	839	0.05%	0.007%
10	3.648	808	811	816	rVB6	2604	2049	0.13%	0.017%
11	3.670	816	818	824	rBV4	1174	986	0.06%	0.008%
12	3.793	846	856	887	rBV	136944	390942	24.81%	3.241%
13	4.256	987	1000	1026	rVB	276517	708601	44.96%	5.875%
14	4.722	1144	1145	1147	rBV2	1068	560	0.04%	0.005%
15	4.809	1165	1172	1174	rBV7	1761	1987	0.13%	0.016%
16	4.844	1181	1183	1185	rBV3	1213	607	0.04%	0.005%
17	4.879	1191	1194	1196	rBV4	1849	1181	0.07%	0.010%
18	4.963	1202	1220	1244	rBV2	578879	1575942	100.00%	13.066%
19	5.278	1316	1318	1320	rBV3	1239	781	0.05%	0.006%
20	5.313	1325	1329	1330	rBV3	872	628	0.04%	0.005%
21	5.326	1330	1333	1335	rBV4	1995	1220	0.08%	0.010%
22	5.407	1356	1358	1362	rBV4	1516	846	0.05%	0.007%
23	5.465	1371	1376	1377	rBV3	1289	1286	0.08%	0.011%
24	5.542	1388	1400	1422	rBV	393953	837555	53.15%	6.944%
25	5.995	1530	1541	1561	rVB	387541	783637	49.72%	6.497%
26	6.310	1636	1639	1641	rBV4	1919	1370	0.09%	0.011%
27	6.555	1712	1715	1716	rBV3	2254	1387	0.09%	0.011%
28	6.661	1743	1748	1753	rBV8	2125	1968	0.12%	0.016%
29	6.741	1771	1773	1780	rVB7	1719	1422	0.09%	0.012%
30	6.825	1797	1799	1802	rBV3	1398	887	0.06%	0.007%
31	6.918	1818	1828	1853	rBV2	158059	314570	19.96%	2.608%
32	7.249	1919	1931	1958	rBV	565904	1022820	64.90%	8.480%
33	7.558	2018	2027	2049	rBV2	125719	229520	14.56%	1.903%
34	7.844	2113	2116	2117	rBV2	904	643	0.04%	0.005%
35	8.030	2164	2174	2205	rBV	429867	856824	54.37%	7.104%
36	8.490	2313	2317	2321	rBV5	2086	2112	0.13%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
 Data File : VV031748.D
 Acq On : 25 Jul 2023 18:02
 Operator : SY/MD
 Sample : 03712-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	8.789	2398	2410	2437	rBV	672584	1149873	72.96%	9.533%
38	9.294	2562	2567	2570	rBV5	1542	1692	0.11%	0.014%
39	9.455	2613	2617	2618	rBV3	1085	647	0.04%	0.005%
40	9.513	2633	2635	2640	rVB5	961	711	0.05%	0.006%
41	9.558	2648	2649	2653	rBV4	618	334	0.02%	0.003%
42	9.590	2657	2659	2662	rVB3	1025	463	0.03%	0.004%
43	9.616	2665	2667	2670	rBV4	1091	896	0.06%	0.007%
44	9.673	2683	2685	2687	rBV3	415	240	0.02%	0.002%
45	9.696	2690	2692	2694	rVB2	527	227	0.01%	0.002%
46	9.728	2700	2702	2705	rBV4	590	398	0.03%	0.003%
47	9.792	2720	2722	2725	rVB3	1305	686	0.04%	0.006%
48	9.818	2725	2730	2737	rVB9	1294	1593	0.10%	0.013%
49	9.847	2737	2739	2741	rBV3	1105	580	0.04%	0.005%
50	9.989	2781	2783	2784	rBV2	423	203	0.01%	0.002%
51	10.024	2788	2794	2796	rBV6	1278	1198	0.08%	0.010%
52	10.098	2815	2817	2818	rBV2	1317	664	0.04%	0.006%
53	10.159	2824	2836	2857	rBV	574396	919807	58.37%	7.626%
54	10.255	2864	2866	2869	rBV3	1619	1285	0.08%	0.011%
55	10.333	2884	2890	2896	rVB5	10445	13019	0.83%	0.108%
56	10.432	2917	2921	2923	rBV4	917	740	0.05%	0.006%
57	10.455	2925	2928	2931	rBV3	1040	780	0.05%	0.006%
58	10.564	2960	2962	2964	rVB2	751	251	0.02%	0.002%
59	10.580	2964	2967	2971	rBV5	835	623	0.04%	0.005%
60	10.680	2996	2998	3001	rBV3	773	428	0.03%	0.004%
61	10.738	3014	3016	3019	rVB5	1183	642	0.04%	0.005%
62	10.757	3019	3022	3023	rBV2	828	520	0.03%	0.004%
63	10.834	3042	3046	3049	rVB4	1172	964	0.06%	0.008%
64	10.857	3049	3053	3055	rBV4	1666	1336	0.08%	0.011%
65	10.905	3064	3068	3069	rBV2	1693	1236	0.08%	0.010%
66	10.966	3086	3087	3089	rBV2	1202	641	0.04%	0.005%
67	10.998	3093	3097	3098	rVV3	950	533	0.03%	0.004%
68	11.069	3117	3119	3121	rVB3	1045	332	0.02%	0.003%
69	11.191	3146	3157	3179	rBV	631842	994711	63.12%	8.247%
70	11.497	3241	3252	3263	rBV5	19117	44234	2.81%	0.367%
71	11.567	3263	3274	3292	rVB	694552	1091190	69.24%	9.047%
72	12.040	3419	3421	3426	rVB4	2104	1842	0.12%	0.015%
73	12.062	3426	3428	3430	rBV3	974	422	0.03%	0.003%
74	12.075	3430	3432	3435	rBV4	1038	628	0.04%	0.005%
75	12.152	3451	3456	3457	rBV5	1494	1269	0.08%	0.011%
76	12.204	3463	3472	3478	rBV3	5523	9137	0.58%	0.076%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
 Data File : VV031748.D
 Acq On : 25 Jul 2023 18:02
 Operator : SY/MD
 Sample : 03712-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	12.487	3558	3560	3562	rBV3	1098	462	0.03%	0.004%
78	12.558	3580	3582	3584	rBV3	1233	538	0.03%	0.004%
79	12.574	3585	3587	3589	rBV3	1529	764	0.05%	0.006%
80	12.696	3623	3625	3626	rBV2	1473	653	0.04%	0.005%
81	12.931	3692	3698	3700	rBV6	1290	1300	0.08%	0.011%
82	12.982	3709	3714	3717	rBV6	2308	2342	0.15%	0.019%
83	13.490	3870	3872	3873	rBV2	566	218	0.01%	0.002%
84	13.586	3898	3902	3905	rBV5	1544	1340	0.09%	0.011%
85	13.876	3990	3992	3994	rBV3	1324	670	0.04%	0.006%
86	14.175	4083	4085	4088	rBV3	1386	725	0.05%	0.006%




Sum of corrected areas: 12061690

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031748.D
Acq On : 25 Jul 2023 18:02
Operator : SY/MD
Sample : 03712-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2X2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

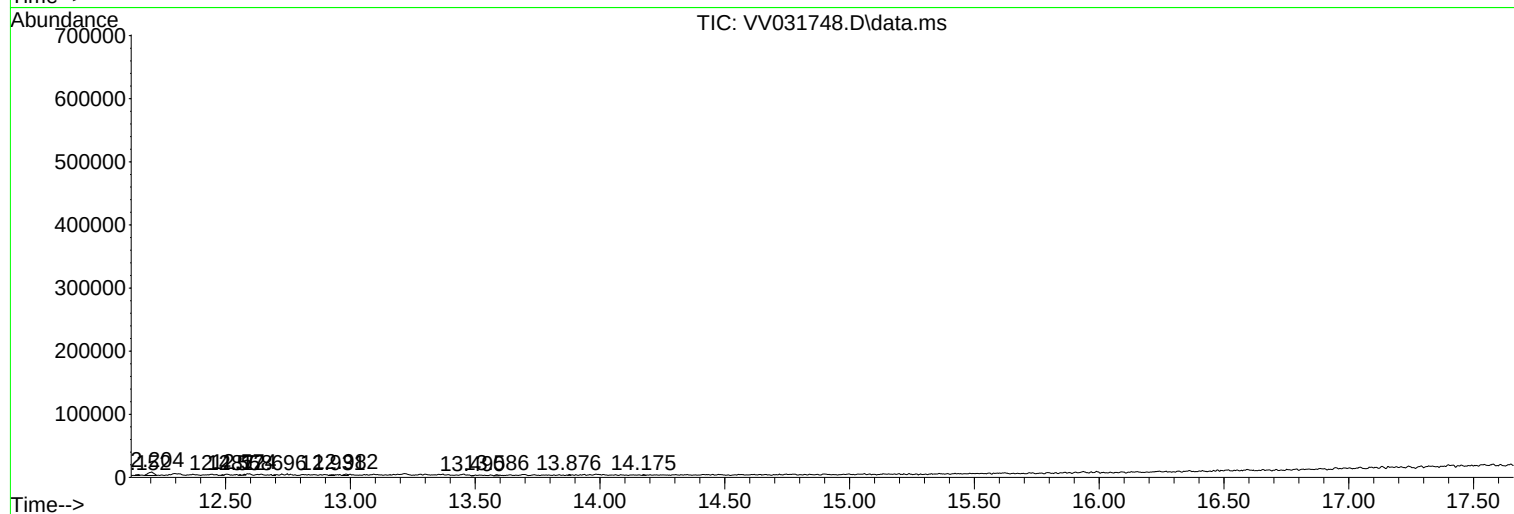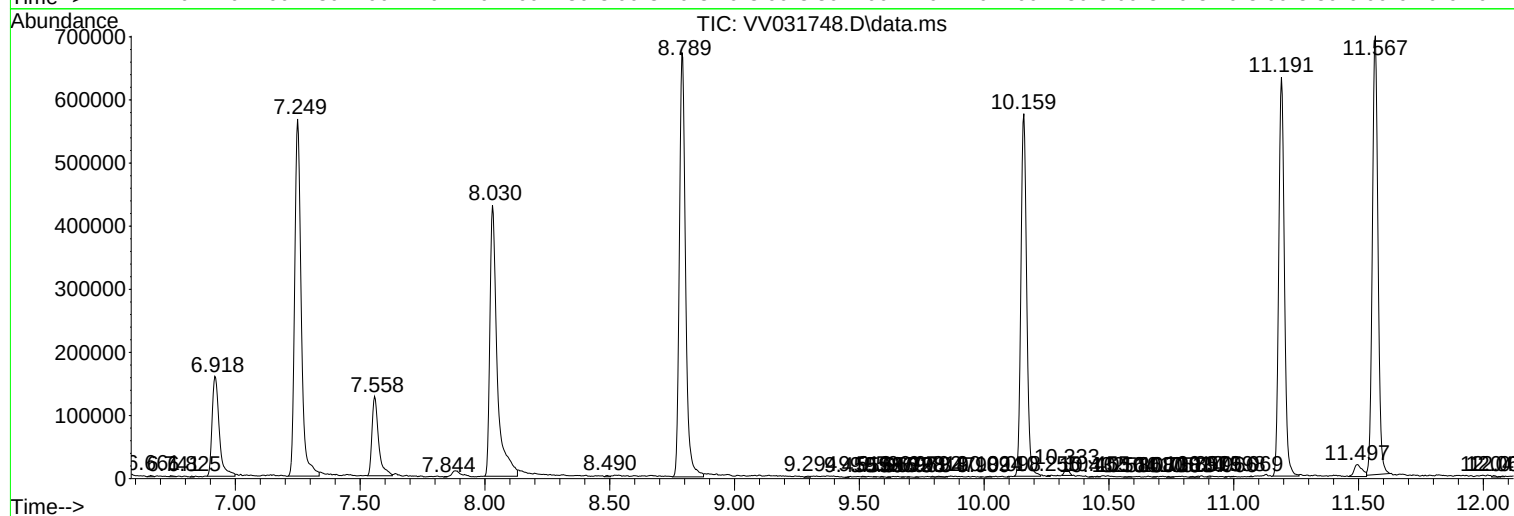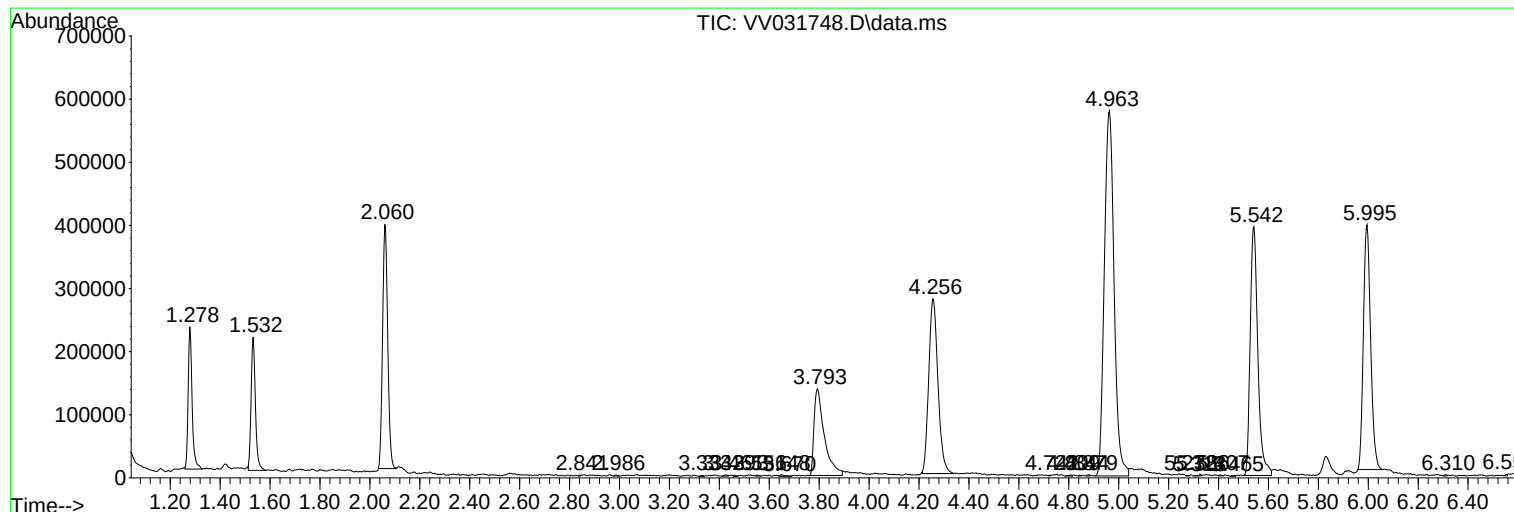

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031748.D
Acq On : 25 Jul 2023 18:02
Operator : SY/MD
Sample : 03712-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2X2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031748.D
Acq On : 25 Jul 2023 18:02
Operator : SY/MD
Sample : 03712-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2X2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------