

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
 Data File : VV031752.D
 Acq On : 25 Jul 2023 19:36
 Operator : SY/MD
 Sample : 03712-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	219555	235482	14.34%	1.904%
2	1.532	146	153	171	rVB	211502	255489	15.56%	2.066%
3	2.060	307	317	330	rBV	359195	549184	33.45%	4.441%
4	2.429	427	432	433	rBV3	1136	883	0.05%	0.007%
5	2.442	434	436	447	rVB9	2243	3104	0.19%	0.025%
6	2.558	468	472	474	rVV5	2314	1999	0.12%	0.016%
7	2.571	474	476	483	rVV6	2776	2059	0.13%	0.017%
8	2.658	498	503	509	rVB3	1231	1316	0.08%	0.011%
9	2.696	509	515	517	rBV4	1165	1107	0.07%	0.009%
10	2.770	534	538	540	rBV3	1094	834	0.05%	0.007%
11	2.790	540	544	548	rVB2	1142	1061	0.06%	0.009%
12	2.809	548	550	552	rBV2	1132	610	0.04%	0.005%
13	2.899	573	578	584	rBV6	1342	1467	0.09%	0.012%
14	2.970	595	600	603	rBV3	1126	1135	0.07%	0.009%
15	3.034	616	620	623	rVB2	1115	885	0.05%	0.007%
16	3.137	649	652	664	rVV6	2182	2351	0.14%	0.019%
17	3.397	730	733	738	rVB3	1478	1240	0.08%	0.010%
18	3.529	763	774	778	rBV3	2549	4756	0.29%	0.038%
19	3.600	793	796	798	rBV3	1173	694	0.04%	0.006%
20	3.658	807	814	816	rBV7	1160	1355	0.08%	0.011%
21	3.735	834	838	841	rBV4	2141	1851	0.11%	0.015%
22	3.790	845	855	889	rBV	147509	415173	25.29%	3.357%
23	4.163	968	971	972	rBV3	1869	1166	0.07%	0.009%
24	4.256	984	1000	1028	rBV	296628	766648	46.70%	6.200%
25	4.606	1104	1109	1113	rBV6	1450	1420	0.09%	0.011%
26	4.687	1132	1134	1138	rBV3	1076	851	0.05%	0.007%
27	4.728	1145	1147	1150	rBV5	1218	716	0.04%	0.006%
28	4.896	1196	1199	1201	rBV2	1464	833	0.05%	0.007%
29	4.963	1203	1220	1244	rBV2	615724	1641651	100.00%	13.276%
30	5.256	1309	1311	1313	rVB3	1420	662	0.04%	0.005%
31	5.278	1313	1318	1320	rVB3	1108	712	0.04%	0.006%
32	5.478	1377	1380	1387	rBV7	1793	1871	0.11%	0.015%
33	5.542	1387	1400	1424	rBV	401845	845747	51.52%	6.839%
34	5.828	1479	1489	1506	rBV2	33131	73093	4.45%	0.591%
35	5.931	1519	1521	1524	rVV4	2223	1472	0.09%	0.012%
36	5.995	1528	1541	1560	rVV	379995	795316	48.45%	6.432%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072523\
 Data File : VW031752.D
 Acq On : 25 Jul 2023 19:36
 Operator : SY/MD
 Sample : 03712-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	6.310	1634	1639	1640	rBV5	1707	1574	0.10%	0.013%
38	6.362	1653	1655	1658	rVB3	1462	768	0.05%	0.006%
39	6.455	1682	1684	1687	rVB3	1700	963	0.06%	0.008%
40	6.545	1709	1712	1713	rBV	1789	978	0.06%	0.008%
41	6.725	1763	1768	1772	rBV6	1986	2059	0.13%	0.017%
42	6.806	1785	1793	1797	rBV6	2481	3550	0.22%	0.029%
43	6.825	1797	1799	1807	rVB6	1986	2097	0.13%	0.017%
44	6.918	1817	1828	1847	rBV	159440	314663	19.17%	2.545%
45	7.249	1917	1931	1956	rBV	569862	1030450	62.77%	8.333%
46	7.558	2018	2027	2043	rBV	125522	224101	13.65%	1.812%
47	7.722	2075	2078	2080	rVB2	1244	672	0.04%	0.005%
48	7.812	2103	2106	2109	rBV4	1346	870	0.05%	0.007%
49	7.863	2119	2122	2124	rBV4	1448	1067	0.06%	0.009%
50	7.879	2124	2127	2128	rBV3	1910	1106	0.07%	0.009%
51	7.941	2145	2146	2150	rVB4	1443	749	0.05%	0.006%
52	8.031	2164	2174	2217	rBV	427332	876047	53.36%	7.084%
53	8.371	2278	2280	2284	rBV5	1290	845	0.05%	0.007%
54	8.391	2284	2286	2288	rBV3	1111	663	0.04%	0.005%
55	8.423	2293	2296	2300	rBV5	1176	959	0.06%	0.008%
56	8.461	2305	2308	2311	rVB4	1220	924	0.06%	0.007%
57	8.529	2325	2329	2332	rVB4	1469	1272	0.08%	0.010%
58	8.568	2336	2341	2343	rBV6	1137	844	0.05%	0.007%
59	8.580	2343	2345	2351	rVV4	1310	1261	0.08%	0.010%
60	8.645	2361	2365	2368	rVB4	1194	776	0.05%	0.006%
61	8.686	2375	2378	2380	rBV3	1445	846	0.05%	0.007%
62	8.789	2398	2410	2436	rBV	666162	1122842	68.40%	9.080%
63	8.940	2454	2457	2461	rBV5	1983	1975	0.12%	0.016%
64	9.008	2476	2478	2484	rVB4	1181	791	0.05%	0.006%
65	9.043	2487	2489	2491	rBV3	1392	778	0.05%	0.006%
66	9.092	2500	2504	2510	rBV6	2158	1952	0.12%	0.016%
67	9.124	2510	2514	2519	rVB5	1288	1172	0.07%	0.009%
68	9.159	2521	2525	2530	rBV8	3430	3471	0.21%	0.028%
69	9.310	2567	2572	2573	rBV4	2514	1964	0.12%	0.016%
70	9.384	2591	2595	2598	rBV4	790	787	0.05%	0.006%
71	9.449	2612	2615	2620	rVB5	1371	1241	0.08%	0.010%
72	9.477	2620	2624	2627	rBV3	1536	1302	0.08%	0.011%
73	9.539	2641	2643	2647	rVB3	915	645	0.04%	0.005%
74	9.587	2650	2658	2660	rBV6	3342	3701	0.23%	0.030%
75	9.883	2747	2750	2751	rBV2	1808	1013	0.06%	0.008%
76	10.034	2794	2797	2801	rBV5	1321	1206	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
 Data File : VV031752.D
 Acq On : 25 Jul 2023 19:36
 Operator : SY/MD
 Sample : 03712-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	10.114	2818	2822	2824	rBV4	1292	1139	0.07%	0.009%
78	10.159	2824	2836	2859	rVV	568627	918272	55.94%	7.426%
79	10.375	2901	2903	2907	rVB4	1963	1308	0.08%	0.011%
80	10.432	2913	2921	2925	rBV5	1567	1810	0.11%	0.015%
81	10.484	2932	2937	2940	rVB4	1218	1193	0.07%	0.010%
82	10.542	2952	2955	2959	rVB4	801	607	0.04%	0.005%
83	10.577	2959	2966	2968	rBV5	1430	1694	0.10%	0.014%
84	10.696	3001	3003	3007	rVB5	930	655	0.04%	0.005%
85	10.825	3041	3043	3046	rVB3	1085	625	0.04%	0.005%
86	10.847	3046	3050	3051	rBV4	913	750	0.05%	0.006%
87	10.908	3067	3069	3073	rVB3	1102	675	0.04%	0.005%
88	11.191	3145	3157	3177	rBV	654825	1026165	62.51%	8.298%
89	11.503	3248	3254	3261	rBV10	4859	7967	0.49%	0.064%
90	11.567	3262	3274	3295	rVB	704553	1123703	68.45%	9.087%
91	11.741	3325	3328	3330	rBV4	1318	805	0.05%	0.007%
92	11.786	3339	3342	3346	rVB5	1354	899	0.05%	0.007%
93	11.908	3377	3380	3382	rBV4	1704	1205	0.07%	0.010%
94	11.950	3384	3393	3405	rVV5	8618	17780	1.08%	0.144%
95	12.522	3569	3571	3573	rBV3	1876	929	0.06%	0.008%
96	12.725	3629	3634	3636	rBV6	1816	1948	0.12%	0.016%
97	12.776	3644	3650	3652	rBV6	1597	2115	0.13%	0.017%
98	13.329	3819	3822	3826	rBV6	1399	1163	0.07%	0.009%
99	13.873	3986	3991	4001	rVB5	14569	19918	1.21%	0.161%
100	14.812	4280	4283	4287	rVB6	2230	1390	0.08%	0.011%




Sum of corrected areas: 12365852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031752.D
Acq On : 25 Jul 2023 19:36
Operator : SY/MD
Sample : 03712-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

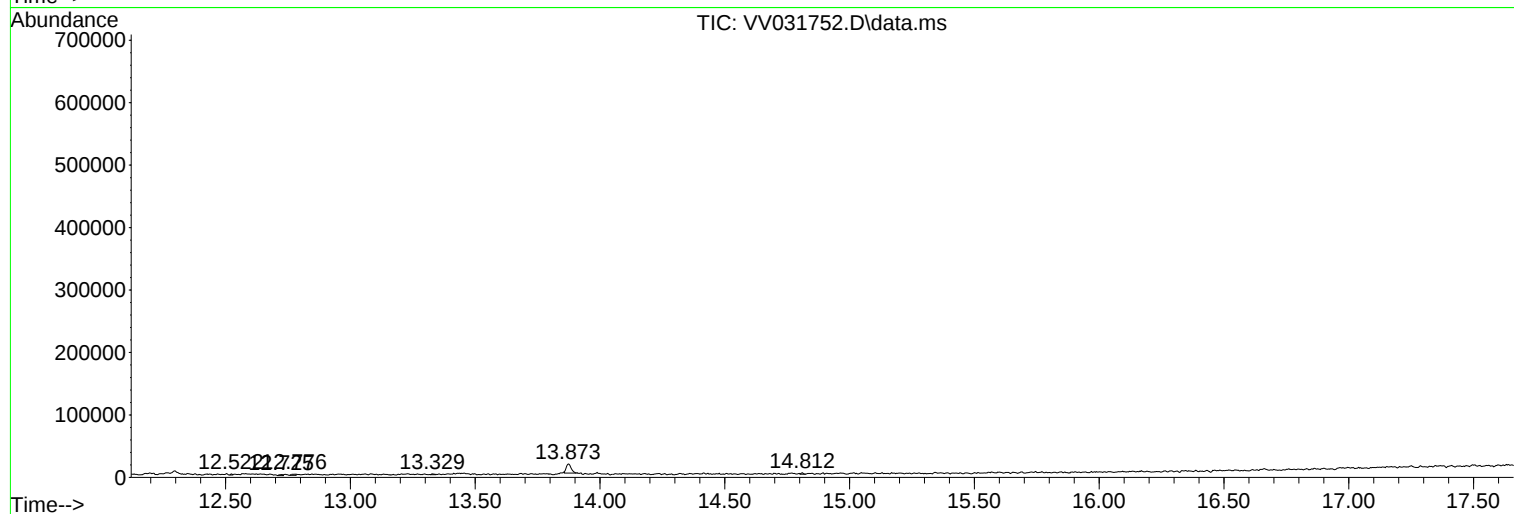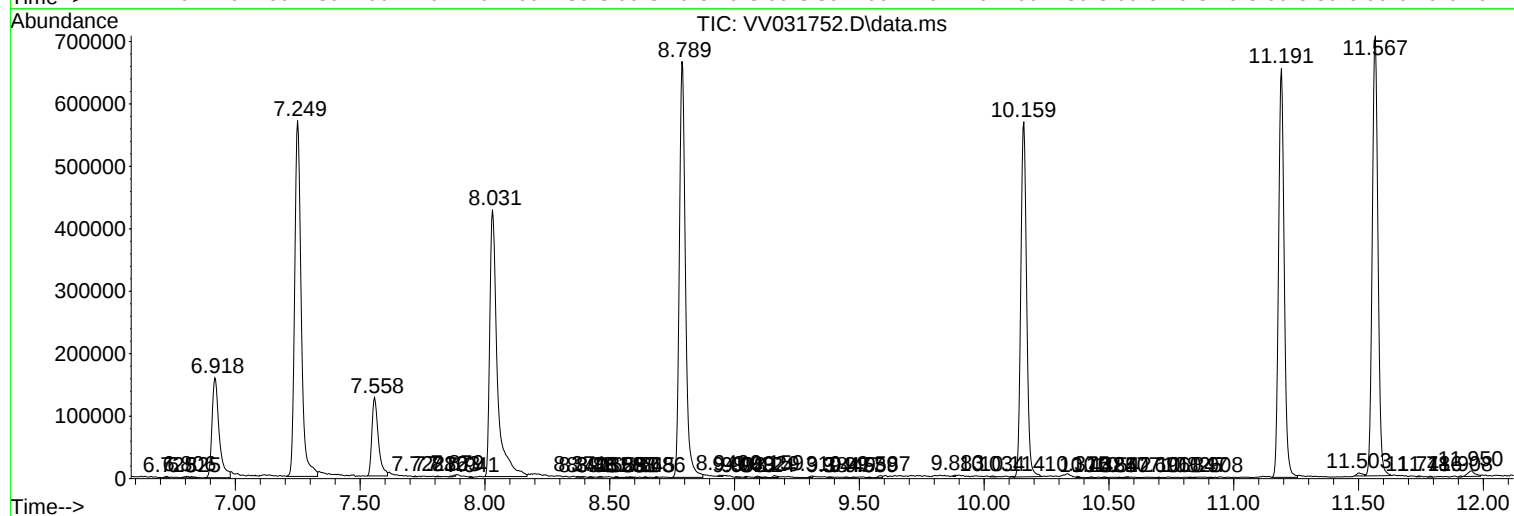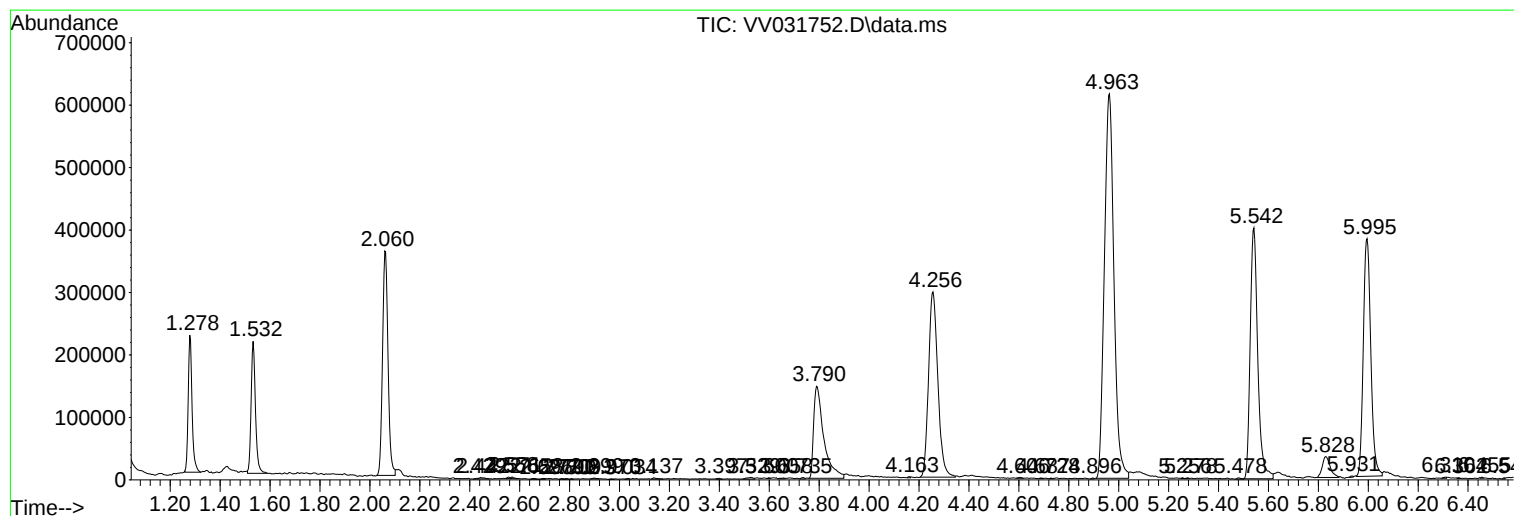

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031752.D
Acq On : 25 Jul 2023 19:36
Operator : SY/MD
Sample : 03712-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031752.D
Acq On : 25 Jul 2023 19:36
Operator : SY/MD
Sample : 03712-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------