
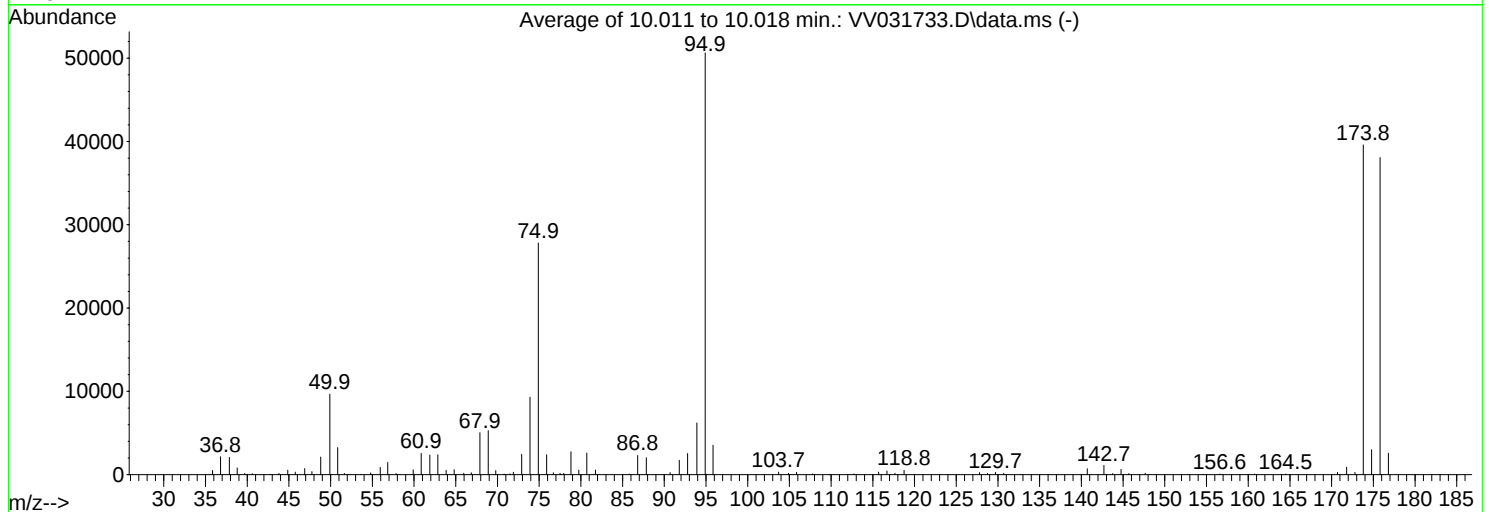


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072523\
Data File : VV031733.D
Acq On : 25 Jul 2023 08:38
Operator : SY/MD
Sample : BFB398
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB398

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Title : VOC Analysis
Last Update : Thu Jul 27 05:18:30 2023

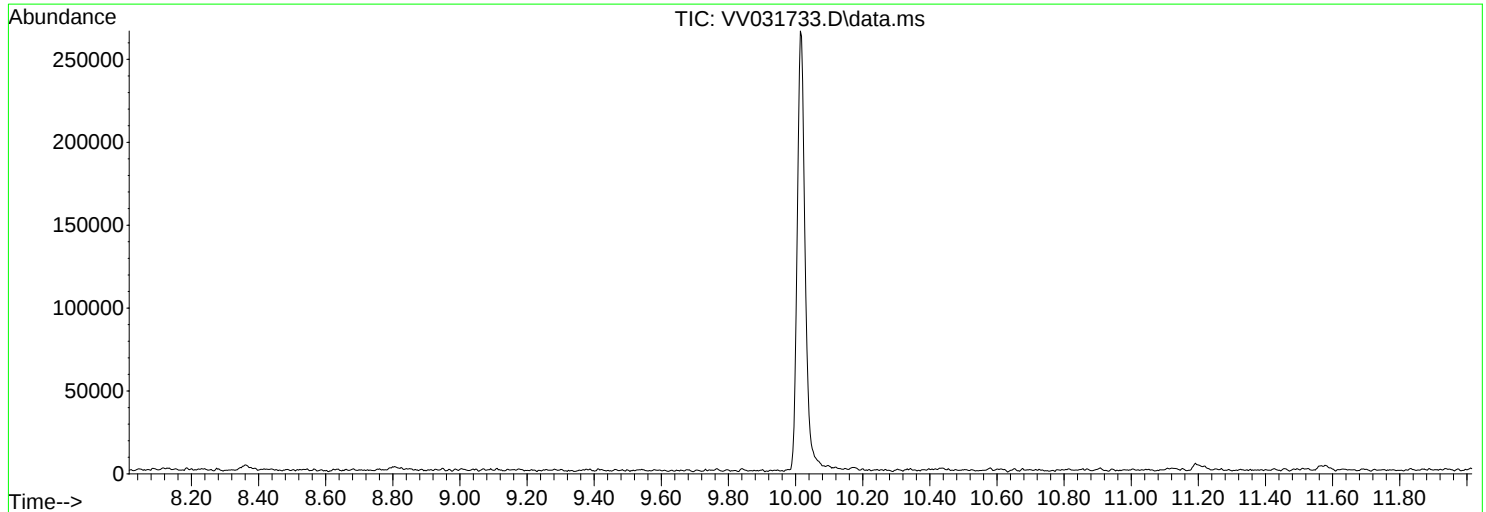

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	9673	PASS
75	95	30	80	54.9	27827	PASS
95	95	100	100	100.0	50643	PASS
96	95	5	9	7.0	3544	PASS
173	174	0.00	2	0.7	265	PASS
174	95	50	120	78.2	39600	PASS
175	174	5	9	7.6	2991	PASS
176	174	95	105	96.1	38069	PASS
177	176	5	10	6.8	2572	PASS

m/z	Abundance
35.80	406.0
36.80	1946.0
37.90	2163.0
38.90	901.0
39.70	590.0
40.60	100.0
42.00	118.0
42.80	119.0
43.80	897.0
44.90	638.0
45.80	259.0
46.90	708.0
47.70	411.0
48.80	2094.0
49.90	9515.0
50.80	3062.0
51.70	155.0
53.60	106.0
54.80	170.0
56.00	950.0
56.80	1352.0
57.80	124.0
59.90	615.0
60.90	2489.0
61.90	2034.0
62.80	2162.0
63.90	627.0
64.80	541.0
66.00	158.0
66.90	221.0
67.90	4859.0
68.90	5119.0
69.80	443.0
70.80	127.0
71.50	146.0
71.90	228.0
72.90	2203.0
73.90	8500.0
74.90	26872.0
75.90	2407.0
76.80	343.0
78.80	2381.0
79.70	458.0
80.70	2343.0
81.70	456.0
86.80	2279.0
87.80	1884.0
90.70	194.0
91.80	1637.0
92.80	2536.0
93.90	6085.0
94.90	47984.0
95.80	3374.0
103.70	245.0
104.90	135.0
105.80	290.0
107.80	144.0
109.80	104.0
112.70	173.0
115.70	256.0
116.70	490.0
117.70	183.0
118.70	580.0
127.80	251.0
128.70	176.0
129.70	233.0
130.70	145.0
140.70	682.0
142.70	1134.0
143.70	136.0
144.70	559.0
145.70	115.0
147.70	127.0
154.60	122.0
160.70	101.0
164.50	119.0
170.80	252.0
171.80	675.0
172.80	795.0
173.80	36576.0
174.80	2810.0
175.80	35256.0
176.80	2382.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398

m/z	Abundance
35.90	519.0
36.80	2226.0
37.80	2129.0
38.90	1018.0
39.70	563.0
40.60	120.0
41.90	148.0
42.70	173.0
43.80	957.0
44.90	712.0
45.70	314.0
46.90	700.0
47.70	371.0
48.80	2330.0
49.90	10102.0
50.80	3377.0
51.60	133.0
54.80	221.0
55.90	880.0
56.80	1502.0
57.80	140.0
59.90	604.0
60.90	2626.0
61.90	2416.0
62.90	2458.0
63.90	669.0
64.80	604.0
66.00	212.0
66.80	244.0
67.90	5179.0
68.90	5521.0
69.80	506.0
70.80	126.0
71.50	132.0
71.90	297.0
72.90	2722.0
73.90	9745.0
74.90	28728.0
75.90	2517.0
76.70	362.0
77.50	234.0
78.00	253.0
78.80	2857.0
79.80	540.0
80.70	2714.0
81.80	584.0
85.80	101.0
86.80	2479.0
87.80	2083.0
90.70	252.0
91.80	1795.0
92.80	2754.0
93.90	6419.0
94.90	52208.0
95.90	3669.0
103.70	315.0
104.90	177.0
105.80	261.0
107.80	120.0
112.80	142.0
115.70	338.0
116.70	442.0
117.70	185.0
118.70	564.0
127.80	277.0
128.80	166.0
129.70	294.0
130.70	174.0
140.70	728.0
142.70	1114.0
143.70	139.0
144.80	659.0
145.60	138.0
147.60	187.0
152.80	101.0
156.60	118.0
160.80	109.0
164.50	102.0
170.60	275.0
171.80	914.0
173.80	41056.0
174.80	3108.0
175.80	39064.0
176.80	2609.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398

m/z	Abundance
35.90	585.0
36.80	2267.0
37.80	1948.0
38.80	991.0
39.80	502.0
40.60	111.0
41.90	134.0
42.80	221.0
43.80	1109.0
44.80	566.0
45.70	331.0
46.90	795.0
47.80	297.0
48.80	2210.0
49.90	9403.0
50.90	3308.0
51.60	117.0
52.10	137.0
54.80	269.0
55.90	749.0
56.90	1513.0
57.90	146.0
59.90	531.0
60.80	2569.0
61.90	2600.0
62.90	2546.0
63.80	584.0
64.80	665.0
65.90	180.0
66.80	231.0
67.90	5040.0
68.90	5202.0
69.80	511.0
71.90	315.0
72.90	2731.0
73.90	9640.0
74.90	27880.0
75.90	2220.0
76.70	381.0
77.50	253.0
77.90	225.0
78.80	3018.0
79.80	601.0
80.70	2744.0
81.80	614.0
85.80	106.0
86.80	2182.0
87.90	2146.0
90.70	285.0
91.80	1731.0
92.90	2651.0
93.90	6115.0
94.90	51736.0
95.90	3588.0
103.70	351.0
104.90	176.0
105.90	230.0
115.70	335.0
116.70	397.0
117.60	124.0
118.80	433.0
127.80	239.0
128.80	120.0
129.70	252.0
130.70	197.0
132.70	103.0
140.70	729.0
142.70	1074.0
143.80	150.0
144.80	704.0
145.80	183.0
147.60	231.0
156.60	132.0
170.70	308.0
171.80	1079.0
173.80	41168.0
174.80	3054.0
175.80	39888.0
176.80	2725.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398

m/z	Abundance
38.80	155.0
39.70	416.0
41.90	135.0
42.80	123.0
43.80	833.0
44.90	106.0
48.00	101.0
49.00	103.0
63.90	111.0
65.20	155.0
73.00	110.0
76.70	138.0
92.70	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398