

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036678.D
 Acq On : 24 Jul 2024 22:08
 Operator : SY/MD
 Sample : P3335-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 25 04:28:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 03:06:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	346422	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	359811	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	162217	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	109944	43.129	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.260%
7) Chloroethane-d5	1.529	69	97616	44.723	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.440%
11) 1,1-Dichloroethene-d2	2.053	65	53096	43.544	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.080%
21) 2-Butanone-d5	3.783	46	109420	83.750	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	83.750%
24) Chloroform-d	4.243	84	226808	43.454	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.900%
26) 1,2-Dichloroethane-d4	4.937	65	143832	46.274	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.540%
32) Benzene-d6	4.953	84	425649	45.100	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.200%
36) 1,2-Dichloropropane-d6	5.985	67	124098	46.318	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.640%
41) Toluene-d8	7.239	98	390840	42.455	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.900%
43) trans-1,3-Dichloroprop...	7.551	79	57255	39.484	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.960%
47) 2-Hexanone-d5	8.021	63	81777	82.470	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.470%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	154155	37.132	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	74.260%
66) 1,2-Dichlorobenzene-d4	11.558	152	172914	51.711	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.420%
Target Compounds						
					Qvalue	
13) Acetone	2.111	43	5586	4.460	ug/L	99
39) cis-1,3-Dichloropropene	6.911	75	3522	0.891	ug/L #	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036678.D
Acq On : 24 Jul 2024 22:08
Operator : SY/MD
Sample : P3335-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jul 25 04:28:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 03:06:08 2024
Response via : Initial Calibration

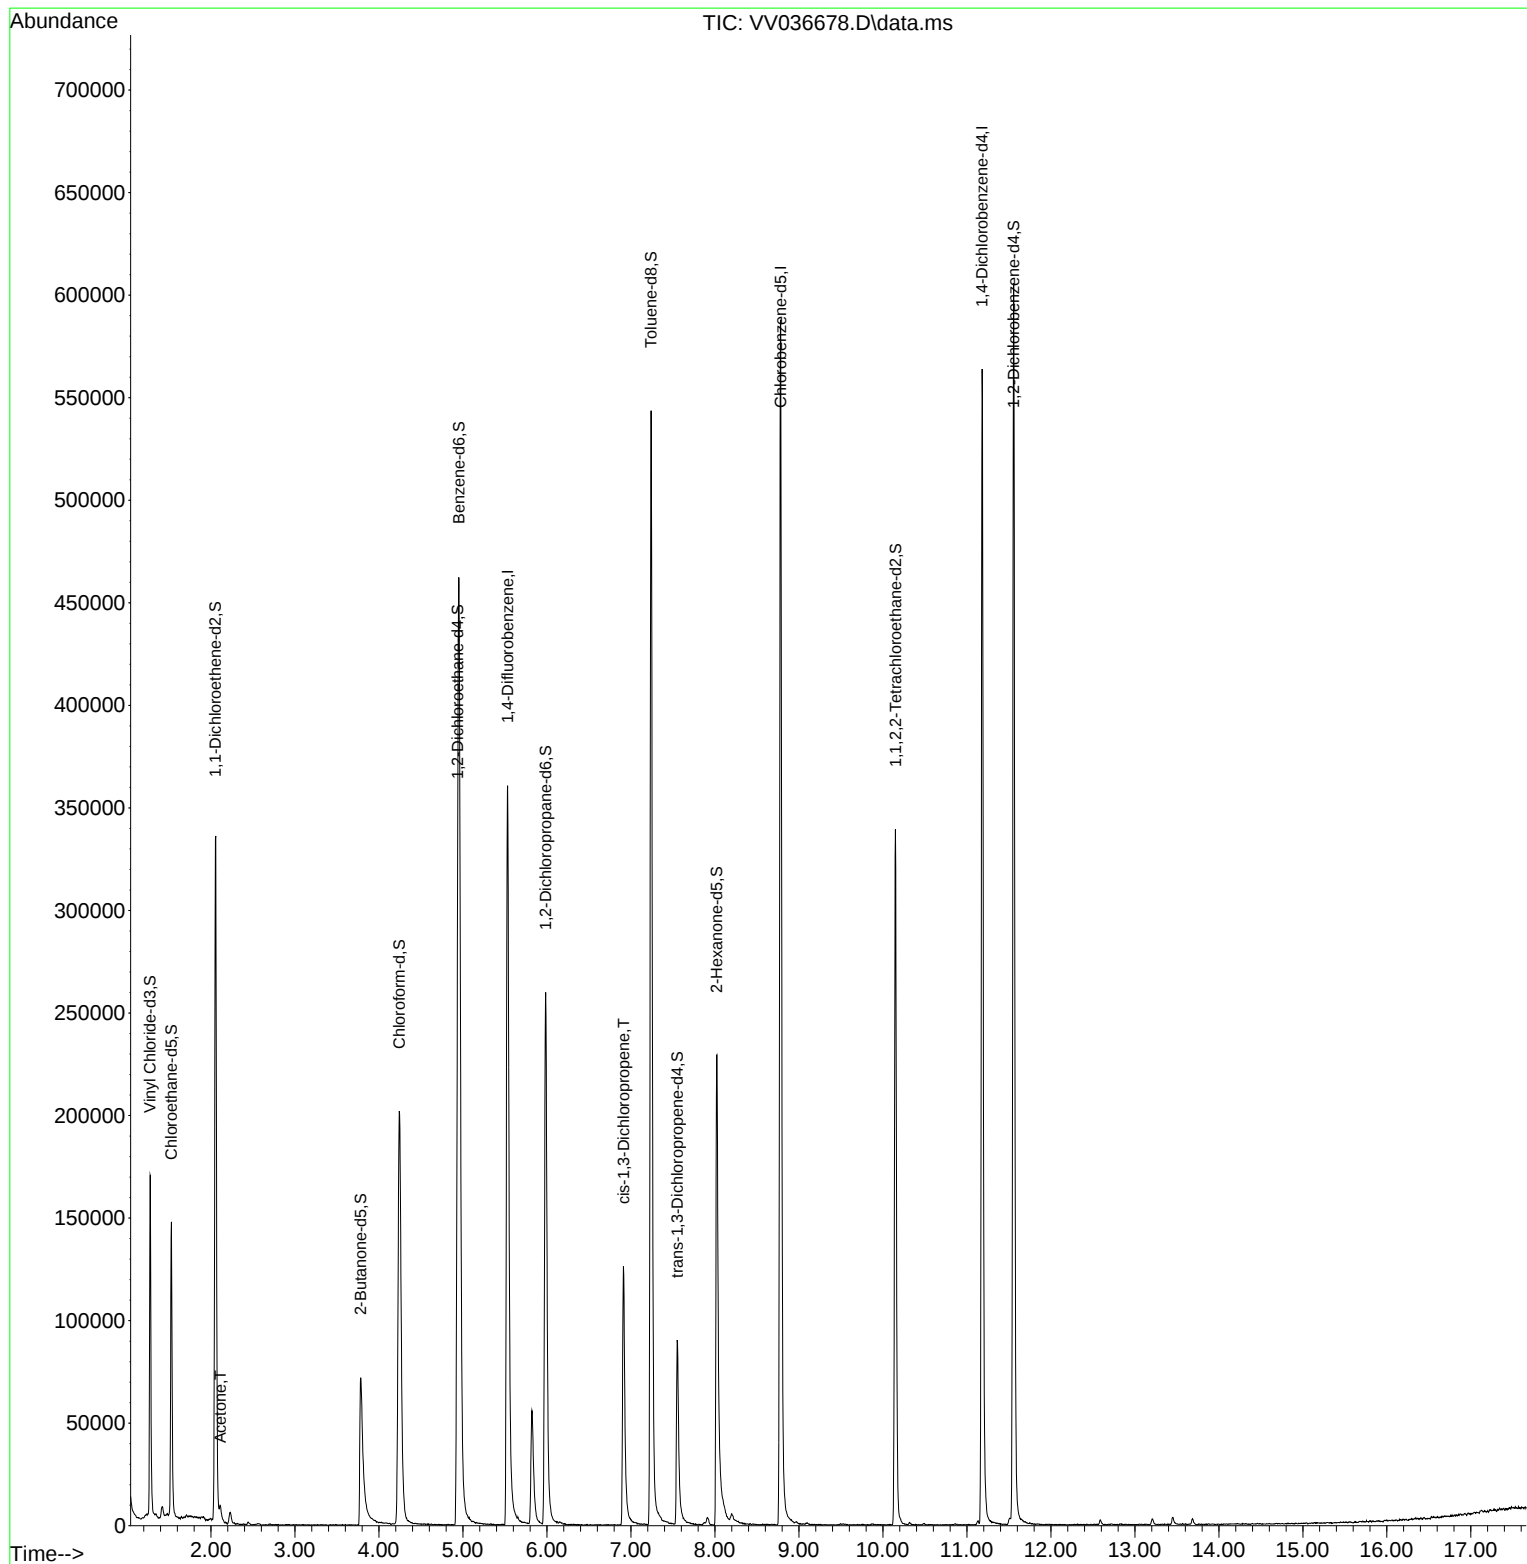

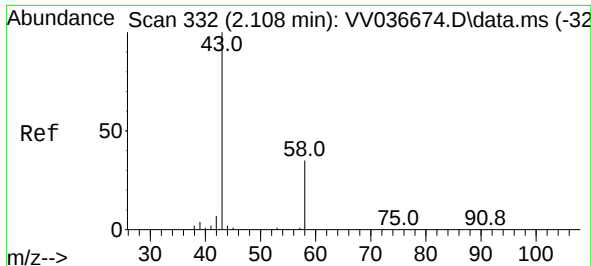

#13

Acetone

Concen: 4.460 ug/L

RT: 2.111 min Scan# 332

Delta R.T. 0.003 min

Lab File: VV036678.D

Acq: 24 Jul 2024 22:08

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 5586

Ion Ratio Lower Upper

43 100

58 35.8 0.0 72.4

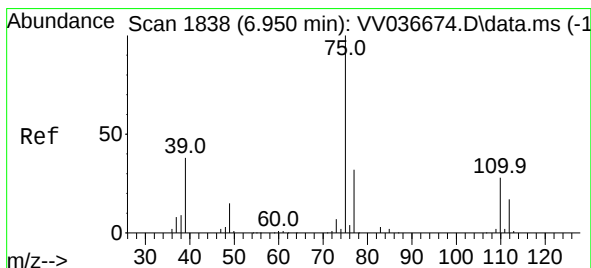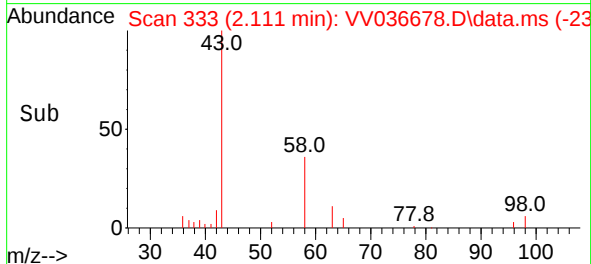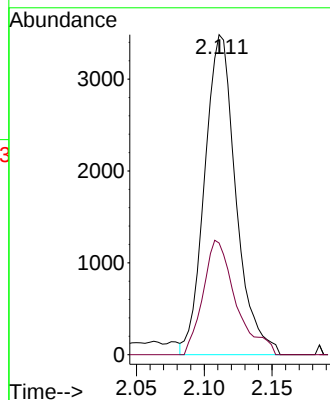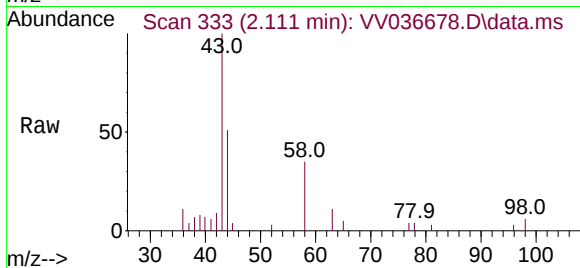

#39

cis-1,3-Dichloropropene

Concen: 0.891 ug/L

RT: 6.911 min Scan# 1826

Delta R.T. -0.039 min

Lab File: VV036678.D

Acq: 24 Jul 2024 22:08

Tgt Ion: 75 Resp: 3522

Ion Ratio Lower Upper

75 100

77 58.7 22.3 41.3#

