

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036682.D
 Acq On : 24 Jul 2024 23:45
 Operator : SY/MD
 Sample : P3335-06DL 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 25 04:29:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 03:06:08 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	335702	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	347109	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	150872	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	106714	43.198	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.400%
7) Chloroethane-d5	1.526	69	96080	45.425	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.860%
11) 1,1-Dichloroethene-d2	2.056	65	50518	42.753	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.500%
21) 2-Butanone-d5	3.780	46	112781	89.079	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.080%
24) Chloroform-d	4.243	84	229850	45.443	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.880%
26) 1,2-Dichloroethane-d4	4.937	65	147526	48.978	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.960%
32) Benzene-d6	4.953	84	419495	46.074	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.140%
36) 1,2-Dichloropropane-d6	5.985	67	124478	48.160	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.320%
41) Toluene-d8	7.239	98	367402	41.369	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.740%
43) trans-1,3-Dichloroprop...	7.551	79	57934	41.414	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.820%
47) 2-Hexanone-d5	8.021	63	82229	85.960	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.960%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	177895	44.418	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.840%
66) 1,2-Dichlorobenzene-d4	11.558	152	164140	52.778	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.560%
Target Compounds						
37) 1,2-Dichloropropane	5.985	63	14288	6.391	ug/L	Qvalue # 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036682.D
Acq On : 24 Jul 2024 23:45
Operator : SY/MD
Sample : P3335-06DL 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jul 25 04:29:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 03:06:08 2024
Response via : Initial Calibration

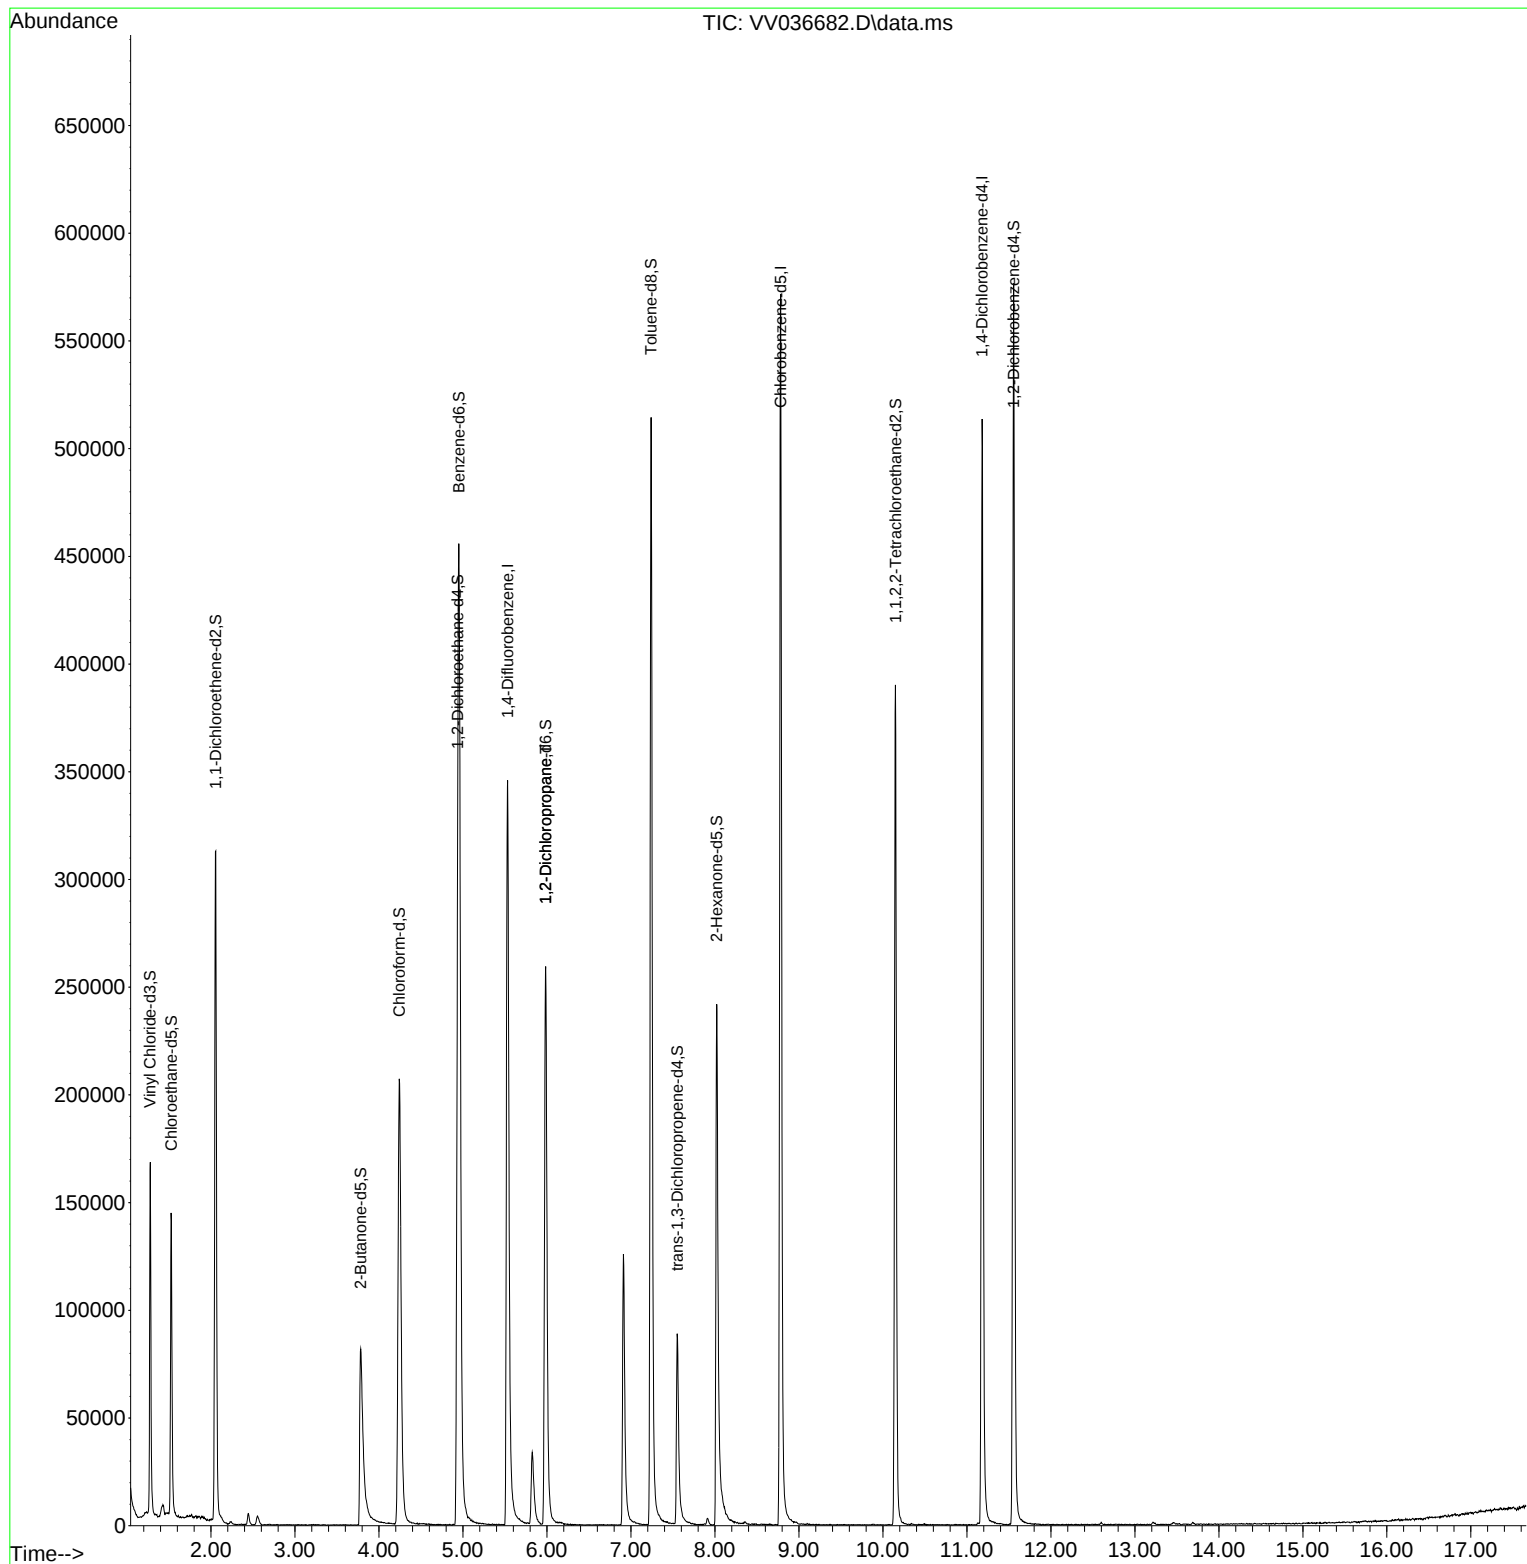

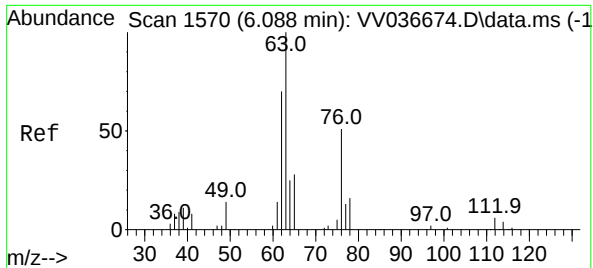

#37
 1,2-Dichloropropane
 Concen: 6.391 ug/L
 RT: 5.985 min Scan# 14
 Delta R.T. -0.103 min
 Lab File: VV036682.D
 Acq: 24 Jul 2024 23:45

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 63 Resp: 14288
 Ion Ratio Lower Upper
 63 100
 112 0.4 5.1 7.7#

