

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036684.D
 Acq On : 25 Jul 2024 00:33
 Operator : SY/MD
 Sample : P3335-09DL 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 25 04:30:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 03:06:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	335033	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	341762	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	144263	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	102761	41.681	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	83.360%	
7) Chloroethane-d5	1.529	69	93447	44.269	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	88.540%	
11) 1,1-Dichloroethene-d2	2.056	65	48837	41.412	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	82.820%	
21) 2-Butanone-d5	3.780	46	114169	90.355	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	90.360%	
24) Chloroform-d	4.243	84	224820	44.538	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	89.080%	
26) 1,2-Dichloroethane-d4	4.937	65	144081	47.930	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.860%	
32) Benzene-d6	4.957	84	403102	44.966	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	89.940%	
36) 1,2-Dichloropropane-d6	5.985	67	120783	47.461	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	94.920%	
41) Toluene-d8	7.239	98	348397	39.843	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	79.680%#	
43) trans-1,3-Dichloroprop...	7.551	79	54682	39.701	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	79.400%	
47) 2-Hexanone-d5	8.021	63	82855	87.970	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	87.970%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	175286	44.451	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	88.900%	
66) 1,2-Dichlorobenzene-d4	11.558	152	155720	52.364	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	104.720%	
Target Compounds						
39) cis-1,3-Dichloropropene	6.911	75	3398	0.905	ug/L	Qvalue # 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036684.D
Acq On : 25 Jul 2024 00:33
Operator : SY/MD
Sample : P3335-09DL 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jul 25 04:30:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 03:06:08 2024
Response via : Initial Calibration

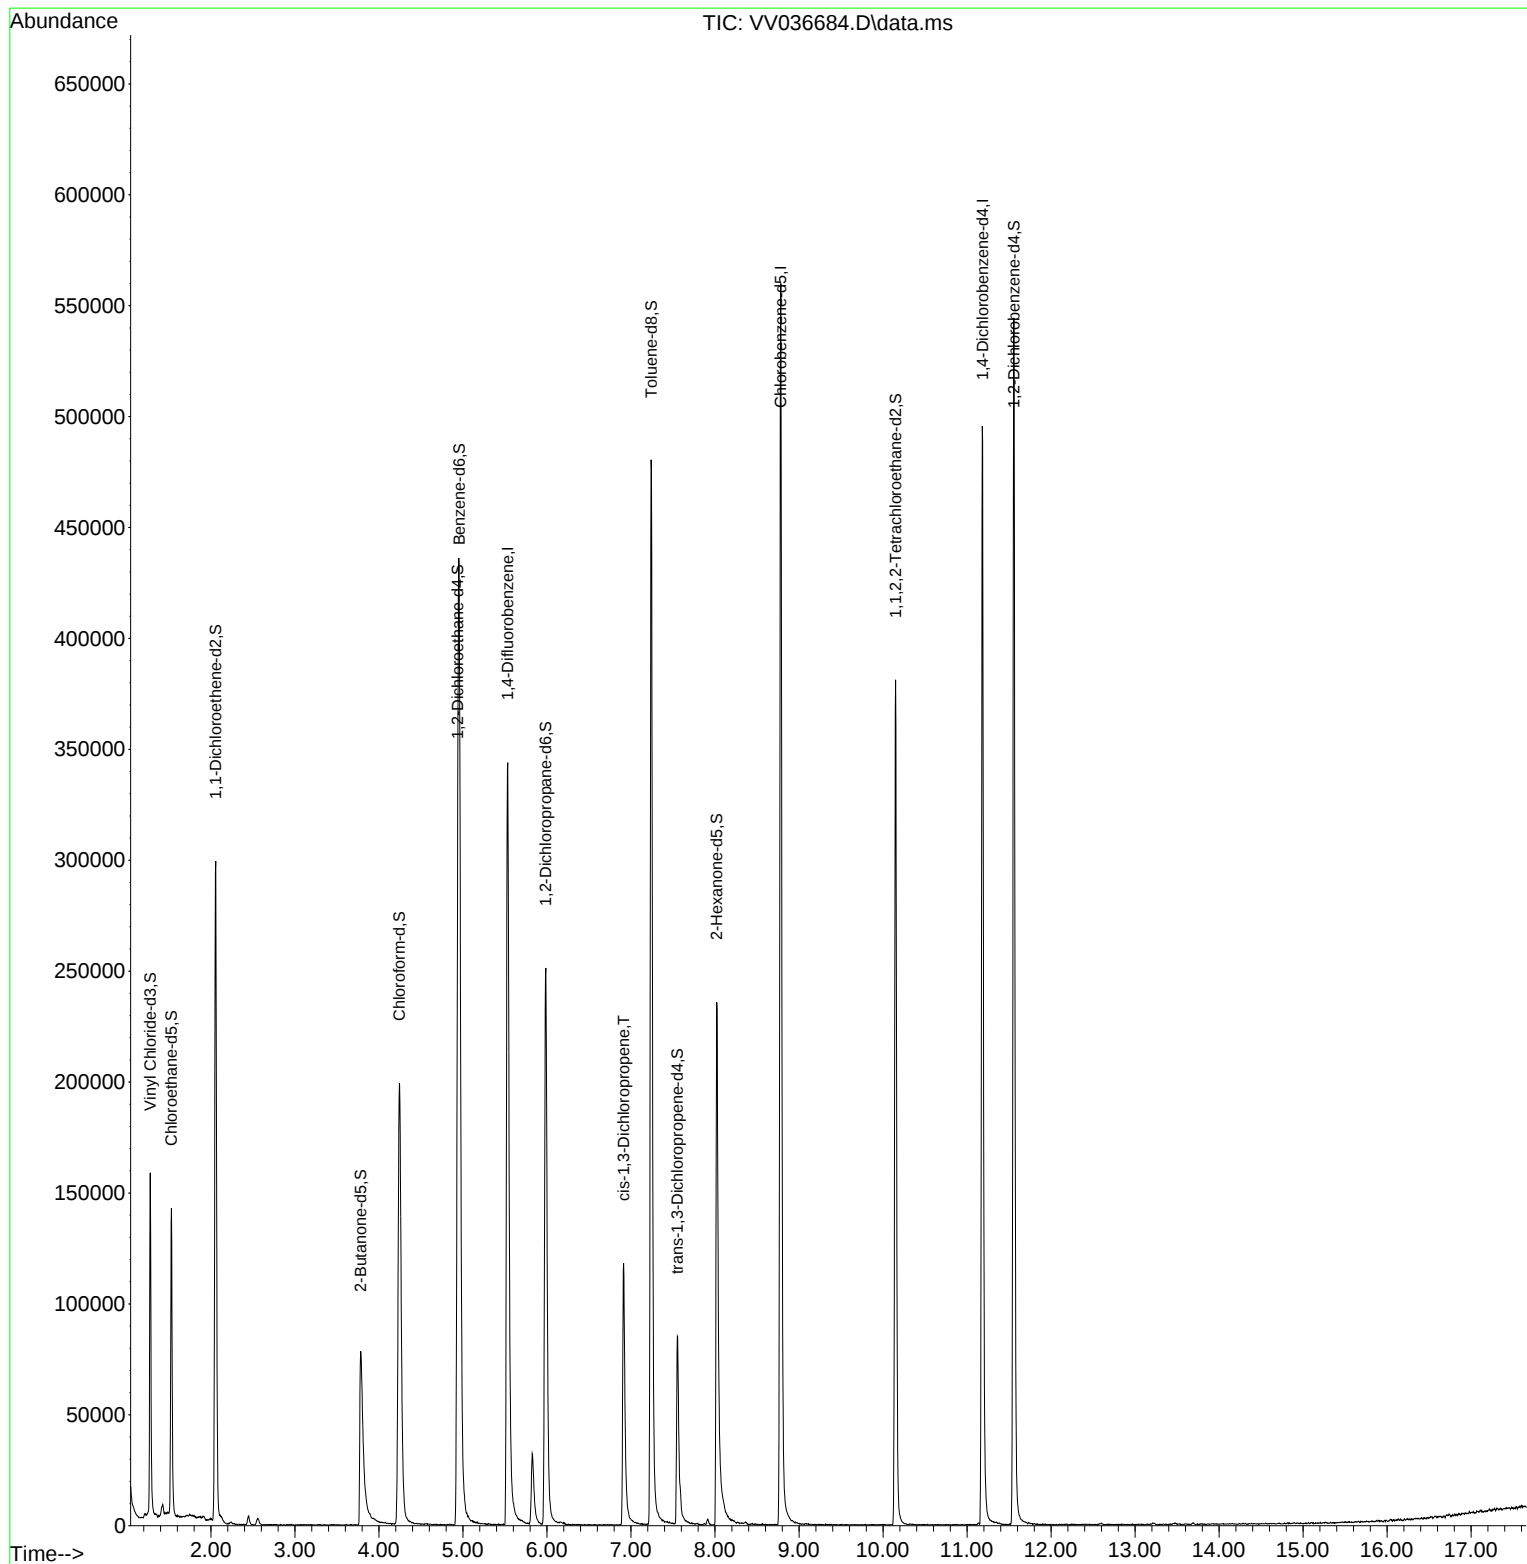

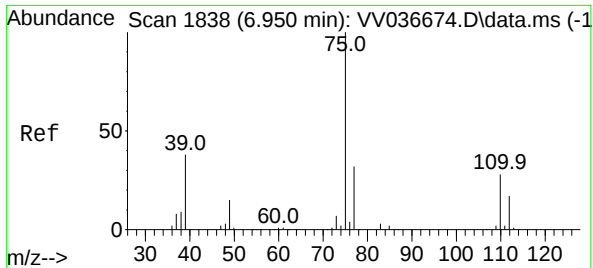

#39
 cis-1,3-Dichloropropene
 Concen: 0.905 ug/L
 RT: 6.911 min Scan# 11
 Delta R.T. -0.039 min
 Lab File: VV036684.D
 Acq: 25 Jul 2024 00:33

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 3398
 Ion Ratio Lower Upper
 75 100
 77 48.8 22.3 41.3#

