

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072524\
 Data File : VW036676.D
 Acq On : 24 Jul 2024 21:19
 Operator : SY/MD
 Sample : P3335-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K8

Quant Time: Jul 25 06:11:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 03:06:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	354044	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	365729	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	169460	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	113931	43.731	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.460%
7) Chloroethane-d5	1.529	69	99775	44.728	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.460%
11) 1,1-Dichloroethene-d2	2.053	65	54760	43.942	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.880%
21) 2-Butanone-d5	3.783	46	113609	85.084	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.080%
24) Chloroform-d	4.243	84	232238	43.537	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.080%
26) 1,2-Dichloroethane-d4	4.937	65	147211	46.342	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.680%
32) Benzene-d6	4.953	84	437376	45.592	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.180%
36) 1,2-Dichloropropane-d6	5.985	67	128261	47.097	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.200%
41) Toluene-d8	7.239	98	402608	43.026	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.060%
43) trans-1,3-Dichloroprop...	7.551	79	59359	40.272	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.540%
47) 2-Hexanone-d5	8.021	63	82199	81.554	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.550%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	174400	41.328	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.660%
66) 1,2-Dichlorobenzene-d4	11.557	152	178460	51.088	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.180%
Target Compounds						
13) Acetone	2.111	43	5745	4.488	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036676.D
Acq On : 24 Jul 2024 21:19
Operator : SY/MD
Sample : P3335-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K8

Quant Time: Jul 25 06:11:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 03:06:08 2024
Response via : Initial Calibration

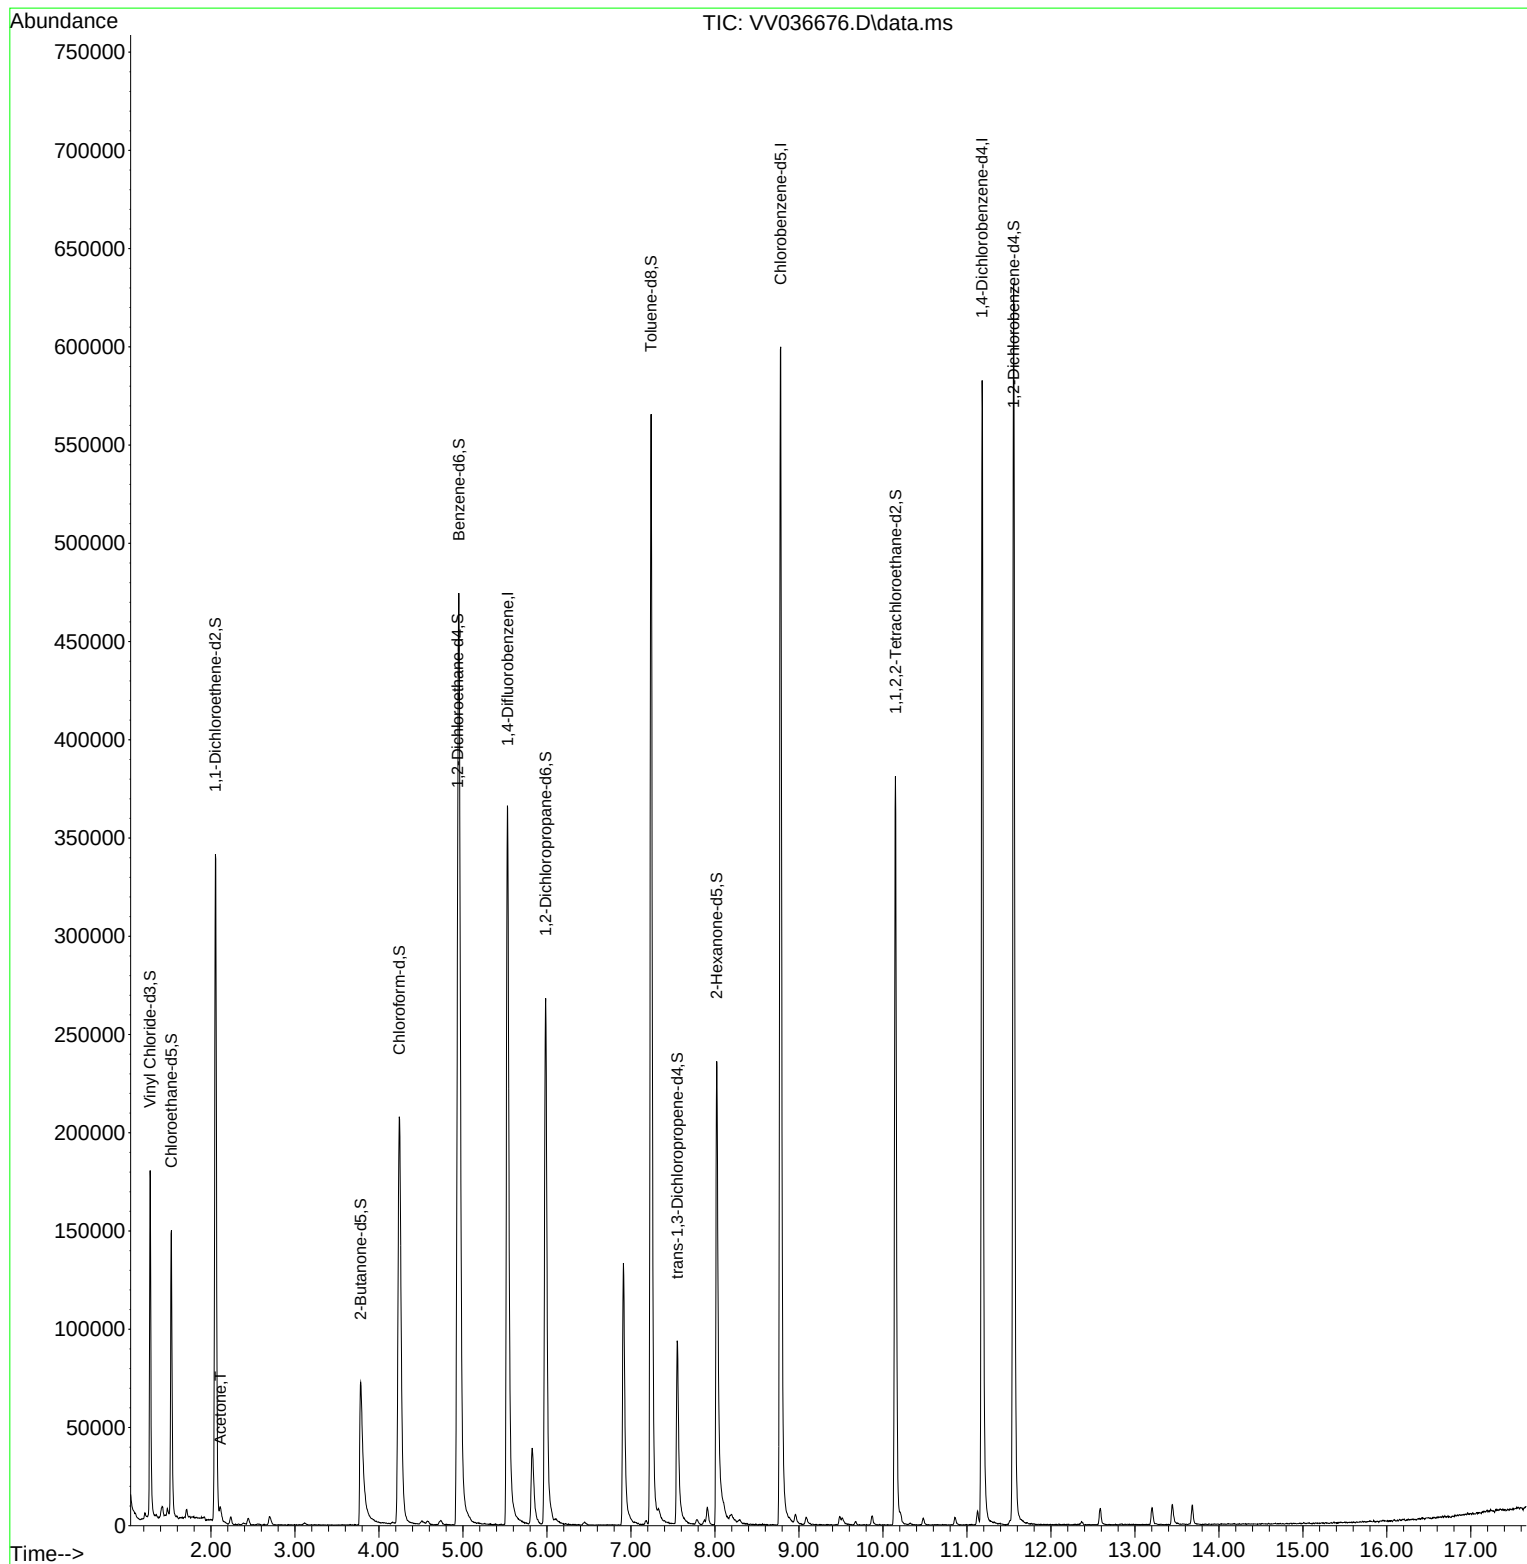

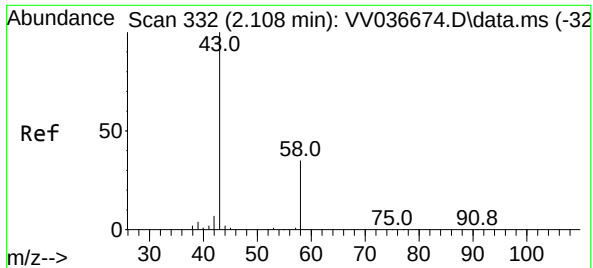

#13

Acetone

Concen: 4.488 ug/L

RT: 2.111 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV036676.D


Acq: 24 Jul 2024 21:19

Instrument :

MSVOA_V

ClientSampleId :

E20K8

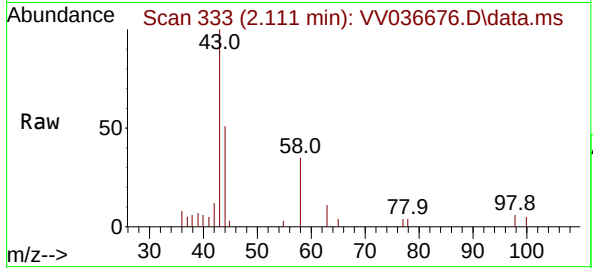

Tgt Ion: 43 Resp: 5745

Ion Ratio Lower Upper

43 100

58 33.9 0.0 72.4

