

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036677.D
 Acq On : 24 Jul 2024 21:44
 Operator : SY/MD
 Sample : P3335-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L2

Quant Time: Jul 25 04:28:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 03:06:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	365598	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	376263	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	169875	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	112447	41.797	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.600%
7) Chloroethane-d5	1.529	69	98201	42.631	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.260%
11) 1,1-Dichloroethene-d2	2.053	65	54247	42.154	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.300%
21) 2-Butanone-d5	3.783	46	109796	79.630	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	79.630%
24) Chloroform-d	4.243	84	234990	42.660	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.320%
26) 1,2-Dichloroethane-d4	4.937	65	147814	45.061	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.120%
32) Benzene-d6	4.953	84	433266	43.900	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.800%
36) 1,2-Dichloropropane-d6	5.985	67	125434	44.769	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.540%
41) Toluene-d8	7.239	98	401111	41.666	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.340%
43) trans-1,3-Dichloroprop...	7.551	79	60753	40.064	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.120%
47) 2-Hexanone-d5	8.021	63	82498	79.559	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.560%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	160491	36.967	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	73.940%
66) 1,2-Dichlorobenzene-d4	11.558	152	176647	50.446	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.900%
Target Compounds						
13) Acetone	2.111	43	9933	7.515	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036677.D
Acq On : 24 Jul 2024 21:44
Operator : SY/MD
Sample : P3335-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20L2

Quant Time: Jul 25 04:28:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 03:06:08 2024
Response via : Initial Calibration

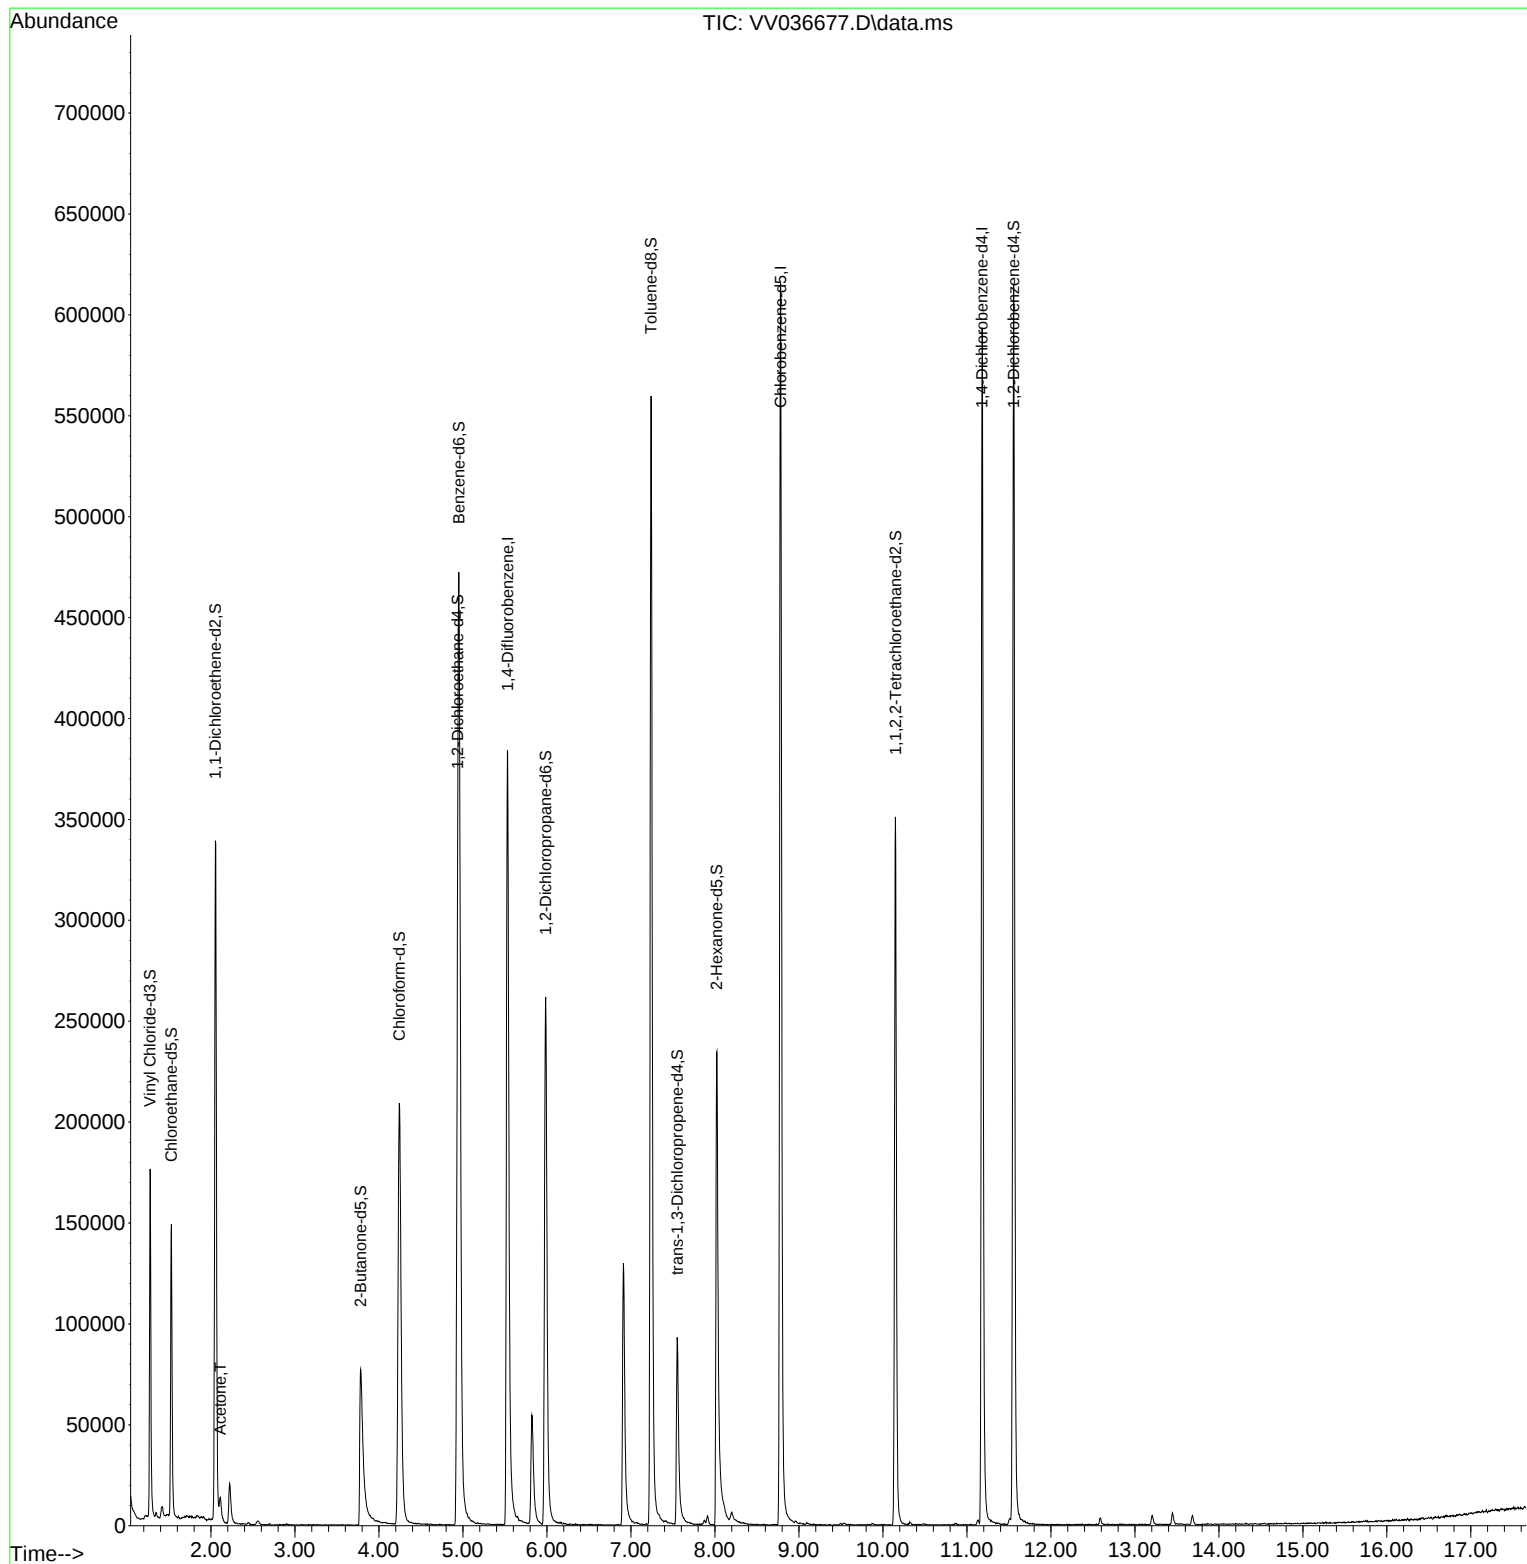

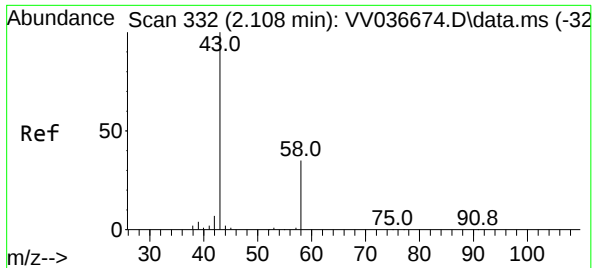

#13
 Acetone
 Concen: 7.515 ug/L
 RT: 2.111 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV036677.D
 Acq: 24 Jul 2024 21:44

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L2

Tgt Ion: 43 Resp: 9933
 Ion Ratio Lower Upper
 43 100
 58 36.1 0.0 72.4

