

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072524\
 Data File : VW036682.D
 Acq On : 24 Jul 2024 23:45
 Operator : SY/MD
 Sample : P3334-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20F3

Quant Time: Jul 25 12:57:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 03:06:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	335702	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	347109	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	150872	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	106714	43.198	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.400%		
7) Chloroethane-d5	1.526	69	96080	45.425	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.860%		
11) 1,1-Dichloroethene-d2	2.056	65	50518	42.753	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.500%		
21) 2-Butanone-d5	3.780	46	112781	89.079	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	89.080%		
24) Chloroform-d	4.243	84	229850	45.443	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.880%		
26) 1,2-Dichloroethane-d4	4.937	65	147526	48.978	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.960%		
32) Benzene-d6	4.953	84	419495	46.074	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.140%		
36) 1,2-Dichloropropane-d6	5.985	67	124478	48.160	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.320%		
41) Toluene-d8	7.239	98	367402	41.369	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.740%		
43) trans-1,3-Dichloroprop...	7.551	79	57934	41.414	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.820%		
47) 2-Hexanone-d5	8.021	63	82229	85.960	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.960%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	177895	44.418	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.840%		
66) 1,2-Dichlorobenzene-d4	11.558	152	164140	52.778	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.560%		
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	5.985	63	14288	6.391	ug/L	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036682.D
Acq On : 24 Jul 2024 23:45
Operator : SY/MD
Sample : P3334-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20F3

Quant Time: Jul 25 12:57:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 03:06:08 2024
Response via : Initial Calibration

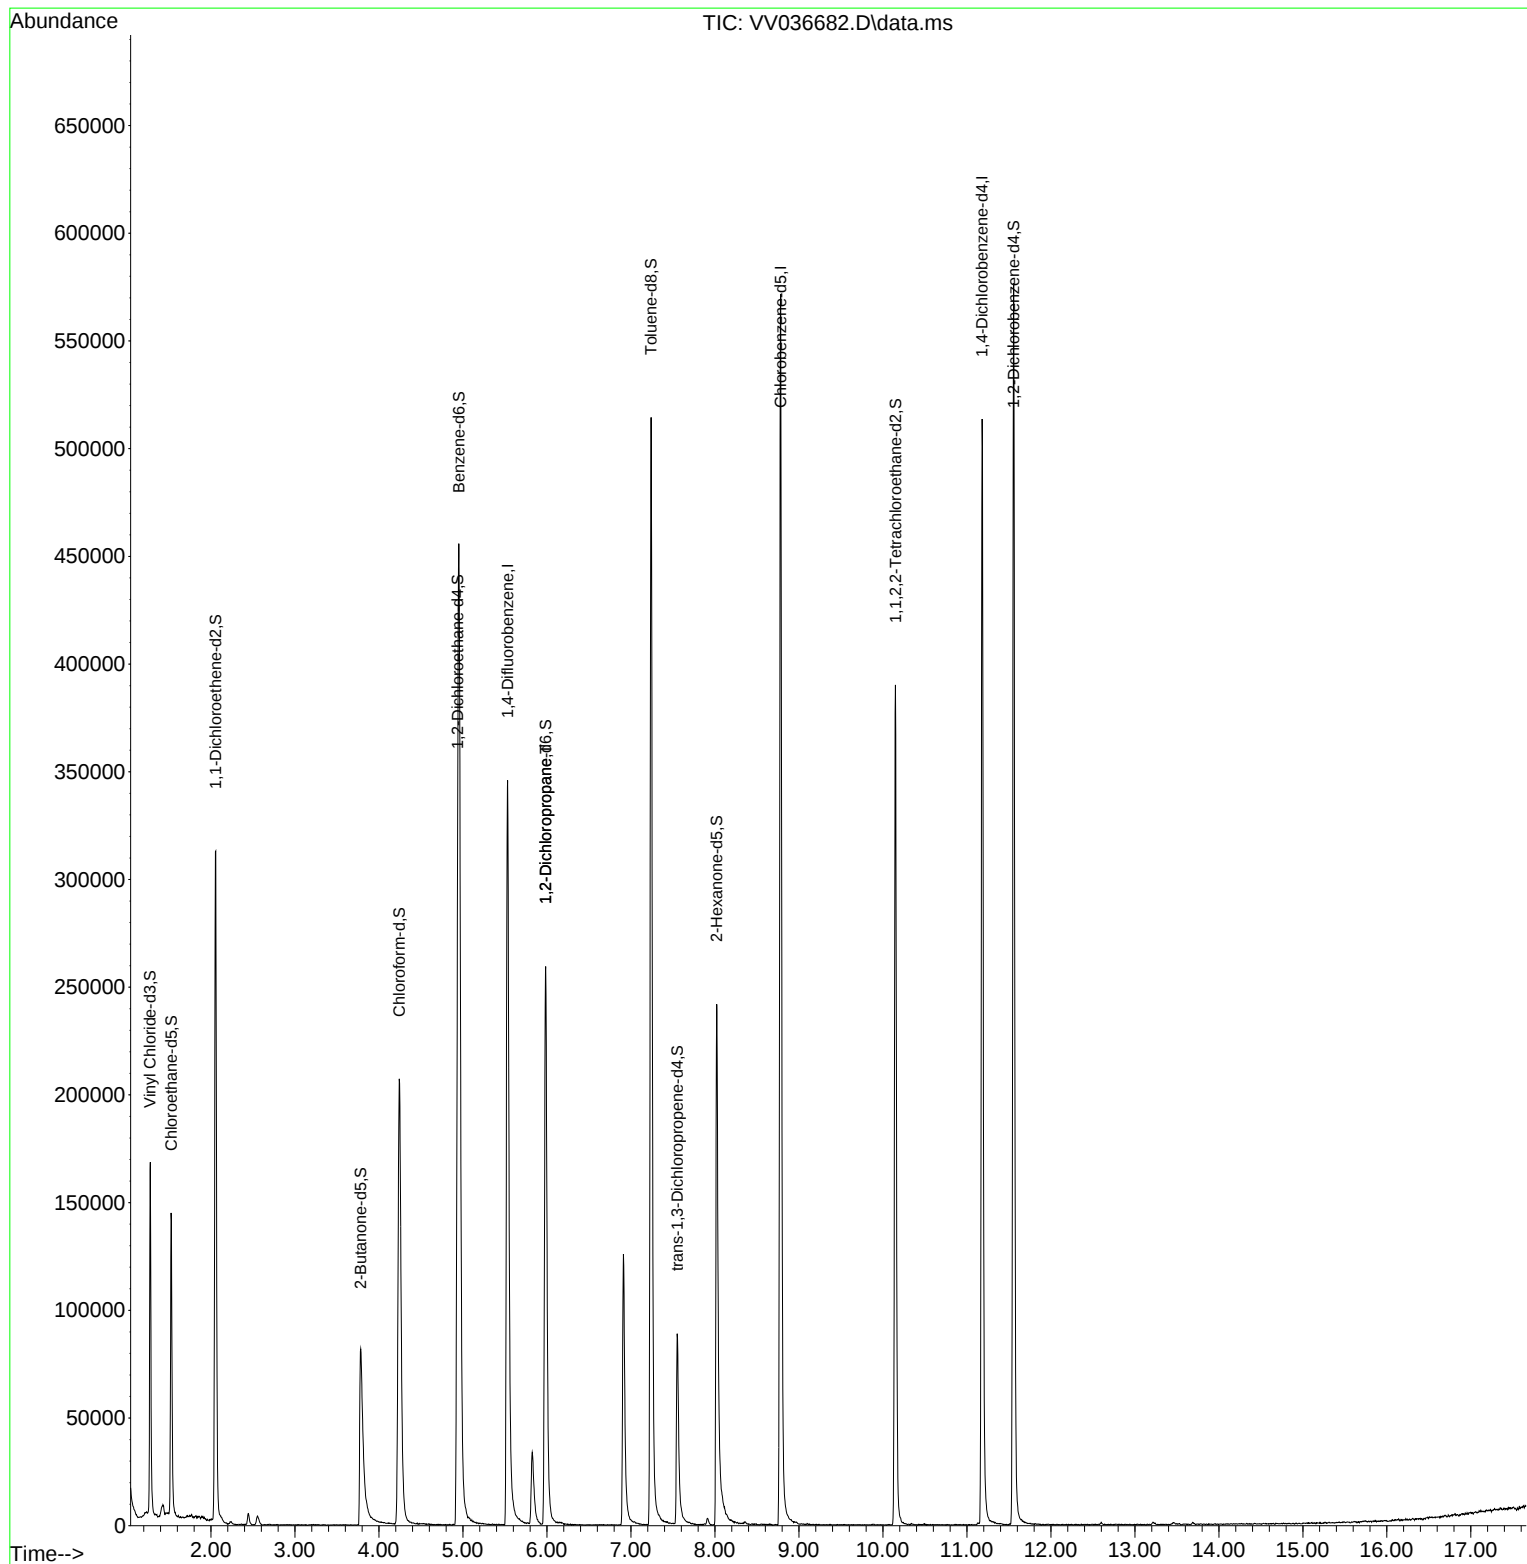

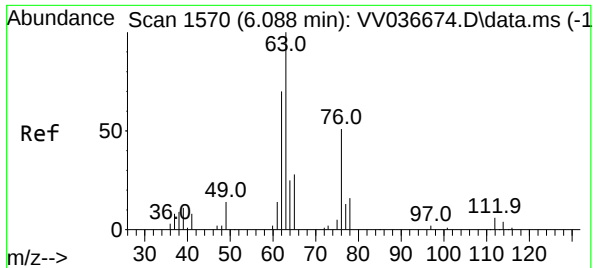

#37
 1,2-Dichloropropane
 Concen: 6.391 ug/L
 RT: 5.985 min Scan# 11
 Delta R.T. -0.103 min
 Lab File: VV036682.D
 Acq: 24 Jul 2024 23:45

Instrument :
 MSVOA_V
 ClientSampleId :
 E20F3

Tgt Ion: 63 Resp: 14288
 Ion Ratio Lower Upper
 63 100
 112 0.4 5.1 7.7#

