

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072524\
 Data File : VW036683.D
 Acq On : 25 Jul 2024 00:09
 Operator : SY/MD
 Sample : P3334-12
 Misc : 5.00mL/MSVOA_V/WATER/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20G9

Quant Time: Jul 25 12:57:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 03:06:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	338116	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	349708	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	155401	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	108297	43.526	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.060%
7) Chloroethane-d5	1.529	69	98194	46.093	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.180%
11) 1,1-Dichloroethene-d2	2.056	65	52514	44.124	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.240%
21) 2-Butanone-d5	3.783	46	108712	85.252	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.250%
24) Chloroform-d	4.246	84	233463	45.828	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.660%
26) 1,2-Dichloroethane-d4	4.937	65	150329	49.553	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.100%
32) Benzene-d6	4.953	84	430311	46.911	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.820%
36) 1,2-Dichloropropane-d6	5.985	67	126549	48.597	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.200%
41) Toluene-d8	7.239	98	381554	42.644	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.280%
43) trans-1,3-Dichloroprop...	7.551	79	57824	41.028	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.060%
47) 2-Hexanone-d5	8.021	63	82811	85.925	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.930%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	181209	44.909	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.820%
66) 1,2-Dichlorobenzene-d4	11.557	152	171096	53.411	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.820%
Target Compounds						
61) 1,2,3-Trichloropropane	11.181	75	14314	5.493	ug/L	Qvalue # 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036683.D
Acq On : 25 Jul 2024 00:09
Operator : SY/MD
Sample : P3334-12
Misc : 5.00mL/MSVOA_V/WATER/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20G9

Quant Time: Jul 25 12:57:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 03:06:08 2024
Response via : Initial Calibration

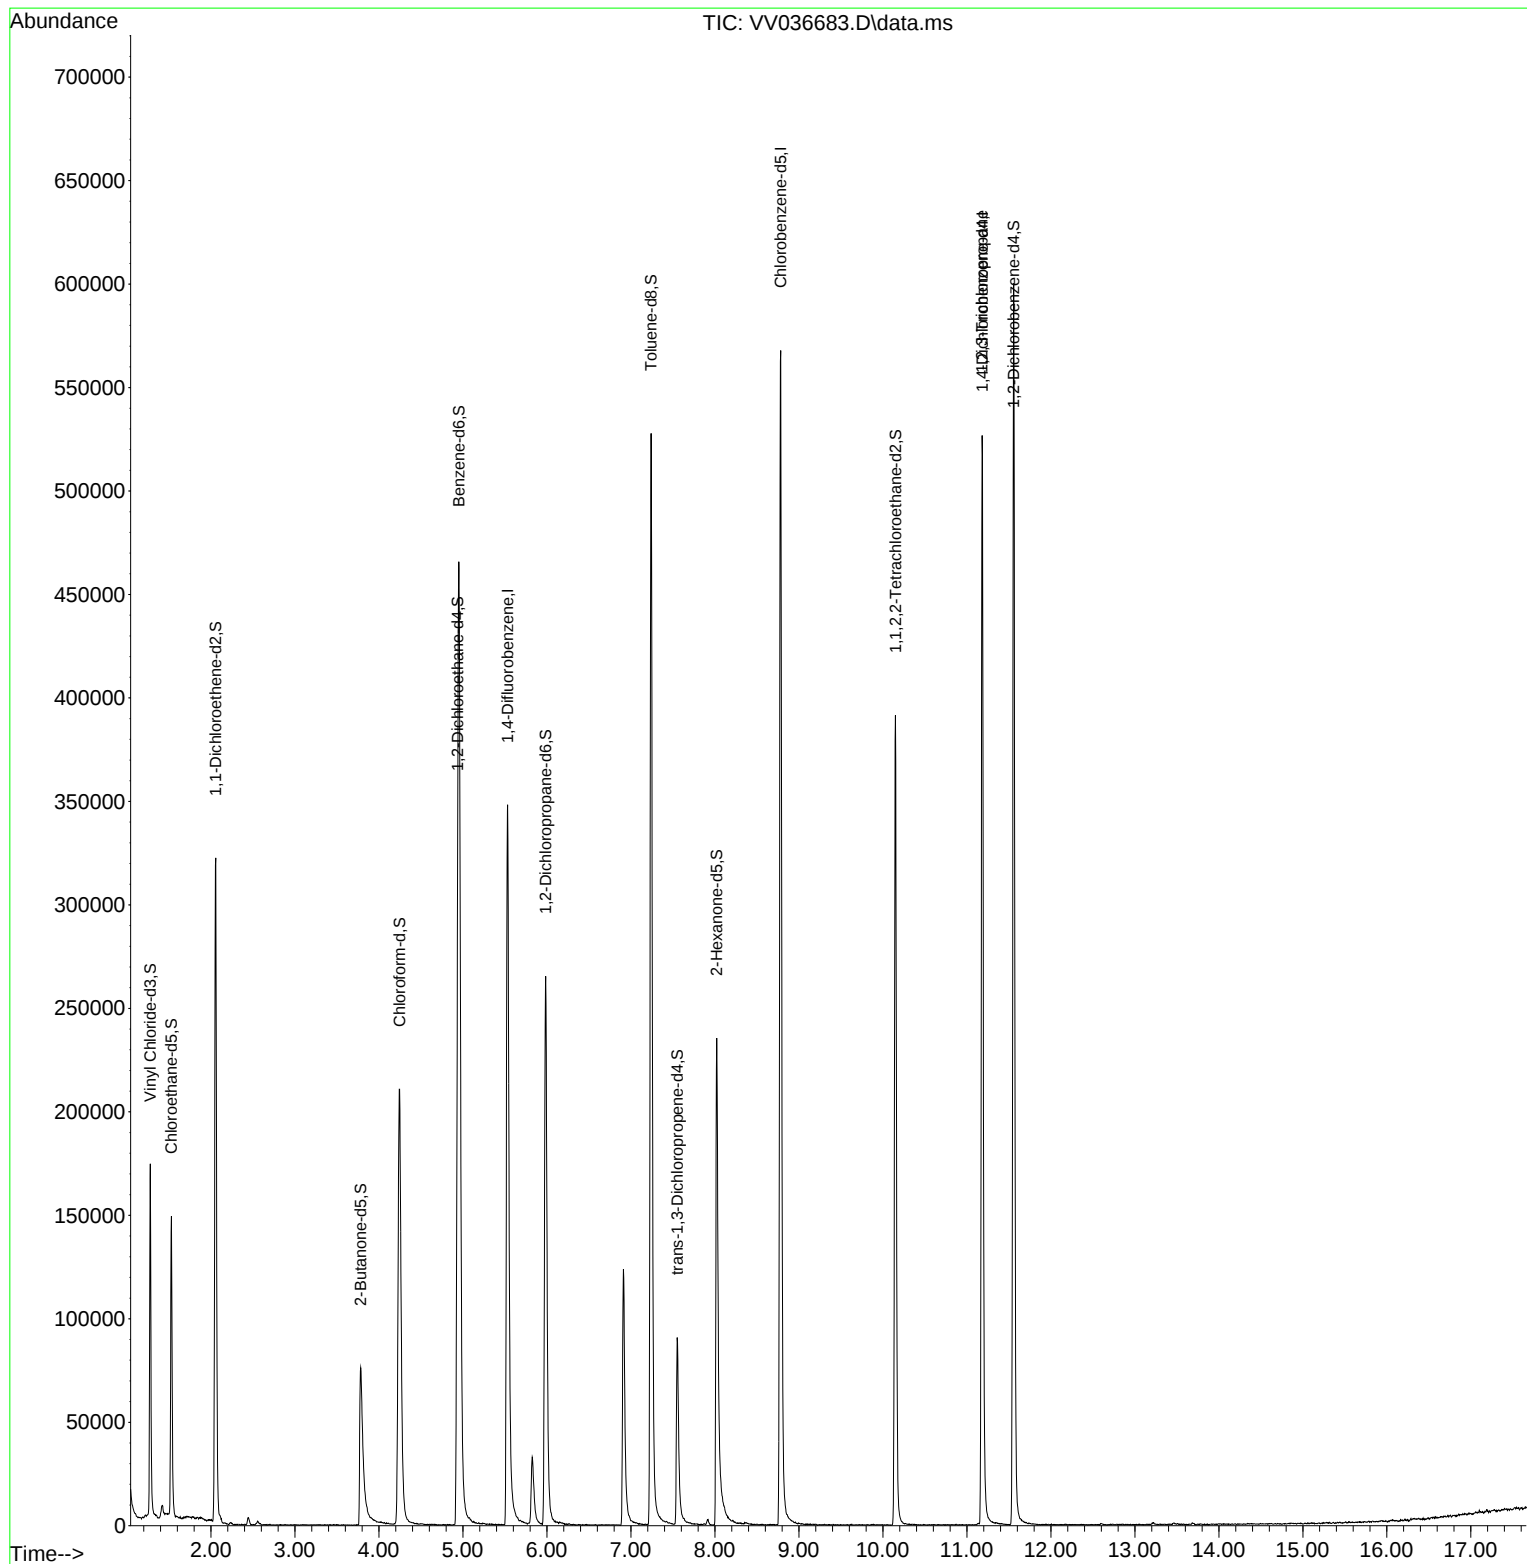

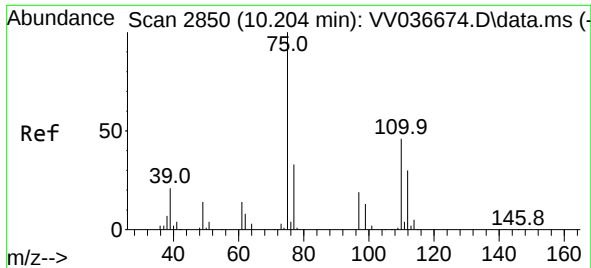

#61
 1,2,3-Trichloropropane
 Concen: 5.493 ug/L
 RT: 11.181 min Scan# 31
 Delta R.T. 0.977 min
 Lab File: VV036683.D
 Acq: 25 Jul 2024 00:09

Instrument :
 MSVOA_V
 ClientSampleId :
 E20G9

Tgt Ion: 75 Resp: 14314
 Ion Ratio Lower Upper
 75 100
 77 35.1 26.1 39.1
 110 3.0 36.7 55.1#

