

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036686.D
 Acq On : 25 Jul 2024 01:22
 Operator : SY/MD
 Sample : P3335-13 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L0

Quant Time: Jul 25 04:30:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 03:06:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	325832	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	343800	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	149938	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	103679	43.241	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.480%		
7) Chloroethane-d5	1.526	69	95066	46.307	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.620%		
11) 1,1-Dichloroethene-d2	2.053	65	50710	44.215	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.420%		
21) 2-Butanone-d5	3.780	46	107739	87.674	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	87.670%		
24) Chloroform-d	4.243	84	224121	45.653	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.300%		
26) 1,2-Dichloroethane-d4	4.937	65	144146	49.306	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.620%		
32) Benzene-d6	4.953	84	411148	45.592	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.180%		
36) 1,2-Dichloropropane-d6	5.982	67	120739	47.163	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.320%		
41) Toluene-d8	7.239	98	362618	41.224	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.440%		
43) trans-1,3-Dichloroprop...	7.554	79	54444	39.294	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.580%		
47) 2-Hexanone-d5	8.021	63	75397	79.577	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	79.580%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	171405	43.209	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	86.420%		
66) 1,2-Dichlorobenzene-d4	11.557	152	164818	53.326	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.660%		
Target Compounds						Qvalue
20) cis-1,2-Dichloroethene	3.818	96	3056	1.168	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036686.D
Acq On : 25 Jul 2024 01:22
Operator : SY/MD
Sample : P3335-13 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20L0

Quant Time: Jul 25 04:30:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 03:06:08 2024
Response via : Initial Calibration

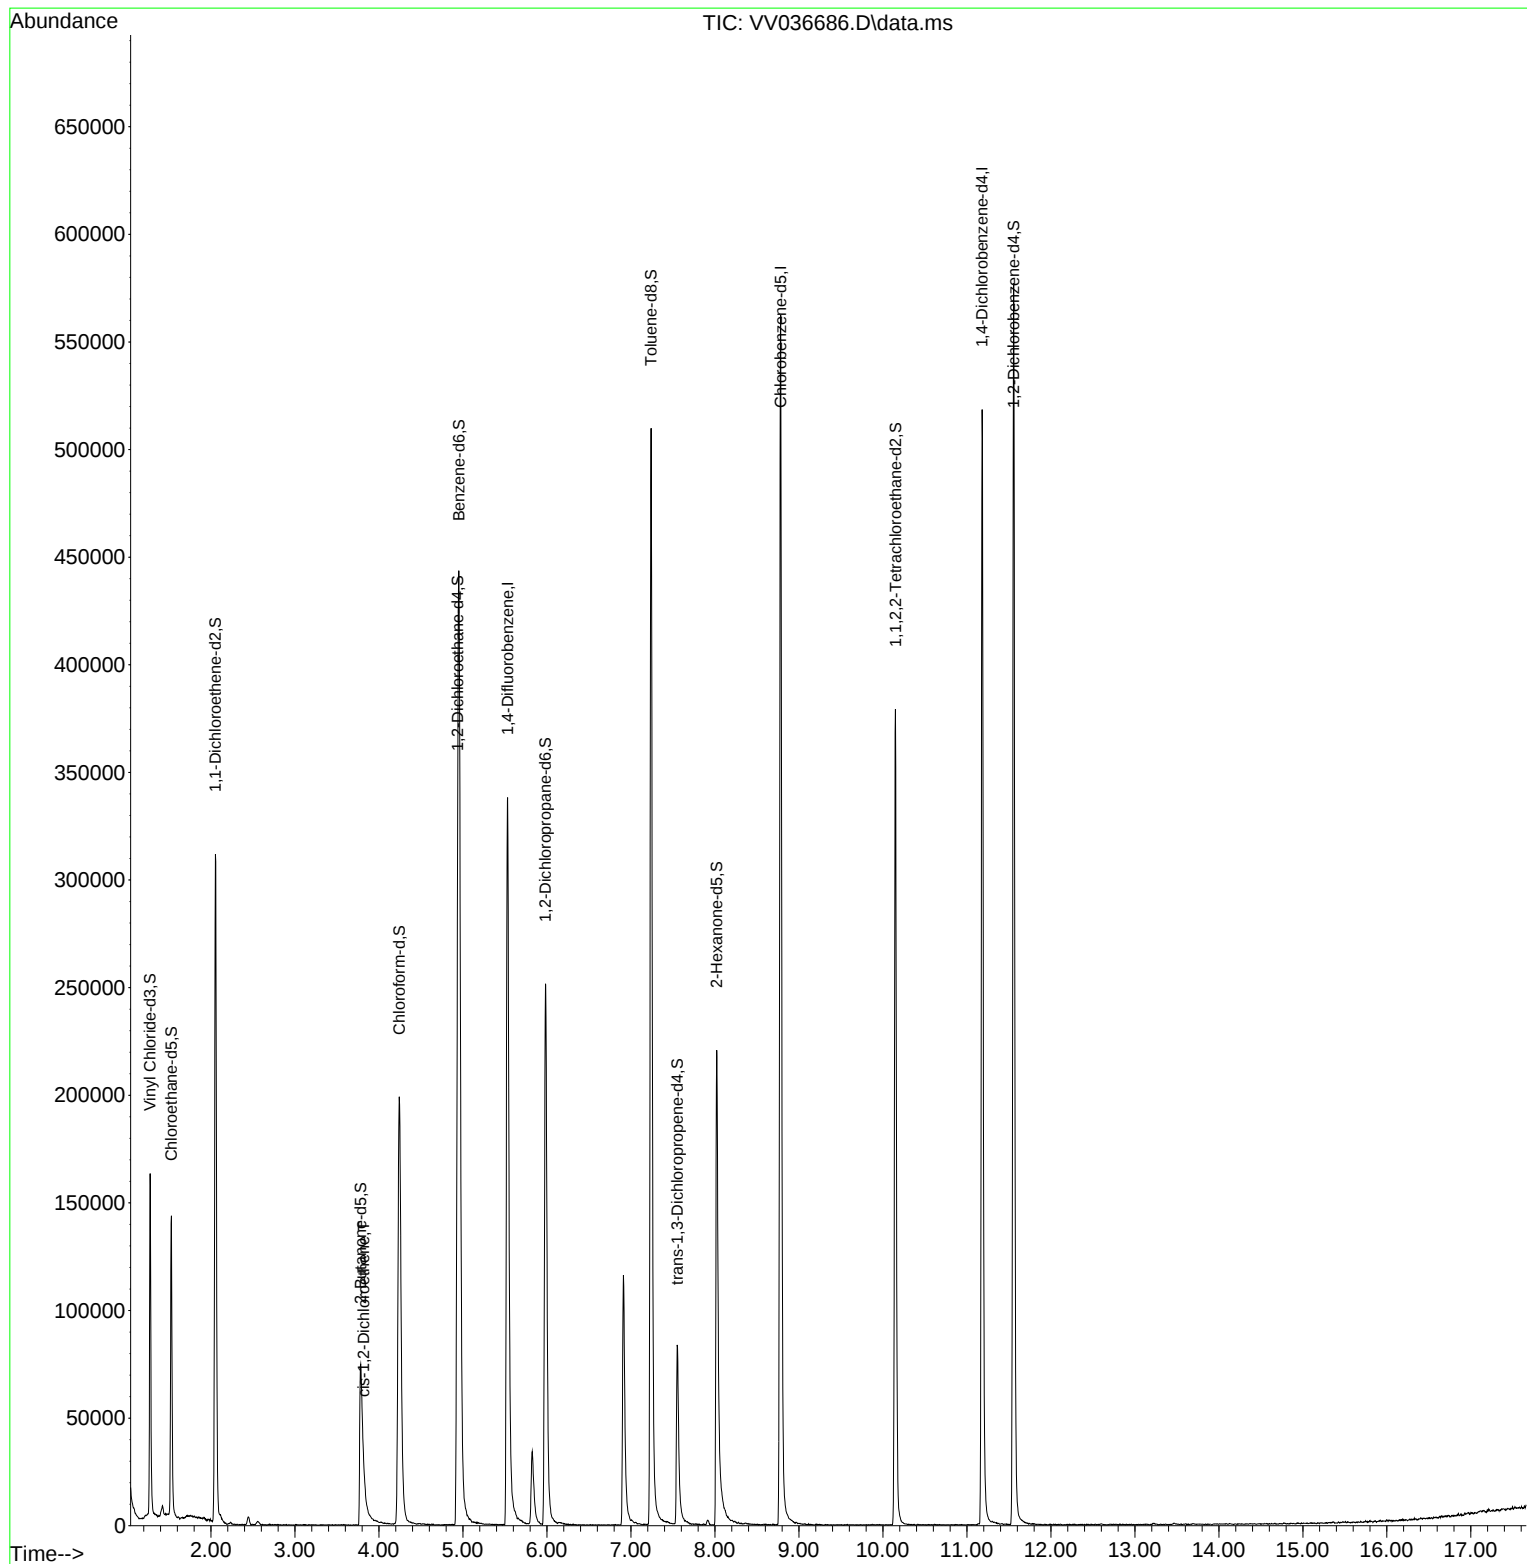

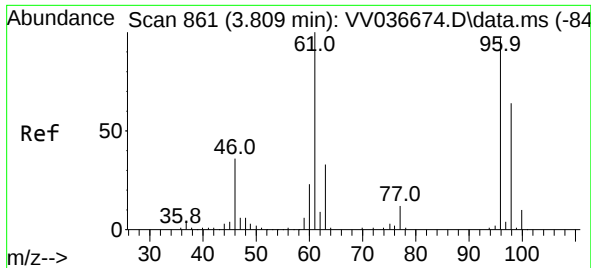

#20
 cis-1,2-Dichloroethene
 Concen: 1.168 ug/L
 RT: 3.818 min Scan# 80
 Delta R.T. 0.010 min
 Lab File: VV036686.D
 Acq: 25 Jul 2024 01:22

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L0

Tgt Ion:	96	Resp:	3056
Ion	Ratio	Lower	Upper
96	100		
61	110.1	73.4	136.2
98	51.4	45.2	84.0

