

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072524\
 Data File : VW036690.D
 Acq On : 25 Jul 2024 02:58
 Operator : SY/MD
 Sample : P3335-17 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20N0

Quant Time: Jul 25 04:31:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 03:06:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	337256	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	357939	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	155168	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	102232	41.193	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	82.380%		
7) Chloroethane-d5	1.529	69	91073	42.860	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	85.720%		
11) 1,1-Dichloroethene-d2	2.056	65	49423	41.633	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.260%		
21) 2-Butanone-d5	3.780	46	103855	81.651	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	81.650%		
24) Chloroform-d	4.243	84	221533	43.597	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.200%		
26) 1,2-Dichloroethane-d4	4.937	65	139062	45.956	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.920%		
32) Benzene-d6	4.953	84	406536	43.300	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.600%		
36) 1,2-Dichloropropane-d6	5.985	67	118732	44.547	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.100%		
41) Toluene-d8	7.239	98	361919	39.519	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	79.040%#		
43) trans-1,3-Dichloroprop...	7.551	79	51881	35.965	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.920%		
47) 2-Hexanone-d5	8.021	63	75490	76.528	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	76.530%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	167778	40.624	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	81.240%		
66) 1,2-Dichlorobenzene-d4	11.558	152	161408	50.462	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.920%		
Target Compounds						Qvalue
34) Trichloroethene	5.838	95	6315	1.918	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036690.D
Acq On : 25 Jul 2024 02:58
Operator : SY/MD
Sample : P3335-17 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20N0

Quant Time: Jul 25 04:31:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 03:06:08 2024
Response via : Initial Calibration

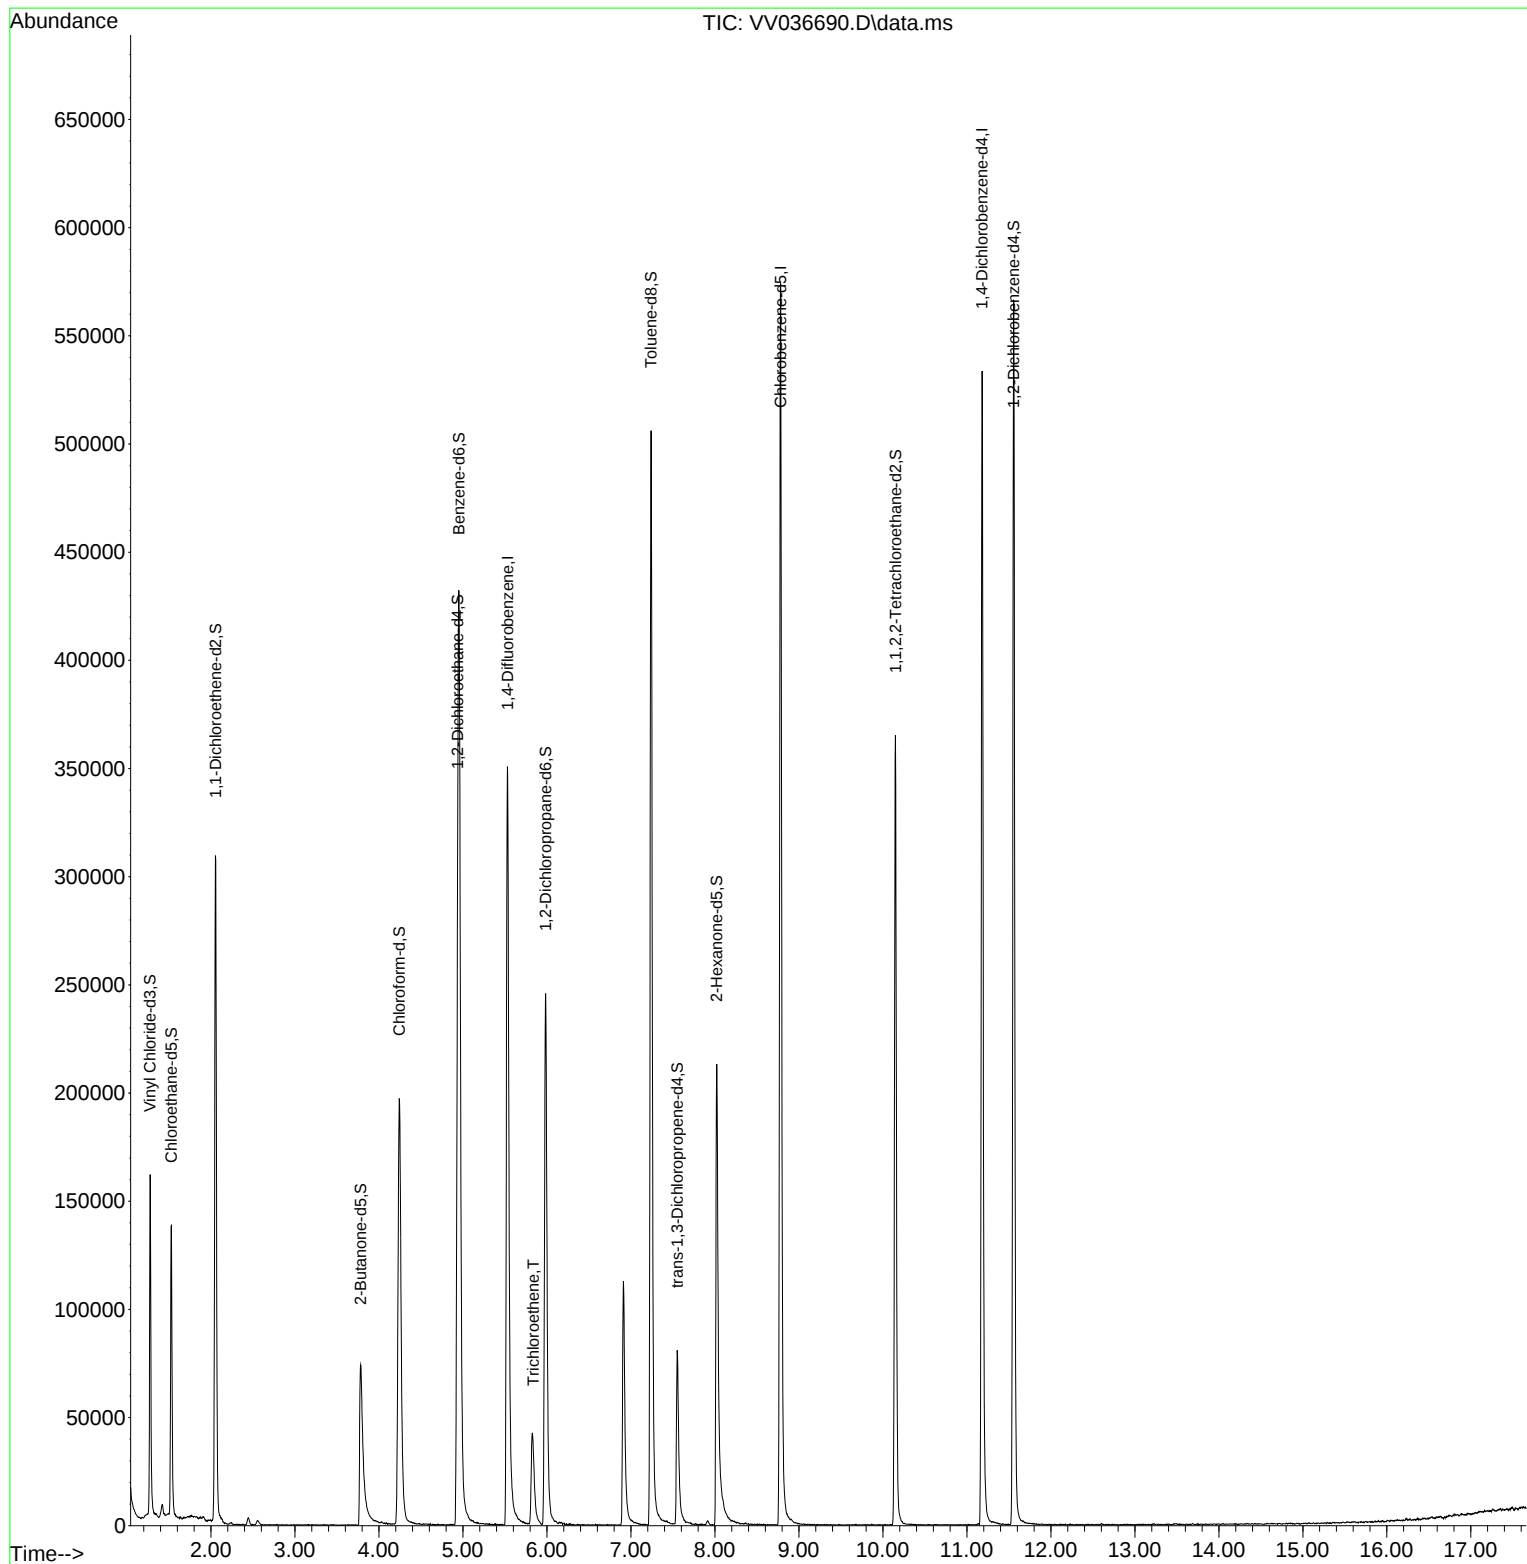

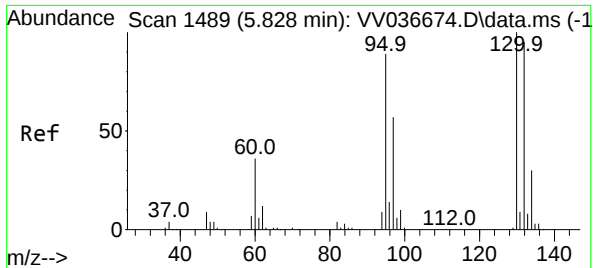

#34
 Trichloroethene
 Concen: 1.918 ug/L
 RT: 5.838 min Scan# 14
 Delta R.T. 0.010 min
 Lab File: VV036690.D
 Acq: 25 Jul 2024 02:58

Instrument :
 MSVOA_V
 ClientSampleId :
 E20N0

Tgt Ion: 95 Resp: 6315

Ion	Ratio	Lower	Upper
95	100		
97	57.7	44.7	83.1
132	104.0	74.3	138.1
130	102.8	77.8	144.4

