

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036675.D
 Acq On : 24 Jul 2024 20:55
 Operator : SY/MD
 Sample : VV0725WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK354

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M

Title : VOC Analysis

Signal : TIC: VV036675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	92	rVB	181884	193765	14.99%	1.913%
2	1.526	144	151	175	rVB	152177	189516	14.66%	1.871%
3	2.053	305	315	330	rBV	354190	510770	39.52%	5.042%
4	2.169	348	351	354	rBV4	440	414	0.03%	0.004%
5	2.233	365	371	382	rVB3	2037	3159	0.24%	0.031%
6	2.297	387	391	396	rBV2	270	272	0.02%	0.003%
7	2.378	413	416	419	rBV2	317	196	0.02%	0.002%
8	2.445	430	437	446	rVB3	1314	2233	0.17%	0.022%
9	2.548	465	469	474	rBV2	262	355	0.03%	0.004%
10	2.603	482	486	489	rBV2	202	199	0.02%	0.002%
11	2.696	509	515	524	rVB5	757	1051	0.08%	0.010%
12	2.953	591	595	597	rBV2	230	228	0.02%	0.002%
13	3.198	668	671	675	rBV2	220	225	0.02%	0.002%
14	3.278	692	696	698	rBV2	251	201	0.02%	0.002%
15	3.333	710	713	719	rVB	157	196	0.02%	0.002%
16	3.513	766	769	775	rBV2	376	369	0.03%	0.004%
17	3.696	820	826	828	rBV2	190	216	0.02%	0.002%
18	3.731	833	837	841	rBV2	215	237	0.02%	0.002%
19	3.780	844	852	893	rBV	75667	214329	16.58%	2.116%
20	4.243	980	996	1029	rBV	214815	559287	43.28%	5.520%
21	4.400	1043	1045	1050	rVB2	522	253	0.02%	0.002%
22	4.584	1100	1102	1106	rVB3	469	272	0.02%	0.003%
23	4.612	1109	1111	1115	rVB2	337	196	0.02%	0.002%
24	4.638	1115	1119	1121	rBV2	244	197	0.02%	0.002%
25	4.731	1146	1148	1151	rVV2	354	210	0.02%	0.002%
26	4.950	1195	1216	1256	rBV2	491858	1292328	100.00%	12.756%
27	5.346	1337	1339	1345	rVB3	353	216	0.02%	0.002%
28	5.452	1370	1372	1377	rBV2	241	210	0.02%	0.002%
29	5.529	1385	1396	1426	rBV	376826	796404	61.63%	7.861%
30	5.825	1477	1488	1523	rVB2	36015	85245	6.60%	0.841%
31	5.982	1523	1537	1572	rBV	275849	575558	44.54%	5.681%
32	6.227	1608	1613	1614	rBV3	261	235	0.02%	0.002%
33	6.278	1626	1629	1633	rBV2	529	347	0.03%	0.003%
34	6.362	1653	1655	1659	rVB2	296	195	0.02%	0.002%
35	6.526	1700	1706	1710	rBV2	224	329	0.03%	0.003%
36	6.911	1815	1826	1858	rBV	135309	265034	20.51%	2.616%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036675.D
 Acq On : 24 Jul 2024 20:55
 Operator : SY/MD
 Sample : VV0725WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK354

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

37	7.091	1879	1882	1886	rVB5	804	561	0.04%	0.006%
38	7.191	1908	1913	1915	rBV3	460	406	0.03%	0.004%
39	7.239	1916	1928	1961	rBV	582662	1035395	80.12%	10.220%
40	7.551	2016	2025	2058	rBV	96702	184973	14.31%	1.826%
41	7.854	2115	2119	2121	rBV2	353	283	0.02%	0.003%
42	7.908	2130	2136	2148	rVB4	3287	5286	0.41%	0.052%
43	8.021	2162	2171	2207	rBV	257845	499377	38.64%	4.929%
44	8.558	2335	2338	2340	rVB4	324	194	0.02%	0.002%
45	8.673	2371	2374	2381	rVB2	354	362	0.03%	0.004%
46	8.709	2381	2385	2395	rBV2	273	356	0.03%	0.004%
47	8.780	2395	2407	2435	rBV	620756	1025470	79.35%	10.122%
48	9.098	2504	2506	2510	rVB3	642	322	0.02%	0.003%
49	9.188	2531	2534	2540	rVB3	228	220	0.02%	0.002%
50	9.461	2616	2619	2622	rBV2	222	201	0.02%	0.002%
51	9.500	2623	2631	2633	rVV4	613	869	0.07%	0.009%
52	9.525	2636	2639	2641	rVV2	485	381	0.03%	0.004%
53	9.538	2641	2643	2647	rVB3	519	354	0.03%	0.003%
54	9.593	2656	2660	2661	rBV3	348	206	0.02%	0.002%
55	9.728	2699	2702	2710	rVV2	265	301	0.02%	0.003%
56	9.869	2741	2746	2747	rBV2	649	534	0.04%	0.005%
57	10.149	2822	2833	2866	rVV	398456	632886	48.97%	6.247%
58	10.464	2926	2931	2932	rBV	324	251	0.02%	0.002%
59	10.484	2932	2937	2944	rVV3	890	1137	0.09%	0.011%
60	10.567	2957	2963	2965	rBV2	266	304	0.02%	0.003%
61	10.619	2972	2979	2985	rBV2	207	318	0.02%	0.003%
62	10.786	3028	3031	3035	rVB2	348	273	0.02%	0.003%
63	10.818	3035	3041	3042	rBV	221	208	0.02%	0.002%
64	10.857	3048	3053	3055	rBV	743	602	0.05%	0.006%
65	10.950	3076	3082	3091	rBV	179	295	0.02%	0.003%
66	11.127	3130	3137	3144	rBV3	3417	5301	0.41%	0.052%
67	11.181	3144	3154	3185	rVV	596704	943074	72.97%	9.309%
68	11.429	3226	3231	3236	rVB3	556	611	0.05%	0.006%
69	11.558	3259	3271	3298	rBV	644860	1026558	79.43%	10.133%
70	11.924	3381	3385	3386	rBV	279	187	0.01%	0.002%
71	12.130	3443	3449	3451	rBV2	288	305	0.02%	0.003%
72	12.294	3498	3500	3506	rVB2	232	233	0.02%	0.002%
73	12.320	3506	3508	3512	rBV	268	224	0.02%	0.002%
74	12.371	3521	3524	3530	rBV3	425	389	0.03%	0.004%
75	12.586	3584	3591	3608	rBV4	4321	7901	0.61%	0.078%
76	12.741	3635	3639	3645	rBV2	284	378	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036675.D
 Acq On : 24 Jul 2024 20:55
 Operator : SY/MD
 Sample : VV0725WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK354

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

77	12.908	3686	3691	3696	rBV2	366	456	0.04%	0.005%
78	12.988	3714	3716	3721	rVB2	336	258	0.02%	0.003%
79	13.078	3739	3744	3745	rBV2	336	284	0.02%	0.003%
80	13.207	3775	3784	3796	rBV3	7520	12393	0.96%	0.122%
81	13.271	3801	3804	3809	rVB2	334	242	0.02%	0.002%
82	13.403	3839	3845	3849	rVB2	370	410	0.03%	0.004%
83	13.445	3849	3858	3875	rBV	12862	24412	1.89%	0.241%
84	13.683	3923	3932	3947	rVB3	8638	14903	1.15%	0.147%
85	13.773	3957	3960	3962	rBV2	510	275	0.02%	0.003%
86	13.847	3978	3983	3984	rBV2	235	207	0.02%	0.002%
87	13.853	3984	3985	3989	rVB	417	208	0.02%	0.002%
88	13.901	3997	4000	4002	rBV	344	256	0.02%	0.003%
89	14.146	4072	4076	4078	rBV2	397	275	0.02%	0.003%
90	14.869	4299	4301	4304	rVB3	380	213	0.02%	0.002%
91	14.885	4304	4306	4310	rVB2	515	293	0.02%	0.003%
92	14.908	4310	4313	4315	rBV3	508	248	0.02%	0.002%
93	14.943	4322	4324	4327	rBV	280	216	0.02%	0.002%
94	15.062	4358	4361	4366	rVB3	451	473	0.04%	0.005%
95	15.091	4366	4370	4371	rBV2	404	303	0.02%	0.003%
96	15.191	4399	4401	4407	rVB3	543	339	0.03%	0.003%
97	15.551	4510	4513	4516	rBV3	503	390	0.03%	0.004%
98	15.766	4577	4580	4582	rBV4	603	381	0.03%	0.004%
99	15.779	4582	4584	4592	rVV5	730	808	0.06%	0.008%
100	15.818	4592	4596	4599	rBV4	982	952	0.07%	0.009%




Sum of corrected areas: 10131128

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036675.D
Acq On : 24 Jul 2024 20:55
Operator : SY/MD
Sample : VV0725WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK354

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

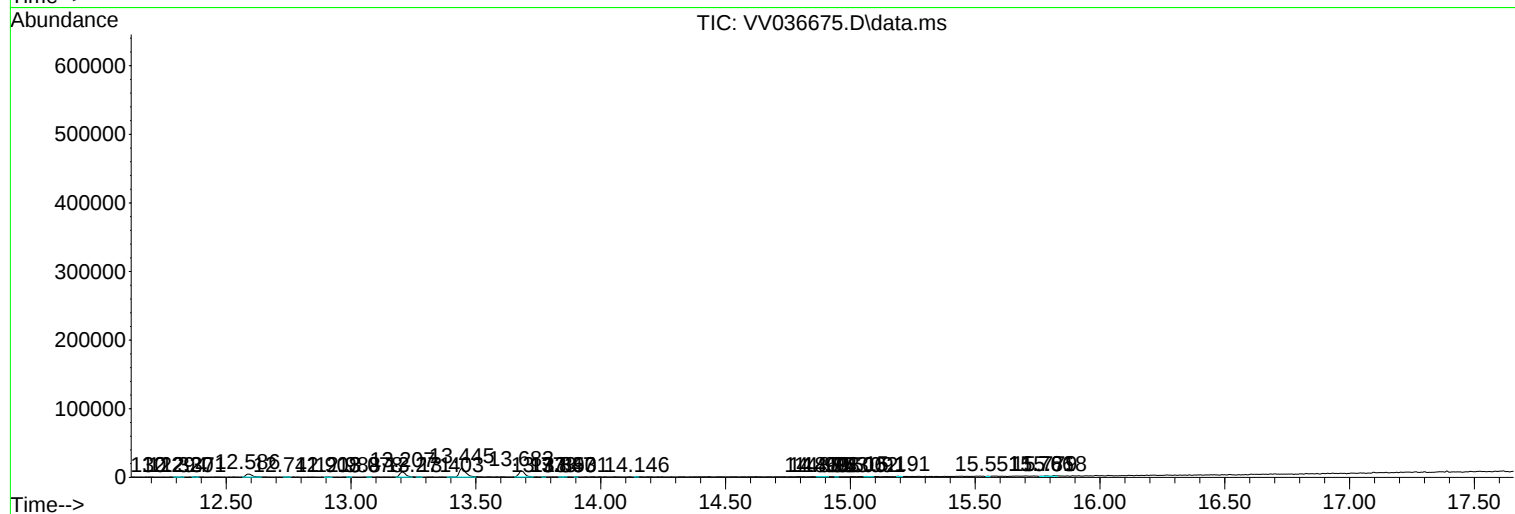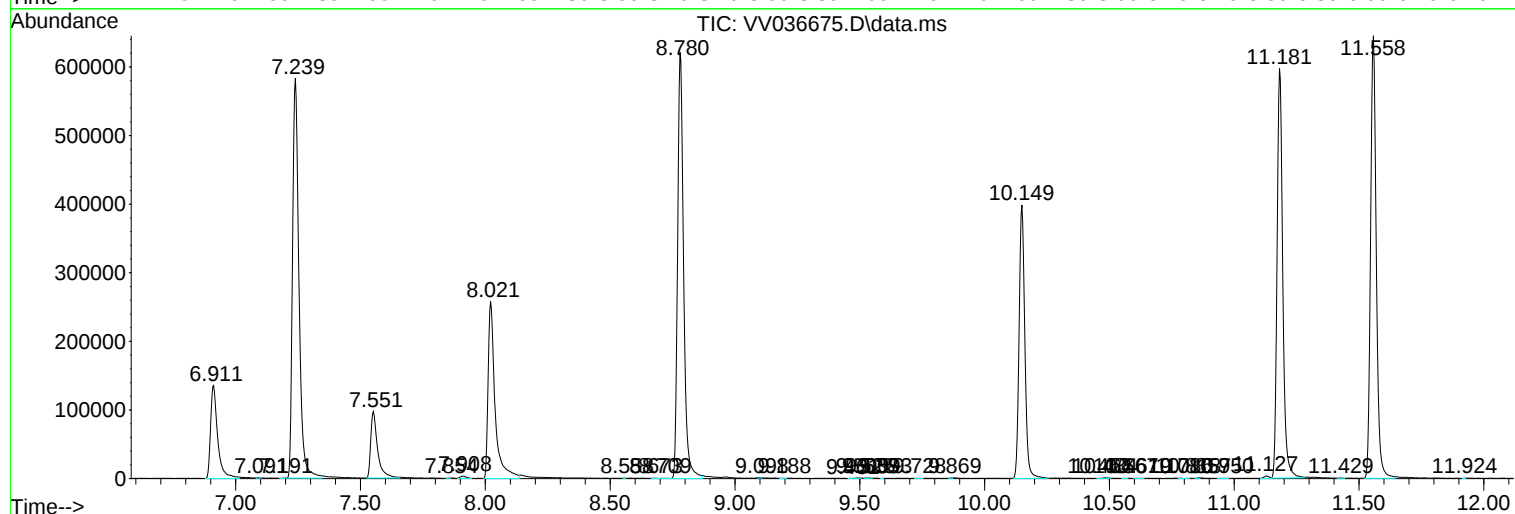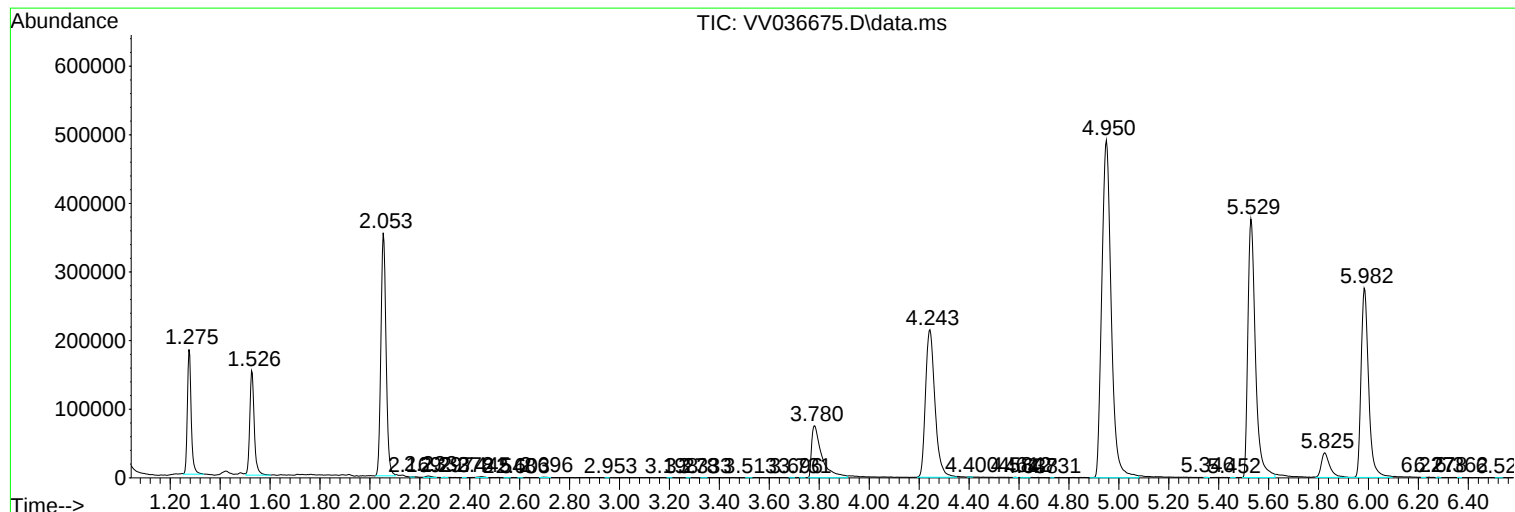

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036675.D
Acq On : 24 Jul 2024 20:55
Operator : SY/MD
Sample : VV0725WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK354

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036675.D
Acq On : 24 Jul 2024 20:55
Operator : SY/MD
Sample : VV0725WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK354

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------