

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036676.D
 Acq On : 24 Jul 2024 21:19
 Operator : SY/MD
 Sample : P3335-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M

Title : VOC Analysis

Signal : TIC: VV036676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	89	rVB	175548	186464	14.69%	1.872%
2	1.529	145	152	170	rVB	145907	179158	14.11%	1.798%
3	2.053	306	315	328	rBV	337606	497643	39.20%	4.995%
4	2.326	395	400	403	rBV2	521	465	0.04%	0.005%
5	2.445	430	437	446	rVB4	3237	5480	0.43%	0.055%
6	2.558	466	472	475	rBV2	391	497	0.04%	0.005%
7	2.600	484	485	486	rBV2	83	31	0.00%	0.000%
8	2.632	491	495	496	rBV2	324	153	0.01%	0.002%
9	2.667	504	506	507	rBV2	173	59	0.00%	0.001%
10	2.699	507	516	531	rVB4	4254	8660	0.68%	0.087%
11	2.809	548	550	551	rBV	152	64	0.01%	0.001%
12	2.915	582	583	584	rBV	211	60	0.00%	0.001%
13	2.928	584	587	591	rVB2	350	271	0.02%	0.003%
14	2.953	591	595	599	rBV	323	262	0.02%	0.003%
15	2.973	599	601	604	rBV	181	77	0.01%	0.001%
16	3.018	613	615	617	rBV2	233	97	0.01%	0.001%
17	3.085	634	636	638	rBV2	268	108	0.01%	0.001%
18	3.114	638	645	654	rVV5	979	1786	0.14%	0.018%
19	3.230	678	681	686	rBV	252	211	0.02%	0.002%
20	3.249	686	687	691	rVB	276	132	0.01%	0.001%
21	3.268	691	693	695	rBV2	127	64	0.01%	0.001%
22	3.285	695	698	699	rBV2	190	113	0.01%	0.001%
23	3.307	703	705	706	rBV2	116	25	0.00%	0.000%
24	3.317	706	708	710	rBV	125	77	0.01%	0.001%
25	3.378	726	727	728	rBV	65	20	0.00%	0.000%
26	3.387	728	730	731	rBV	153	46	0.00%	0.000%
27	3.439	744	746	749	rBV2	247	161	0.01%	0.002%
28	3.461	752	753	755	rVB	46	16	0.00%	0.000%
29	3.477	755	758	761	rBV	204	149	0.01%	0.001%
30	3.516	768	770	771	rBV	81	28	0.00%	0.000%
31	3.561	781	784	787	rBV	243	144	0.01%	0.001%
32	3.712	829	831	832	rBV	190	57	0.00%	0.001%
33	3.744	837	841	844	rBV	204	198	0.02%	0.002%
34	3.783	845	853	894	rBV	72416	214872	16.92%	2.157%
35	4.243	982	996	1032	rBV	206608	540731	42.59%	5.428%
36	4.738	1138	1150	1157	rBV4	2182	4518	0.36%	0.045%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036676.D
 Acq On : 24 Jul 2024 21:19
 Operator : SY/MD
 Sample : P3335-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

37	4.802	1167	1170	1172	rBV2	371	187	0.01%	0.002%
38	4.950	1200	1216	1271	rBV2	474195	1269569	100.00%	12.744%
39	5.368	1344	1346	1349	rBV	246	142	0.01%	0.001%
40	5.529	1386	1396	1436	rBV	365743	785024	61.83%	7.880%
41	5.825	1477	1488	1507	rBV5	38241	88461	6.97%	0.888%
42	5.985	1526	1538	1568	rBV	266939	559418	44.06%	5.615%
43	6.255	1619	1622	1624	rBV3	510	246	0.02%	0.002%
44	6.336	1644	1647	1650	rVB3	366	260	0.02%	0.003%
45	6.352	1650	1652	1653	rBV3	131	39	0.00%	0.000%
46	6.448	1670	1682	1690	rBV5	1568	3222	0.25%	0.032%
47	6.616	1732	1734	1735	rBV	115	26	0.00%	0.000%
48	6.712	1762	1764	1765	rVB	123	31	0.00%	0.000%
49	6.911	1815	1826	1861	rBV	133321	266275	20.97%	2.673%
50	7.239	1917	1928	1951	rBV	564804	998988	78.69%	10.028%
51	7.551	2016	2025	2050	rBV	92904	179376	14.13%	1.801%
52	7.789	2090	2099	2112	rVB7	2498	5127	0.40%	0.051%
53	7.876	2120	2126	2129	rBV3	1894	2111	0.17%	0.021%
54	8.021	2162	2171	2209	rBV	235898	480379	37.84%	4.822%
55	8.525	2325	2328	2330	rBV2	368	234	0.02%	0.002%
56	8.561	2337	2339	2340	rBV	319	158	0.01%	0.002%
57	8.609	2353	2354	2358	rVB2	337	166	0.01%	0.002%
58	8.625	2358	2359	2360	rBV2	214	61	0.00%	0.001%
59	8.783	2391	2408	2449	rBV	599659	1027898	80.96%	10.318%
60	9.088	2496	2503	2515	rVB4	3288	5506	0.43%	0.055%
61	9.156	2521	2524	2525	rBV	211	122	0.01%	0.001%
62	9.249	2551	2553	2555	rVB	233	90	0.01%	0.001%
63	9.262	2555	2557	2562	rVB2	290	201	0.02%	0.002%
64	9.329	2576	2578	2581	rBB	221	102	0.01%	0.001%
65	9.345	2581	2583	2585	rBV	229	133	0.01%	0.001%
66	9.442	2611	2613	2618	rVB2	259	152	0.01%	0.002%
67	9.487	2618	2627	2632	rBV5	4305	6797	0.54%	0.068%
68	9.673	2678	2685	2697	rBV4	1725	2643	0.21%	0.027%
69	9.722	2697	2700	2702	rVB	200	97	0.01%	0.001%
70	9.754	2708	2710	2711	rBV	182	73	0.01%	0.001%
71	9.873	2738	2747	2753	rBV3	4469	6681	0.53%	0.067%
72	9.963	2769	2775	2782	rBV4	406	465	0.04%	0.005%
73	9.992	2782	2784	2789	rBV2	221	203	0.02%	0.002%
74	10.059	2803	2805	2809	rBV2	189	122	0.01%	0.001%
75	10.149	2822	2833	2849	rBV	380882	608693	47.94%	6.110%
76	10.445	2922	2925	2928	rBV2	291	189	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036676.D
 Acq On : 24 Jul 2024 21:19
 Operator : SY/MD
 Sample : P3335-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

77	10.480	2928	2936	2951	rVV4	3573	5976	0.47%	0.060%
78	10.709	3001	3007	3011	rBV2	317	339	0.03%	0.003%
79	10.789	3023	3032	3034	rBV2	206	337	0.03%	0.003%
80	10.857	3046	3053	3071	rVB3	4023	7337	0.58%	0.074%
81	10.921	3071	3073	3080	rBV2	355	426	0.03%	0.004%
82	11.056	3112	3115	3121	rBV3	289	271	0.02%	0.003%
83	11.127	3130	3137	3144	rBV2	6688	9433	0.74%	0.095%
84	11.181	3144	3154	3183	rVV	581280	930747	73.31%	9.343%
85	11.480	3241	3247	3250	rBV3	587	562	0.04%	0.006%
86	11.558	3260	3271	3295	rBV	629278	1001420	78.88%	10.052%
87	11.786	3340	3342	3347	rBV3	394	253	0.02%	0.003%
88	12.094	3434	3438	3439	rBV2	366	247	0.02%	0.002%
89	12.194	3465	3469	3471	rBV3	278	239	0.02%	0.002%
90	12.316	3505	3507	3508	rBV3	277	139	0.01%	0.001%
91	12.339	3513	3514	3516	rBV3	320	107	0.01%	0.001%
92	12.586	3583	3591	3601	rBV2	8174	13074	1.03%	0.131%
93	13.078	3742	3744	3746	rBV2	247	168	0.01%	0.002%
94	13.204	3775	3783	3794	rBV2	8659	14388	1.13%	0.144%
95	13.445	3850	3858	3874	rBV2	10259	19157	1.51%	0.192%
96	13.683	3924	3932	3945	rBV3	9636	14753	1.16%	0.148%
97	13.805	3967	3970	3972	rBV	357	234	0.02%	0.002%
98	13.911	4001	4003	4005	rBV	289	156	0.01%	0.002%




Sum of corrected areas: 9962327

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036676.D
Acq On : 24 Jul 2024 21:19
Operator : SY/MD
Sample : P3335-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

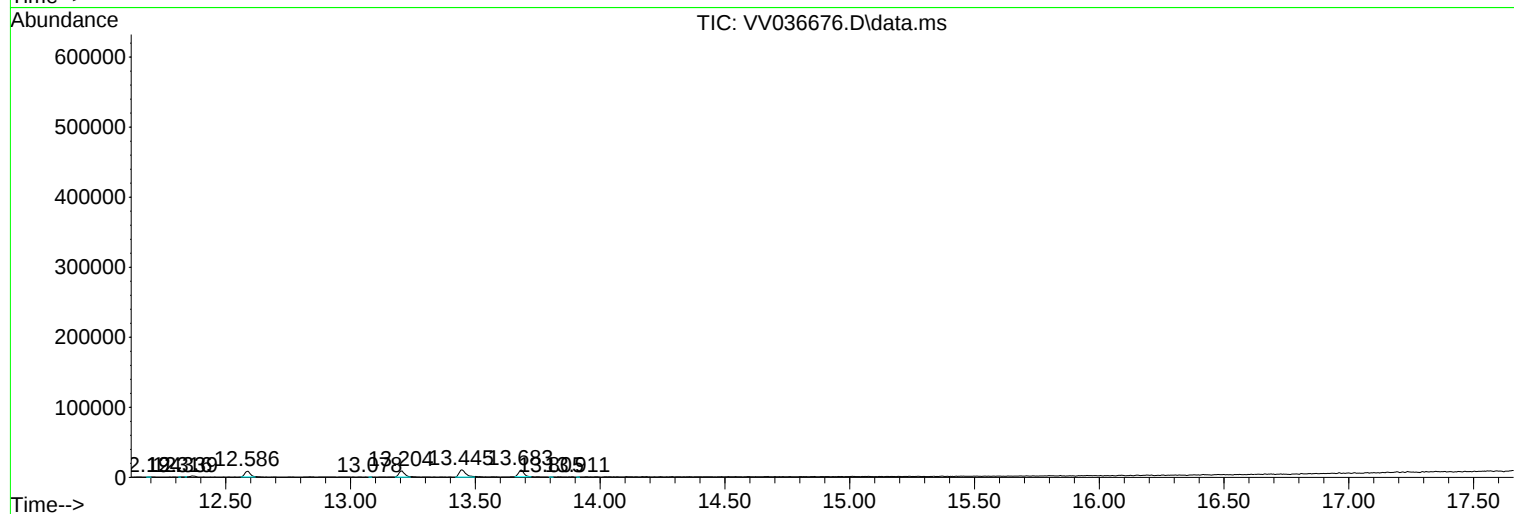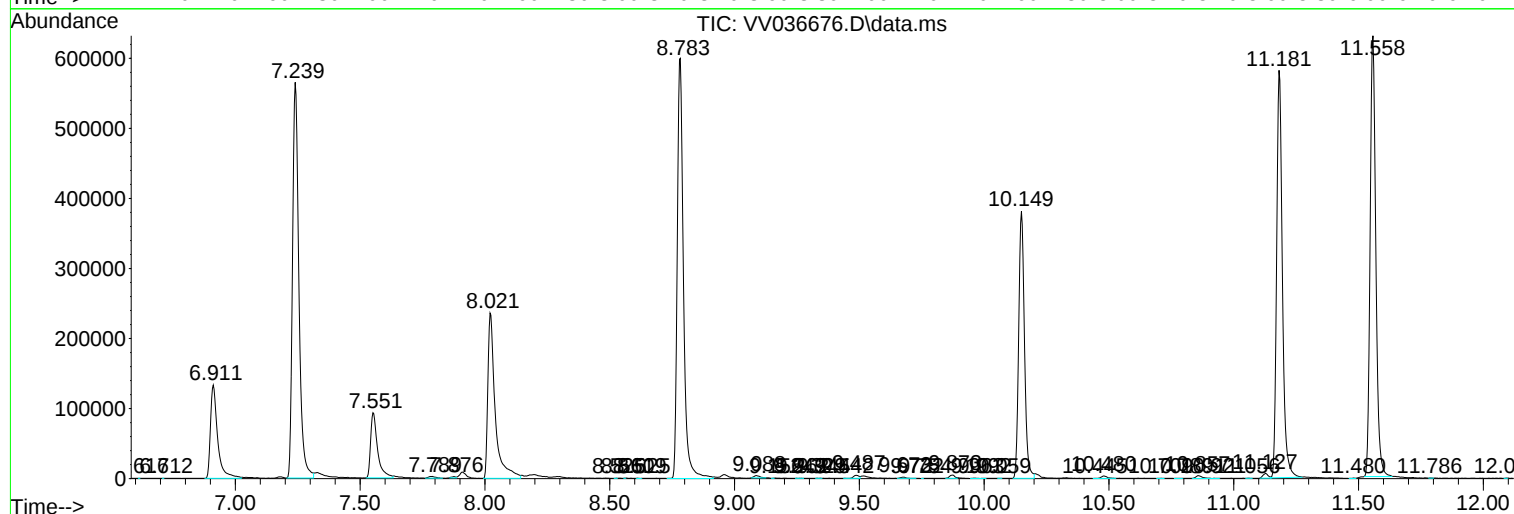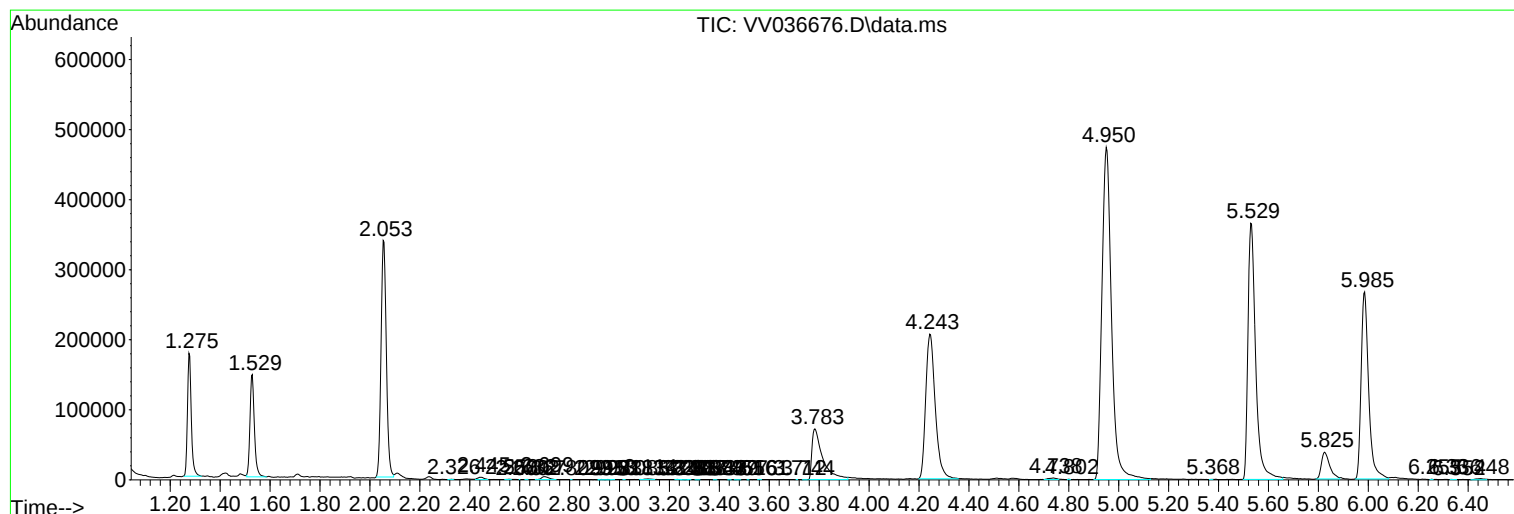

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036676.D
Acq On : 24 Jul 2024 21:19
Operator : SY/MD
Sample : P3335-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036676.D
Acq On : 24 Jul 2024 21:19
Operator : SY/MD
Sample : P3335-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------