

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036677.D
 Acq On : 24 Jul 2024 21:44
 Operator : SY/MD
 Sample : P3335-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

Signal : TIC: VV036677.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	90	rVB	172174	185657	14.96%	1.876%
2	1.529	144	152	170	rVB	144810	175100	14.11%	1.770%
3	2.053	305	315	328	rBV	335885	490889	39.56%	4.961%
4	2.224	359	368	388	rVB	19759	37113	2.99%	0.375%
5	2.368	411	413	417	rVB2	357	200	0.02%	0.002%
6	2.442	431	436	439	rBV5	848	811	0.07%	0.008%
7	2.487	447	450	457	rVB2	354	395	0.03%	0.004%
8	2.519	457	460	461	rBV	371	211	0.02%	0.002%
9	2.558	461	472	484	rVV4	2029	4891	0.39%	0.049%
10	2.613	487	489	494	rVV2	279	208	0.02%	0.002%
11	2.693	511	514	515	rBV2	531	313	0.03%	0.003%
12	3.072	624	632	636	rBV	365	443	0.04%	0.004%
13	3.355	713	720	721	rBV	337	287	0.02%	0.003%
14	3.561	781	784	791	rBV2	342	412	0.03%	0.004%
15	3.677	815	820	824	rBV2	170	189	0.02%	0.002%
16	3.783	844	853	886	rBV	77111	226351	18.24%	2.288%
17	4.243	981	996	1029	rBV	208585	542871	43.75%	5.487%
18	4.564	1094	1096	1100	rBV	415	343	0.03%	0.003%
19	4.619	1110	1113	1118	rVB2	512	451	0.04%	0.005%
20	4.648	1118	1122	1126	rBV3	243	269	0.02%	0.003%
21	4.850	1178	1185	1186	rBV	239	261	0.02%	0.003%
22	4.950	1198	1216	1245	rBV2	472072	1240859	100.00%	12.541%
23	5.397	1352	1355	1358	rVB2	278	207	0.02%	0.002%
24	5.529	1384	1396	1428	rBV	383780	804839	64.86%	8.134%
25	5.821	1476	1487	1523	rVB3	54113	123930	9.99%	1.253%
26	5.985	1525	1538	1576	rBV	261312	554021	44.65%	5.599%
27	6.275	1624	1628	1635	rVB4	531	604	0.05%	0.006%
28	6.307	1635	1638	1644	rVB3	423	340	0.03%	0.003%
29	6.342	1647	1649	1651	rVV	501	207	0.02%	0.002%
30	6.516	1700	1703	1705	rVV2	320	200	0.02%	0.002%
31	6.722	1761	1767	1772	rBV2	159	199	0.02%	0.002%
32	6.911	1815	1826	1858	rBV	129688	258103	20.80%	2.609%
33	7.127	1889	1893	1896	rBV2	260	236	0.02%	0.002%
34	7.185	1907	1911	1916	rBV3	378	323	0.03%	0.003%
35	7.239	1916	1928	1963	rBV	559115	997299	80.37%	10.079%
36	7.551	2016	2025	2058	rBV	92474	178971	14.42%	1.809%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036677.D
 Acq On : 24 Jul 2024 21:44
 Operator : SY/MD
 Sample : P3335-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

37	7.847	2115	2117	2119	rVV	607	344	0.03%	0.003%
38	7.876	2119	2126	2131	rVV4	2293	3342	0.27%	0.034%
39	7.911	2131	2137	2149	rVB3	4338	6788	0.55%	0.069%
40	8.024	2163	2172	2217	rBV	234509	485902	39.16%	4.911%
41	8.474	2308	2312	2316	rVB3	259	273	0.02%	0.003%
42	8.567	2336	2341	2344	rBV3	260	237	0.02%	0.002%
43	8.661	2364	2370	2372	rBV2	226	263	0.02%	0.003%
44	8.693	2375	2380	2382	rBV	315	250	0.02%	0.003%
45	8.783	2396	2408	2447	rBV	615097	1034073	83.34%	10.451%
46	9.011	2477	2479	2489	rVB4	639	695	0.06%	0.007%
47	9.095	2498	2505	2515	rBV5	898	1375	0.11%	0.014%
48	9.178	2527	2531	2536	rVV4	459	434	0.03%	0.004%
49	9.262	2550	2557	2563	rBV3	300	447	0.04%	0.005%
50	9.368	2584	2590	2596	rVB2	418	555	0.04%	0.006%
51	9.416	2600	2605	2607	rBV	297	230	0.02%	0.002%
52	9.497	2624	2630	2634	rBV3	703	737	0.06%	0.007%
53	9.532	2637	2641	2642	rBV2	615	471	0.04%	0.005%
54	9.706	2686	2695	2697	rBV	197	260	0.02%	0.003%
55	9.870	2739	2746	2747	rBV2	632	612	0.05%	0.006%
56	10.149	2821	2833	2858	rBV	350801	558325	45.00%	5.643%
57	10.268	2868	2870	2875	rVB2	317	195	0.02%	0.002%
58	10.307	2879	2882	2883	rBV2	506	243	0.02%	0.002%
59	10.320	2883	2886	2895	rVB4	1377	1642	0.13%	0.017%
60	10.484	2930	2937	2942	rBV3	512	744	0.06%	0.008%
61	10.558	2956	2960	2961	rBV	341	211	0.02%	0.002%
62	10.860	3050	3054	3055	rBV2	743	423	0.03%	0.004%
63	10.937	3075	3078	3082	rBV2	203	202	0.02%	0.002%
64	11.133	3130	3139	3144	rBV6	2406	3551	0.29%	0.036%
65	11.181	3144	3154	3181	rBV	592567	932621	75.16%	9.426%
66	11.513	3248	3257	3260	rVV5	2872	4667	0.38%	0.047%
67	11.558	3260	3271	3296	rVB	612940	988333	79.65%	9.989%
68	11.779	3338	3340	3342	rVB3	464	187	0.02%	0.002%
69	11.796	3342	3345	3350	rVB4	386	349	0.03%	0.004%
70	11.834	3354	3357	3361	rBV3	328	303	0.02%	0.003%
71	11.931	3384	3387	3391	rVB4	206	202	0.02%	0.002%
72	12.008	3406	3411	3418	rBV3	328	452	0.04%	0.005%
73	12.130	3445	3449	3451	rBV2	223	199	0.02%	0.002%
74	12.188	3464	3467	3470	rBV2	314	257	0.02%	0.003%
75	12.294	3497	3500	3502	rBV2	322	233	0.02%	0.002%
76	12.371	3522	3524	3530	rVB3	378	252	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036677.D
 Acq On : 24 Jul 2024 21:44
 Operator : SY/MD
 Sample : P3335-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

77	12.413	3533	3537	3538	rBV	319	210	0.02%	0.002%
78	12.448	3543	3548	3550	rBV2	336	270	0.02%	0.003%
79	12.490	3558	3561	3566	rVB	311	249	0.02%	0.003%
80	12.519	3566	3570	3574	rBV2	238	257	0.02%	0.003%
81	12.541	3574	3577	3578	rBV	473	229	0.02%	0.002%
82	12.586	3584	3591	3603	rBV5	3240	5188	0.42%	0.052%
83	12.673	3611	3618	3622	rBV3	420	501	0.04%	0.005%
84	12.731	3631	3636	3640	rBV3	378	342	0.03%	0.003%
85	12.857	3670	3675	3679	rBV2	447	457	0.04%	0.005%
86	12.963	3706	3708	3713	rBV2	397	368	0.03%	0.004%
87	13.207	3775	3784	3792	rBV3	4578	7215	0.58%	0.073%
88	13.300	3811	3813	3820	rVB4	216	212	0.02%	0.002%
89	13.448	3849	3859	3870	rBV2	5916	9778	0.79%	0.099%
90	13.612	3908	3910	3913	rVV2	233	187	0.02%	0.002%
91	13.686	3925	3933	3946	rVB4	4556	7488	0.60%	0.076%
92	13.750	3950	3953	3957	rBV	248	181	0.01%	0.002%
93	13.873	3988	3991	3995	rVB3	372	267	0.02%	0.003%
94	13.956	4010	4017	4022	rBV2	338	564	0.05%	0.006%
95	13.985	4023	4026	4029	rVB2	291	202	0.02%	0.002%
96	14.654	4232	4234	4238	rBV	254	192	0.02%	0.002%
97	14.783	4272	4274	4276	rBV2	335	179	0.01%	0.002%
98	14.975	4331	4334	4335	rBV	290	180	0.01%	0.002%
99	15.278	4424	4428	4430	rVB4	793	579	0.05%	0.006%
100	15.770	4579	4581	4585	rVB4	790	385	0.03%	0.004%




Sum of corrected areas: 9894562

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036677.D
Acq On : 24 Jul 2024 21:44
Operator : SY/MD
Sample : P3335-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

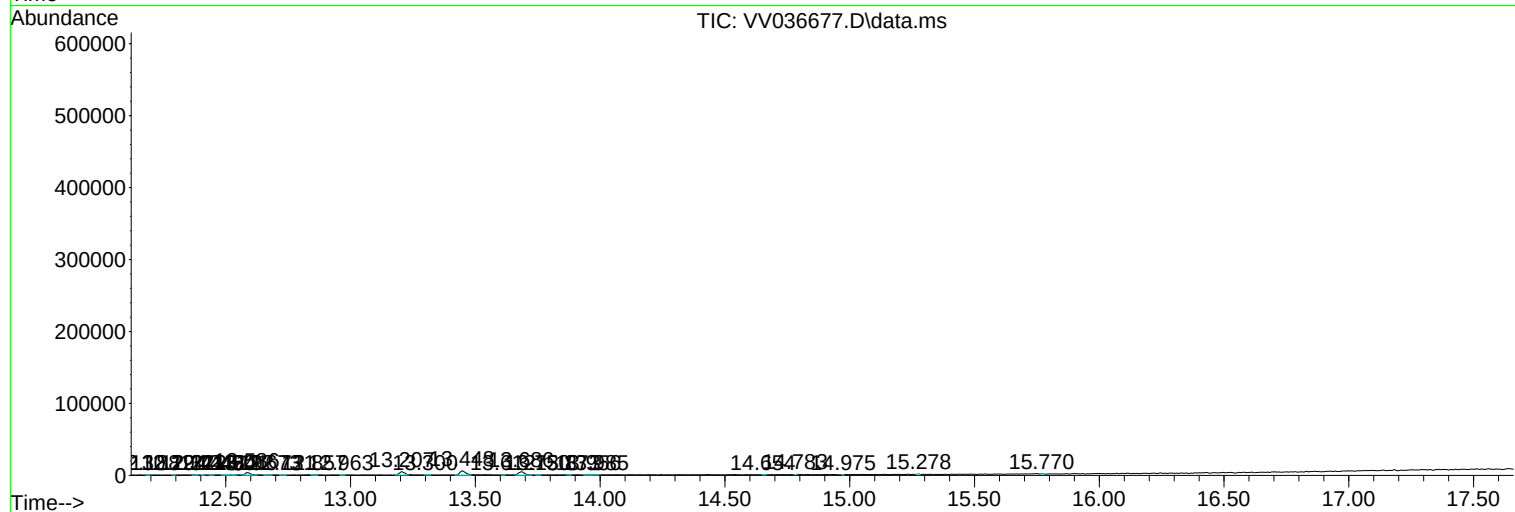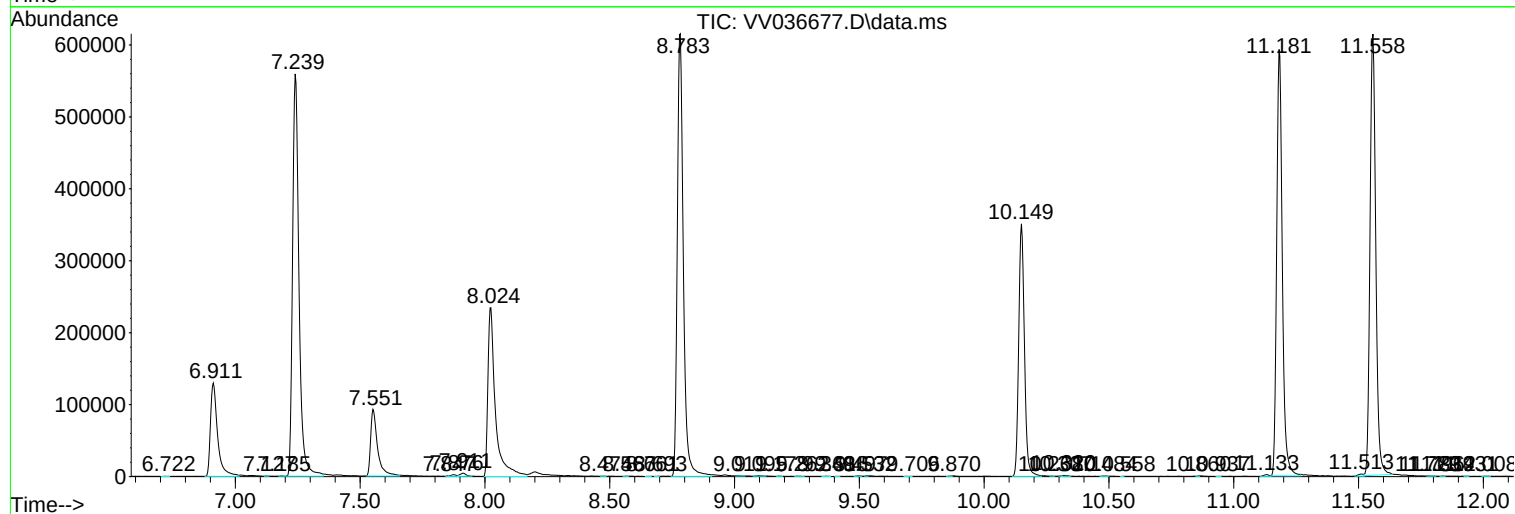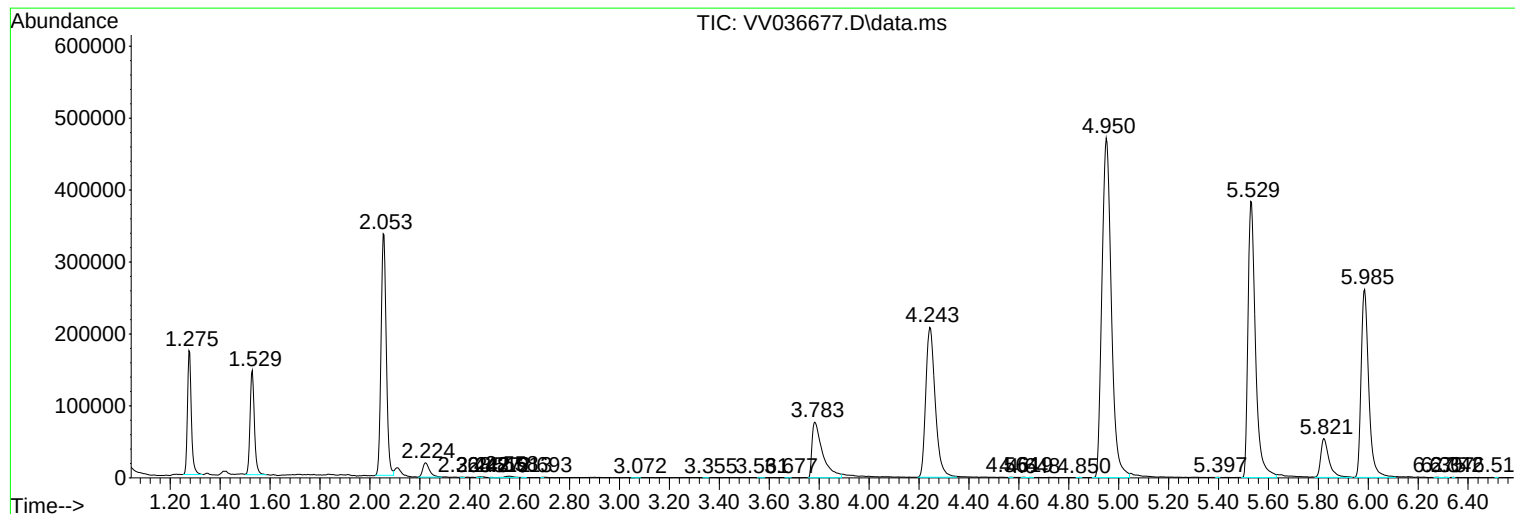

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036677.D
Acq On : 24 Jul 2024 21:44
Operator : SY/MD
Sample : P3335-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036677.D
Acq On : 24 Jul 2024 21:44
Operator : SY/MD
Sample : P3335-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc