

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036678.D
 Acq On : 24 Jul 2024 22:08
 Operator : SY/MD
 Sample : P3335-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

Signal : TIC: VV036678.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	91	rVB	165640	178431	14.60%	1.863%
2	1.420	112	118	126	rBV8	4704	7653	0.63%	0.080%
3	1.529	144	152	170	rVB	143796	174115	14.25%	1.818%
4	2.056	305	316	329	rBV	333389	486015	39.77%	5.075%
5	2.230	359	370	380	rBV4	5822	11647	0.95%	0.122%
6	2.310	391	395	396	rBV	293	216	0.02%	0.002%
7	2.381	414	417	420	rBV2	335	287	0.02%	0.003%
8	2.442	431	436	450	rVB5	1391	2116	0.17%	0.022%
9	2.555	468	471	472	rBV2	314	192	0.02%	0.002%
10	2.629	490	494	498	rBV	194	230	0.02%	0.002%
11	2.651	498	501	507	rVB2	251	240	0.02%	0.003%
12	2.693	507	514	517	rBV3	578	584	0.05%	0.006%
13	2.767	533	537	538	rVV	258	175	0.01%	0.002%
14	2.802	542	548	553	rVB	364	383	0.03%	0.004%
15	2.918	582	584	588	rBV	221	173	0.01%	0.002%
16	2.969	599	600	603	rBV	270	186	0.02%	0.002%
17	3.021	607	616	619	rVV2	179	252	0.02%	0.003%
18	3.088	633	637	640	rVB2	238	210	0.02%	0.002%
19	3.288	695	699	702	rBV2	157	185	0.02%	0.002%
20	3.420	737	740	744	rVV	295	235	0.02%	0.002%
21	3.455	749	751	755	rVB	307	209	0.02%	0.002%
22	3.487	755	761	765	rBV2	426	455	0.04%	0.005%
23	3.564	781	785	787	rVB2	295	183	0.01%	0.002%
24	3.587	787	792	796	rBV2	197	274	0.02%	0.003%
25	3.783	844	853	892	rBV	71821	207291	16.96%	2.165%
26	4.156	966	969	970	rBV2	338	196	0.02%	0.002%
27	4.243	980	996	1027	rBV	201083	528485	43.25%	5.519%
28	4.590	1101	1104	1106	rBV2	373	184	0.02%	0.002%
29	4.712	1138	1142	1145	rVB2	318	238	0.02%	0.002%
30	4.776	1158	1162	1169	rVB3	257	321	0.03%	0.003%
31	4.821	1173	1176	1183	rBV2	228	215	0.02%	0.002%
32	4.950	1201	1216	1253	rBV2	461952	1221934	100.00%	12.761%
33	5.326	1330	1333	1336	rBV2	405	277	0.02%	0.003%
34	5.365	1341	1345	1348	rVB2	327	231	0.02%	0.002%
35	5.532	1385	1397	1432	rBV	360371	769237	62.95%	8.033%
36	5.821	1476	1487	1516	rBV2	55178	126031	10.31%	1.316%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036678.D
 Acq On : 24 Jul 2024 22:08
 Operator : SY/MD
 Sample : P3335-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

37	5.985	1525	1538	1574	rBV	259196	544463	44.56%	5.686%
38	6.149	1586	1589	1590	rBV3	582	356	0.03%	0.004%
39	6.313	1637	1640	1645	rVB3	355	249	0.02%	0.003%
40	6.333	1645	1646	1653	rVB2	349	327	0.03%	0.003%
41	6.365	1653	1656	1660	rBV	349	279	0.02%	0.003%
42	6.911	1816	1826	1849	rBV	125910	243873	19.96%	2.547%
43	7.239	1916	1928	1969	rBV	543174	980305	80.23%	10.237%
44	7.551	2016	2025	2047	rBV	89648	170248	13.93%	1.778%
45	7.767	2090	2092	2098	rVB3	399	298	0.02%	0.003%
46	7.876	2118	2126	2128	rBV2	1177	1608	0.13%	0.017%
47	7.908	2131	2136	2150	rVB4	3571	6720	0.55%	0.070%
48	8.024	2163	2172	2208	rBV	229159	470767	38.53%	4.916%
49	8.455	2301	2306	2308	rBV3	353	335	0.03%	0.003%
50	8.571	2337	2342	2344	rBV3	416	324	0.03%	0.003%
51	8.596	2347	2350	2353	rVB2	375	190	0.02%	0.002%
52	8.622	2353	2358	2359	rBV	320	285	0.02%	0.003%
53	8.680	2371	2376	2380	rVV3	207	296	0.02%	0.003%
54	8.783	2393	2408	2447	rBV	587630	997877	81.66%	10.421%
55	9.017	2479	2481	2484	rVB	371	169	0.01%	0.002%
56	9.091	2498	2504	2505	rBV2	621	591	0.05%	0.006%
57	9.146	2517	2521	2525	rBV3	361	324	0.03%	0.003%
58	9.262	2555	2557	2561	rVB2	408	233	0.02%	0.002%
59	9.497	2624	2630	2635	rBV4	598	767	0.06%	0.008%
60	9.525	2635	2639	2642	rBV3	330	316	0.03%	0.003%
61	9.577	2651	2655	2660	rVB2	237	169	0.01%	0.002%
62	9.606	2662	2664	2669	rVB2	334	212	0.02%	0.002%
63	9.632	2669	2672	2677	rBV2	236	306	0.03%	0.003%
64	9.860	2740	2743	2744	rBV2	385	207	0.02%	0.002%
65	10.008	2787	2789	2795	rVB	239	203	0.02%	0.002%
66	10.149	2821	2833	2860	rBV	339035	536304	43.89%	5.601%
67	10.320	2879	2886	2892	rBV3	1108	1494	0.12%	0.016%
68	10.358	2894	2898	2906	rVB2	343	527	0.04%	0.006%
69	10.394	2906	2909	2913	rBV2	454	316	0.03%	0.003%
70	10.493	2931	2940	2950	rVB2	733	1217	0.10%	0.013%
71	10.744	3012	3018	3021	rBV	312	364	0.03%	0.004%
72	10.857	3049	3053	3054	rBV2	407	305	0.02%	0.003%
73	11.133	3130	3139	3143	rBV6	1978	2743	0.22%	0.029%
74	11.181	3143	3154	3183	rVV	562963	893182	73.10%	9.327%
75	11.509	3247	3256	3259	rBV5	3050	4527	0.37%	0.047%
76	11.558	3260	3271	3298	rVB	603641	968421	79.25%	10.113%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036678.D
 Acq On : 24 Jul 2024 22:08
 Operator : SY/MD
 Sample : P3335-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

77	11.776	3336	3339	3341	rBV3	304	175	0.01%	0.002%
78	11.805	3346	3348	3351	rVB2	368	216	0.02%	0.002%
79	11.889	3372	3374	3380	rVB3	281	232	0.02%	0.002%
80	12.281	3492	3496	3498	rBV3	234	176	0.01%	0.002%
81	12.429	3538	3542	3546	rBV2	323	277	0.02%	0.003%
82	12.586	3584	3591	3602	rVB3	2356	3548	0.29%	0.037%
83	12.821	3661	3664	3666	rBV2	360	217	0.02%	0.002%
84	12.879	3678	3682	3685	rBV	295	268	0.02%	0.003%
85	13.049	3733	3735	3738	rVV	286	227	0.02%	0.002%
86	13.078	3742	3744	3749	rVB	315	196	0.02%	0.002%
87	13.207	3776	3784	3799	rVB5	2825	4824	0.39%	0.050%
88	13.278	3804	3806	3811	rVB2	263	240	0.02%	0.003%
89	13.310	3813	3816	3819	rBV3	277	204	0.02%	0.002%
90	13.451	3852	3860	3873	rBV2	3480	6285	0.51%	0.066%
91	13.570	3894	3897	3901	rVB2	456	279	0.02%	0.003%
92	13.686	3925	3933	3946	rVB4	2897	4862	0.40%	0.051%
93	13.792	3964	3966	3971	rBV2	316	258	0.02%	0.003%
94	13.876	3987	3992	3998	rBV3	375	495	0.04%	0.005%
95	13.905	3998	4001	4005	rBV3	191	204	0.02%	0.002%
96	14.027	4037	4039	4044	rVB2	295	201	0.02%	0.002%
97	14.397	4148	4154	4159	rBV3	460	546	0.04%	0.006%
98	14.519	4190	4192	4195	rBV2	376	230	0.02%	0.002%
99	14.824	4282	4287	4290	rBV4	419	415	0.03%	0.004%
100	15.165	4390	4393	4394	rBV3	546	301	0.02%	0.003%




Sum of corrected areas: 9575859

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036678.D
Acq On : 24 Jul 2024 22:08
Operator : SY/MD
Sample : P3335-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

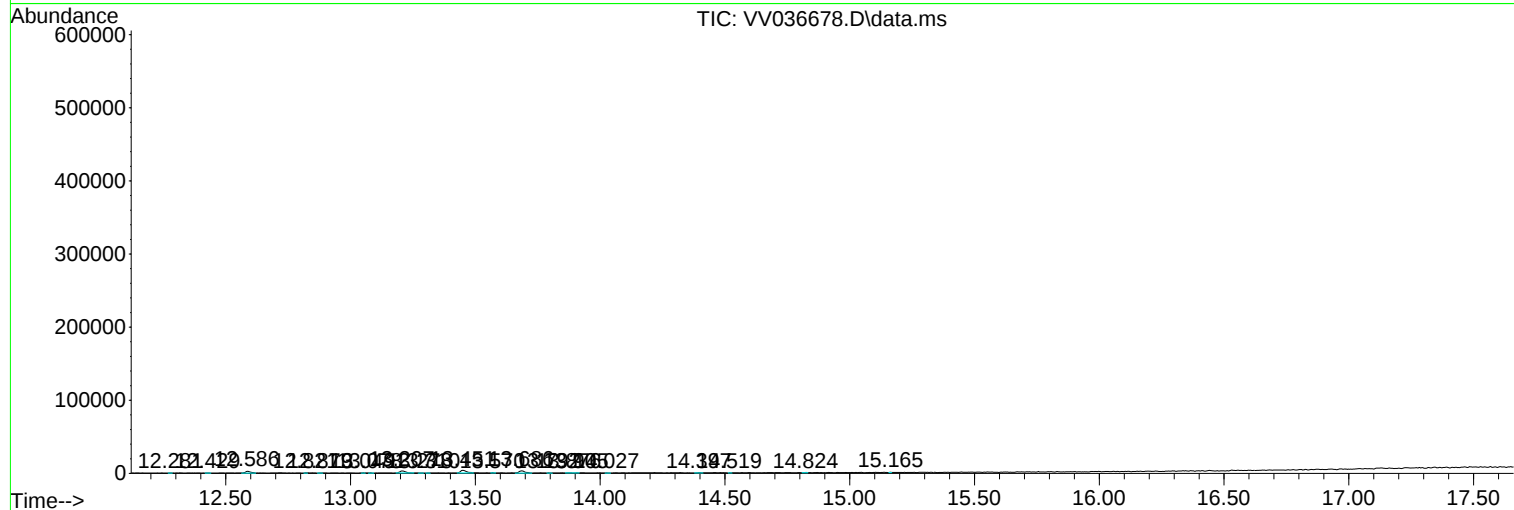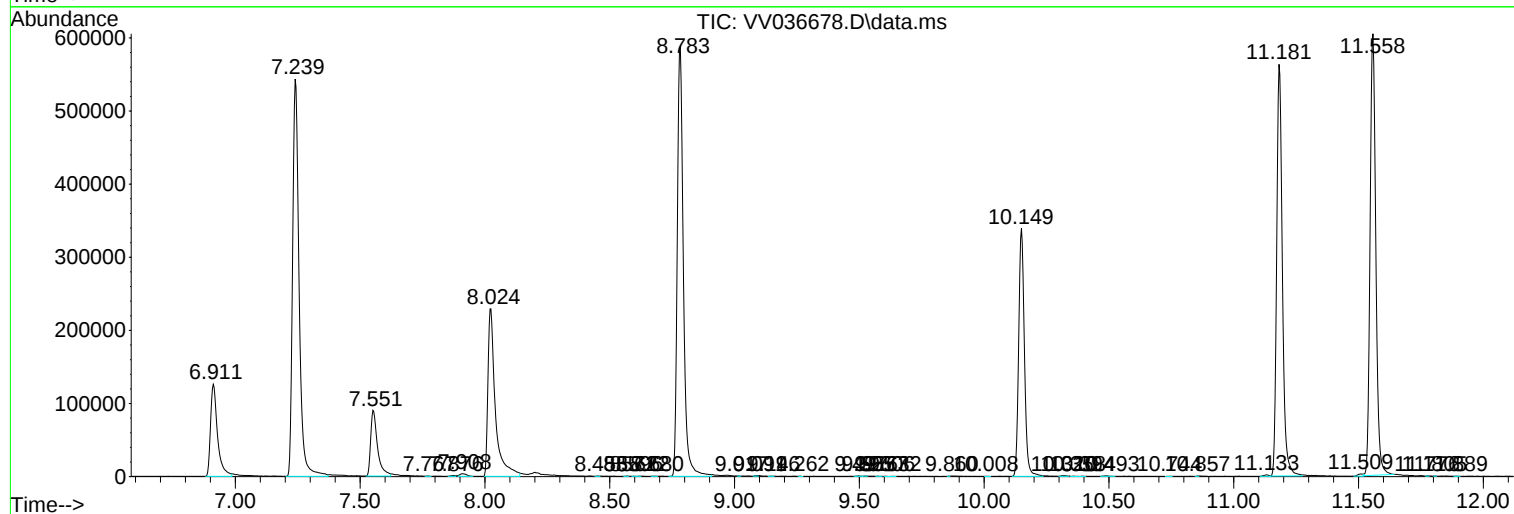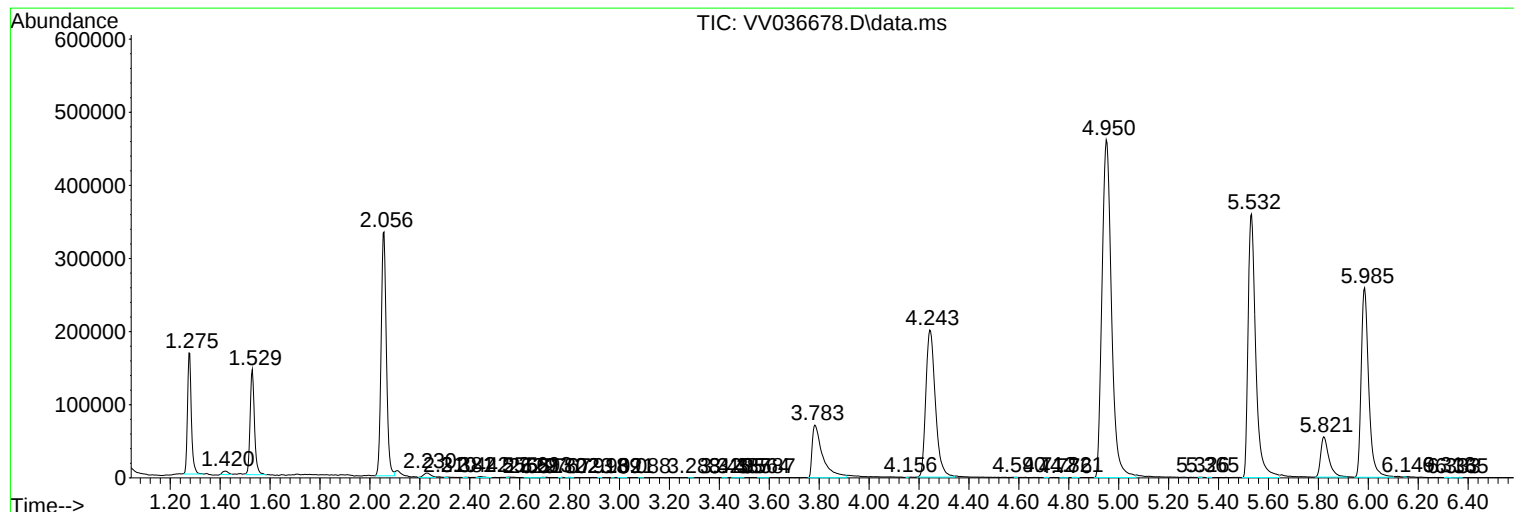

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036678.D
Acq On : 24 Jul 2024 22:08
Operator : SY/MD
Sample : P3335-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036678.D
Acq On : 24 Jul 2024 22:08
Operator : SY/MD
Sample : P3335-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------