

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036679.D
 Acq On : 24 Jul 2024 22:32
 Operator : SY/MD
 Sample : P3335-04 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M

Title : VOC Analysis

Signal : TIC: VV036679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	91	rVB	168094	180621	4.87%	1.347%
2	1.526	144	151	170	rVB	146990	180559	4.87%	1.346%
3	2.053	306	315	330	rBV	327700	476462	12.85%	3.553%
4	2.445	429	437	449	rVB3	4227	7149	0.19%	0.053%
5	2.558	460	472	483	rBV2	2667	5668	0.15%	0.042%
6	2.764	534	536	538	rBV	137	84	0.00%	0.001%
7	2.812	548	551	553	rBV2	205	163	0.00%	0.001%
8	2.928	584	587	590	rBV2	255	232	0.01%	0.002%
9	2.989	604	606	607	rBV	245	101	0.00%	0.001%
10	3.034	616	620	621	rBV2	201	154	0.00%	0.001%
11	3.076	631	633	636	rVB2	156	87	0.00%	0.001%
12	3.095	636	639	641	rBV2	232	169	0.00%	0.001%
13	3.175	662	664	665	rBV	124	65	0.00%	0.000%
14	3.252	684	688	691	rBV	199	153	0.00%	0.001%
15	3.314	702	707	709	rBV2	221	222	0.01%	0.002%
16	3.394	730	732	737	rBV2	116	84	0.00%	0.001%
17	3.445	746	748	750	rBV	45	22	0.00%	0.000%
18	3.478	753	758	764	rVB2	247	355	0.01%	0.003%
19	3.506	764	767	769	rBV2	195	153	0.00%	0.001%
20	3.558	779	783	788	rVB2	208	164	0.00%	0.001%
21	3.590	788	793	797	rBV	300	334	0.01%	0.002%
22	3.783	840	853	902	rBV2	82233	266548	7.19%	1.988%
23	4.243	980	996	1029	rBV	208201	545515	14.72%	4.068%
24	4.748	1151	1153	1155	rBV	228	125	0.00%	0.001%
25	4.854	1184	1186	1189	rVB	251	155	0.00%	0.001%
26	4.873	1189	1192	1195	rBV2	235	150	0.00%	0.001%
27	4.899	1195	1200	1201	rBV	214	182	0.00%	0.001%
28	4.950	1201	1216	1248	rBV3	471177	1243205	33.54%	9.271%
29	5.529	1386	1396	1431	rBV	371146	789958	21.31%	5.891%
30	5.825	1475	1488	1525	rBV	1872155	3706663	100.00%	27.642%
31	5.985	1528	1538	1565	rVB	269676	557247	15.03%	4.156%
32	6.291	1631	1633	1635	rVB2	461	122	0.00%	0.001%
33	6.375	1656	1659	1661	rBV	275	153	0.00%	0.001%
34	6.429	1675	1676	1677	rBV	131	45	0.00%	0.000%
35	6.519	1700	1704	1707	rBV	229	171	0.00%	0.001%
36	6.580	1720	1723	1726	rBV2	288	255	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036679.D
 Acq On : 24 Jul 2024 22:32
 Operator : SY/MD
 Sample : P3335-04 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

37	6.596	1726	1728	1729	rVV2	138	42	0.00%	0.000%
38	6.670	1746	1751	1752	rBV2	287	225	0.01%	0.002%
39	6.699	1756	1760	1763	rVV2	184	146	0.00%	0.001%
40	6.744	1772	1774	1782	rVB2	403	378	0.01%	0.003%
41	6.786	1782	1787	1791	rBV2	356	340	0.01%	0.003%
42	6.812	1791	1795	1796	rVV2	316	206	0.01%	0.002%
43	6.834	1799	1802	1804	rVB2	176	84	0.00%	0.001%
44	6.870	1811	1813	1816	rBV2	172	95	0.00%	0.001%
45	6.911	1816	1826	1858	rBV2	130292	259056	6.99%	1.932%
46	7.239	1917	1928	1961	rBV	552981	980416	26.45%	7.311%
47	7.551	2016	2025	2051	rBV	95003	178196	4.81%	1.329%
48	7.764	2089	2091	2096	rVB2	604	313	0.01%	0.002%
49	7.854	2117	2119	2120	rBV	399	171	0.00%	0.001%
50	7.908	2128	2136	2150	rVB4	9902	17777	0.48%	0.133%
51	8.021	2162	2171	2217	rBV	245025	493091	13.30%	3.677%
52	8.439	2298	2301	2303	rBV2	363	180	0.00%	0.001%
53	8.558	2334	2338	2342	rBV2	496	465	0.01%	0.003%
54	8.741	2394	2395	2397	rBV	285	118	0.00%	0.001%
55	8.780	2397	2407	2431	rBV	597066	1000846	27.00%	7.464%
56	9.490	2626	2628	2634	rVB2	400	390	0.01%	0.003%
57	9.519	2634	2637	2644	rBV2	497	549	0.01%	0.004%
58	9.606	2661	2664	2669	rBV2	427	454	0.01%	0.003%
59	9.931	2762	2765	2766	rBV2	309	157	0.00%	0.001%
60	10.095	2814	2816	2820	rVB2	230	164	0.00%	0.001%
61	10.149	2820	2833	2861	rBV	399188	636020	17.16%	4.743%
62	10.317	2882	2885	2888	rBV2	462	374	0.01%	0.003%
63	10.365	2898	2900	2901	rBV	319	119	0.00%	0.001%
64	10.432	2920	2921	2923	rVB	232	67	0.00%	0.000%
65	10.464	2928	2931	2932	rBV	153	85	0.00%	0.001%
66	10.474	2932	2934	2935	rVB	188	48	0.00%	0.000%
67	10.542	2953	2955	2960	rVB2	236	134	0.00%	0.001%
68	10.619	2971	2979	2983	rBV3	402	513	0.01%	0.004%
69	10.654	2987	2990	2995	rVV2	256	203	0.01%	0.002%
70	10.863	3052	3055	3060	rBV4	499	549	0.01%	0.004%
71	11.133	3132	3139	3143	rBV3	1593	1982	0.05%	0.015%
72	11.181	3144	3154	3187	rVV	563472	893491	24.10%	6.663%
73	11.455	3236	3239	3241	rBV2	476	296	0.01%	0.002%
74	11.558	3259	3271	3296	rBV	602775	967890	26.11%	7.218%
75	11.869	3362	3368	3371	rBV3	443	503	0.01%	0.004%
76	12.037	3414	3420	3423	rBV2	546	523	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036679.D
 Acq On : 24 Jul 2024 22:32
 Operator : SY/MD
 Sample : P3335-04 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M

Title : VOC Analysis

77	12.239	3480	3483	3484	rBV	352	222	0.01%	0.002%
78	12.316	3505	3507	3509	rBV	230	87	0.00%	0.001%
79	12.471	3549	3555	3557	rBV	457	327	0.01%	0.002%
80	12.593	3587	3593	3598	rBV3	1388	1820	0.05%	0.014%
81	12.677	3618	3619	3624	rVB2	361	193	0.01%	0.001%
82	12.734	3634	3637	3640	rBV	310	202	0.01%	0.002%
83	12.828	3664	3666	3668	rBV	232	113	0.00%	0.001%
84	12.882	3680	3683	3684	rBV	279	149	0.00%	0.001%
85	13.120	3755	3757	3759	rBV2	275	135	0.00%	0.001%
86	13.210	3777	3785	3794	rBV4	2179	3470	0.09%	0.026%
87	13.291	3807	3810	3814	rBV3	305	212	0.01%	0.002%
88	13.448	3857	3859	3870	rVB2	2055	2683	0.07%	0.020%




Sum of corrected areas: 13409764

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036679.D
Acq On : 24 Jul 2024 22:32
Operator : SY/MD
Sample : P3335-04 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

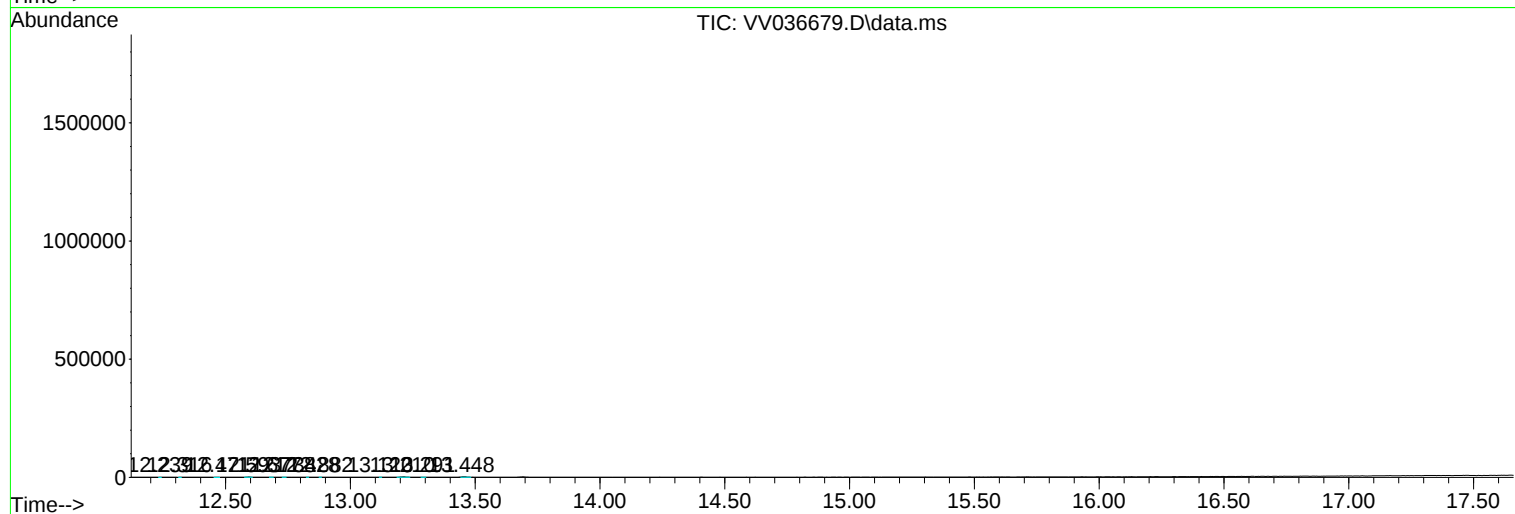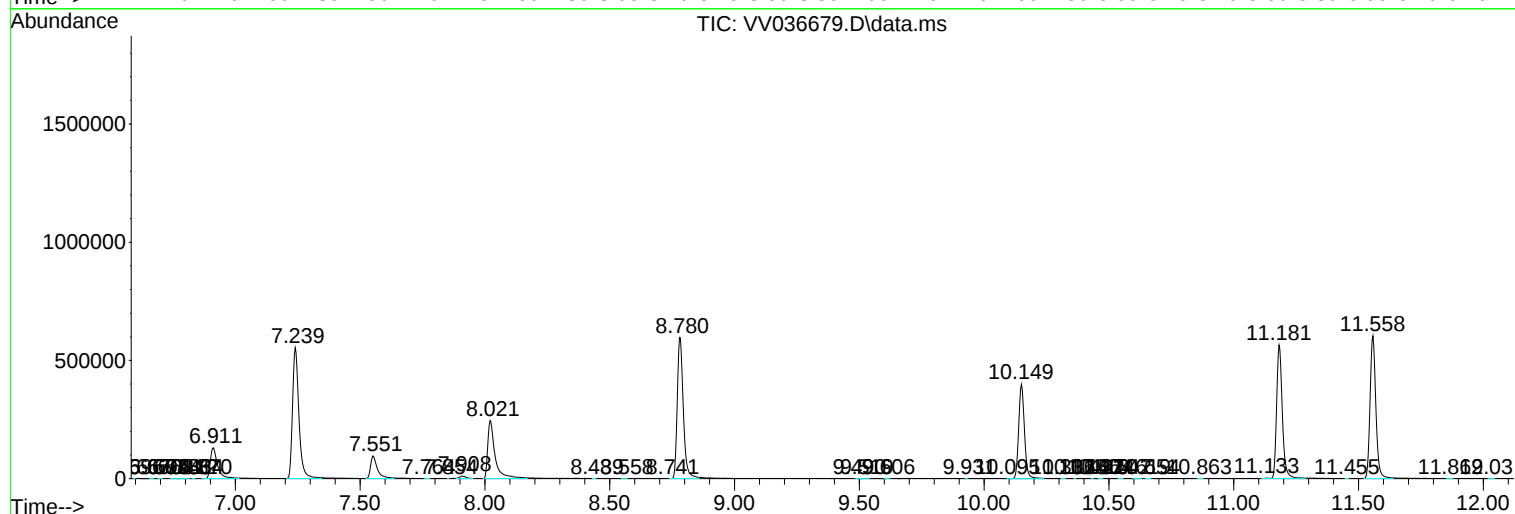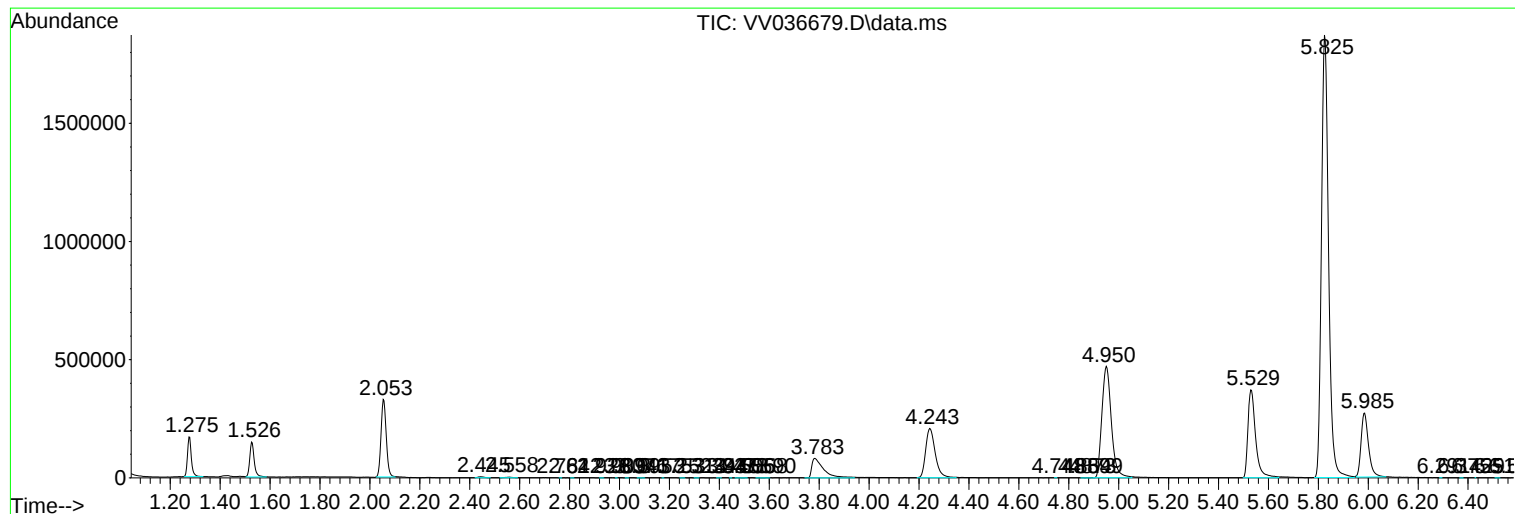

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036679.D
Acq On : 24 Jul 2024 22:32
Operator : SY/MD
Sample : P3335-04 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036679.D
Acq On : 24 Jul 2024 22:32
Operator : SY/MD
Sample : P3335-04 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------