

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036681.D
 Acq On : 24 Jul 2024 23:21
 Operator : SY/MD
 Sample : P3335-06 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M

Title : VOC Analysis

Signal : TIC: VV036681.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	89	rVB	164653	178824	12.21%	1.586%
2	1.413	110	116	118	rBV4	4730	5033	0.34%	0.045%
3	1.526	144	151	169	rVB	140774	173952	11.88%	1.543%
4	2.053	304	315	331	rBV	329290	484026	33.05%	4.293%
5	2.223	364	368	369	rBV	746	451	0.03%	0.004%
6	2.310	391	395	399	rBV3	327	317	0.02%	0.003%
7	2.359	404	410	412	rBV2	219	198	0.01%	0.002%
8	2.445	425	437	447	rVB4	4202	7438	0.51%	0.066%
9	2.500	451	454	459	rBV2	213	203	0.01%	0.002%
10	2.555	463	471	472	rBV2	1729	2104	0.14%	0.019%
11	2.641	495	498	506	rVB3	265	300	0.02%	0.003%
12	2.696	506	515	517	rBV4	872	890	0.06%	0.008%
13	2.992	604	607	613	rVB2	336	344	0.02%	0.003%
14	3.018	613	615	618	rBV2	299	208	0.01%	0.002%
15	3.056	625	627	634	rVB2	350	315	0.02%	0.003%
16	3.085	634	636	639	rBV2	368	256	0.02%	0.002%
17	3.101	639	641	645	rVV2	256	204	0.01%	0.002%
18	3.137	645	652	657	rVV2	326	363	0.02%	0.003%
19	3.188	665	668	671	rBV2	231	202	0.01%	0.002%
20	3.252	682	688	691	rBV2	224	255	0.02%	0.002%
21	3.294	697	701	704	rBV2	192	200	0.01%	0.002%
22	3.407	730	736	738	rBV2	258	280	0.02%	0.002%
23	3.484	751	760	763	rBV2	242	358	0.02%	0.003%
24	3.625	800	804	808	rVB2	279	290	0.02%	0.003%
25	3.786	844	854	891	rBV2	82322	303996	20.76%	2.696%
26	4.108	951	954	962	rBV4	361	482	0.03%	0.004%
27	4.243	980	996	1038	rBV	207507	541076	36.95%	4.799%
28	4.670	1125	1129	1131	rBV2	383	226	0.02%	0.002%
29	4.686	1131	1134	1136	rBV3	317	197	0.01%	0.002%
30	4.793	1163	1167	1169	rBV2	237	214	0.01%	0.002%
31	4.825	1174	1177	1183	rVB3	218	284	0.02%	0.003%
32	4.950	1201	1216	1252	rBV2	464719	1235633	84.38%	10.959%
33	5.297	1323	1324	1332	rVB3	813	684	0.05%	0.006%
34	5.333	1332	1335	1337	rBV	250	197	0.01%	0.002%
35	5.532	1386	1397	1437	rBV	365978	785553	53.64%	6.967%
36	5.757	1464	1467	1472	rBV3	401	357	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036681.D
 Acq On : 24 Jul 2024 23:21
 Operator : SY/MD
 Sample : P3335-06 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

37	5.828	1472	1489	1522	rBV	706337	1464410	100.00%	12.988%
38	5.985	1526	1538	1568	rVB	259788	548236	37.44%	4.863%
39	6.284	1629	1631	1636	rVB2	505	294	0.02%	0.003%
40	6.320	1638	1642	1646	rBV3	365	317	0.02%	0.003%
41	6.362	1651	1655	1659	rBV3	251	217	0.01%	0.002%
42	6.403	1662	1668	1669	rBV3	331	298	0.02%	0.003%
43	6.455	1681	1684	1687	rVB	282	193	0.01%	0.002%
44	6.773	1778	1783	1786	rBV	253	207	0.01%	0.002%
45	6.911	1816	1826	1856	rBV	127761	251200	17.15%	2.228%
46	7.120	1889	1891	1896	rVB	440	291	0.02%	0.003%
47	7.146	1896	1899	1905	rBV4	321	285	0.02%	0.003%
48	7.239	1917	1928	1970	rBV	549413	986316	67.35%	8.748%
49	7.551	2016	2025	2054	rBV	89731	175095	11.96%	1.553%
50	7.799	2100	2102	2104	rVB3	481	220	0.02%	0.002%
51	7.860	2117	2121	2123	rVV2	428	363	0.02%	0.003%
52	7.905	2123	2135	2163	rVB3	64830	117254	8.01%	1.040%
53	8.021	2163	2171	2216	rBV	234729	474520	32.40%	4.209%
54	8.333	2266	2268	2271	rBV3	375	219	0.01%	0.002%
55	8.429	2296	2298	2304	rVB2	639	478	0.03%	0.004%
56	8.458	2304	2307	2311	rBV3	298	267	0.02%	0.002%
57	8.564	2336	2340	2345	rVB4	393	280	0.02%	0.002%
58	8.641	2361	2364	2372	rVB	310	259	0.02%	0.002%
59	8.783	2396	2408	2434	rBV	600349	1005395	68.66%	8.917%
60	9.101	2499	2507	2508	rBV2	355	411	0.03%	0.004%
61	9.172	2526	2529	2532	rBV2	272	196	0.01%	0.002%
62	9.236	2544	2549	2555	rBV3	300	462	0.03%	0.004%
63	9.294	2561	2567	2570	rBV2	250	280	0.02%	0.002%
64	9.374	2588	2592	2597	rBV	305	349	0.02%	0.003%
65	9.503	2627	2632	2636	rVV3	239	259	0.02%	0.002%
66	9.599	2656	2662	2665	rVV3	313	308	0.02%	0.003%
67	9.622	2665	2669	2674	rVV2	300	217	0.01%	0.002%
68	10.066	2803	2807	2812	rBV2	234	286	0.02%	0.003%
69	10.149	2821	2833	2855	rBV	389255	622979	42.54%	5.525%
70	10.455	2923	2928	2929	rBV	223	194	0.01%	0.002%
71	10.487	2934	2938	2941	rBV2	364	262	0.02%	0.002%
72	10.750	3015	3020	3024	rBV2	330	357	0.02%	0.003%
73	10.770	3024	3026	3033	rVV2	288	227	0.02%	0.002%
74	10.857	3047	3053	3055	rBV2	277	248	0.02%	0.002%
75	10.934	3072	3077	3085	rBV2	188	362	0.02%	0.003%
76	11.024	3099	3105	3106	rBV2	188	206	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036681.D
 Acq On : 24 Jul 2024 23:21
 Operator : SY/MD
 Sample : P3335-06 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

77	11.133	3134	3139	3144	rBV3	929	1136	0.08%	0.010%
78	11.181	3144	3154	3180	rBV	570891	902715	61.64%	8.007%
79	11.490	3249	3250	3254	rVB2	475	222	0.02%	0.002%
80	11.558	3258	3271	3296	rBV	612093	980975	66.99%	8.701%
81	11.705	3315	3317	3321	rBV2	494	296	0.02%	0.003%
82	11.757	3330	3333	3336	rBV2	398	312	0.02%	0.003%
83	11.815	3349	3351	3358	rVB3	358	279	0.02%	0.002%
84	12.249	3482	3486	3489	rBV2	265	206	0.01%	0.002%
85	12.368	3521	3523	3529	rVB2	389	209	0.01%	0.002%
86	12.593	3587	3593	3597	rBV3	955	1173	0.08%	0.010%
87	12.857	3673	3675	3682	rVB3	503	423	0.03%	0.004%
88	12.889	3682	3685	3686	rBV2	308	196	0.01%	0.002%
89	13.107	3750	3753	3756	rBV2	269	195	0.01%	0.002%
90	13.217	3780	3787	3788	rBV4	1181	1146	0.08%	0.010%
91	13.410	3842	3847	3850	rVB3	325	258	0.02%	0.002%
92	13.458	3855	3862	3863	rBV3	1267	1164	0.08%	0.010%
93	13.512	3877	3879	3885	rVB4	513	408	0.03%	0.004%
94	13.696	3927	3936	3939	rBV3	1054	1559	0.11%	0.014%
95	13.750	3947	3953	3958	rBV2	426	484	0.03%	0.004%
96	13.998	4026	4030	4031	rBV2	322	227	0.02%	0.002%
97	14.242	4103	4106	4110	rBV2	259	244	0.02%	0.002%
98	14.670	4237	4239	4242	rBV2	392	194	0.01%	0.002%
99	14.995	4338	4340	4343	rBV3	373	259	0.02%	0.002%
100	15.258	4418	4422	4423	rBV2	470	341	0.02%	0.003%




Sum of corrected areas: 11274748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036681.D
Acq On : 24 Jul 2024 23:21
Operator : SY/MD
Sample : P3335-06 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

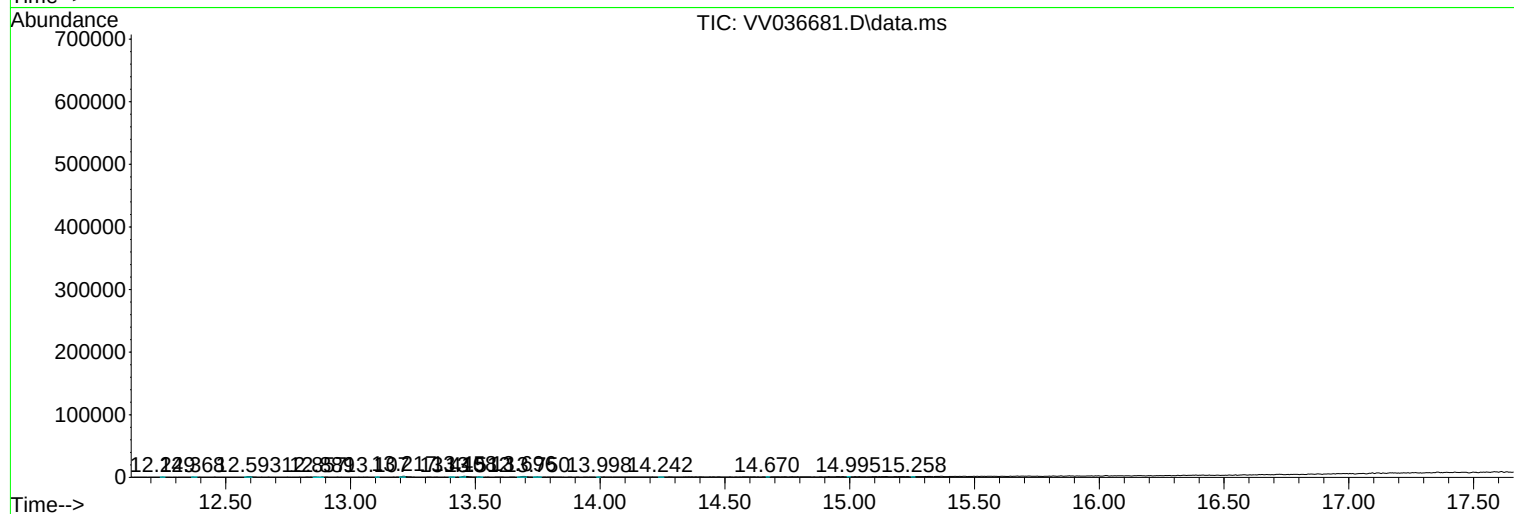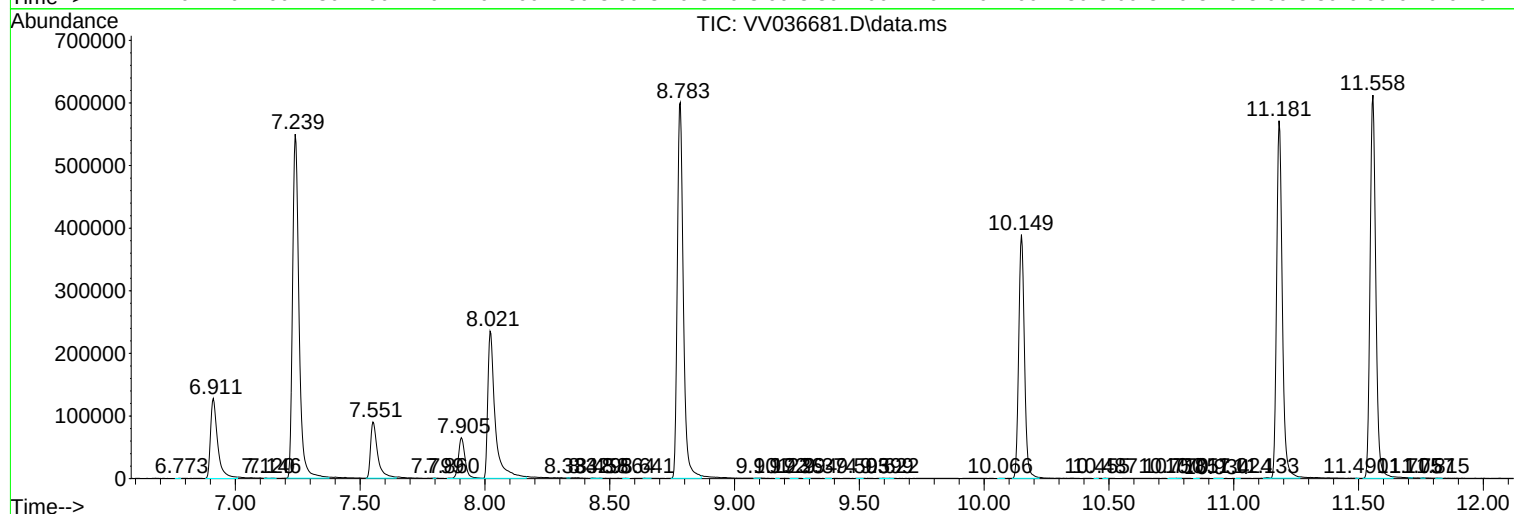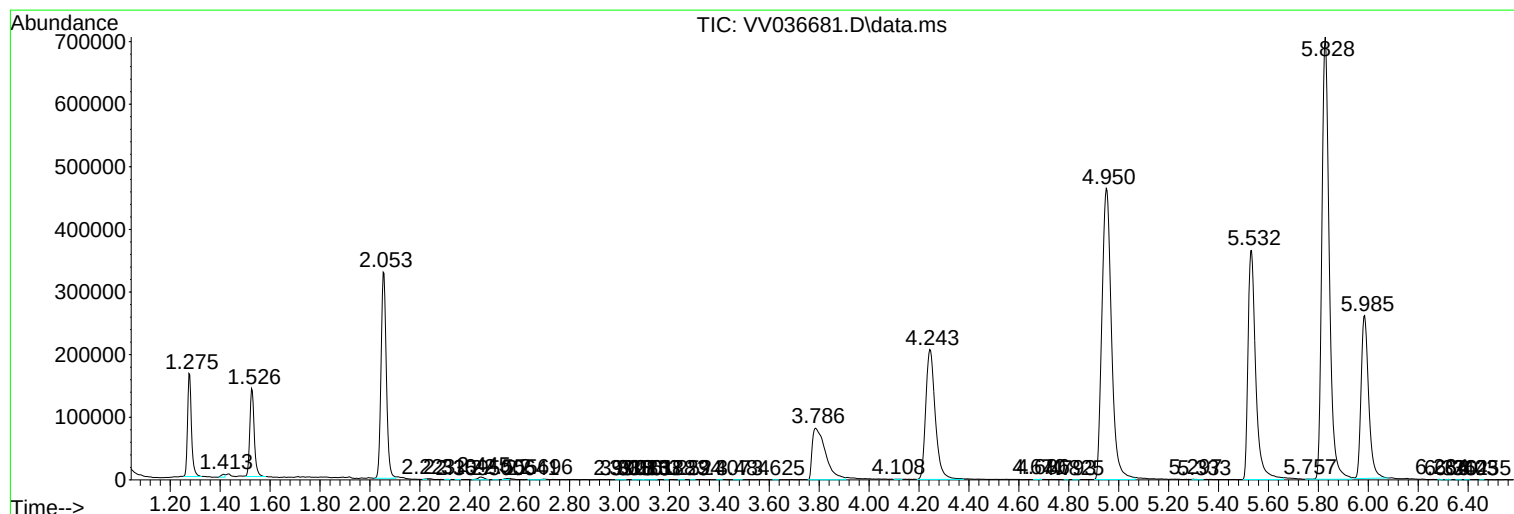

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036681.D
Acq On : 24 Jul 2024 23:21
Operator : SY/MD
Sample : P3335-06 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036681.D
Acq On : 24 Jul 2024 23:21
Operator : SY/MD
Sample : P3335-06 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc