

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036684.D
 Acq On : 25 Jul 2024 00:33
 Operator : SY/MD
 Sample : P3335-10 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M

Title : VOC Analysis

Signal : TIC: VV036684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	153968	170027	14.57%	1.877%
2	1.529	144	152	173	rVB	139127	172039	14.74%	1.900%
3	2.056	305	316	332	rBV	297150	438288	37.56%	4.840%
4	2.207	361	363	366	rVB	392	172	0.01%	0.002%
5	2.240	366	373	381	rBV2	852	1384	0.12%	0.015%
6	2.449	428	438	450	rVB2	3930	6232	0.53%	0.069%
7	2.558	459	472	488	rVB4	2963	6448	0.55%	0.071%
8	2.629	490	494	497	rBV2	211	170	0.01%	0.002%
9	2.719	518	522	526	rVB	290	289	0.02%	0.003%
10	2.744	526	530	534	rBV2	286	287	0.02%	0.003%
11	2.828	549	556	558	rBV2	268	196	0.02%	0.002%
12	2.899	576	578	581	rBV2	278	187	0.02%	0.002%
13	3.008	609	612	615	rBV2	234	210	0.02%	0.002%
14	3.069	627	631	635	rVB2	251	201	0.02%	0.002%
15	3.108	637	643	646	rBV2	369	348	0.03%	0.004%
16	3.220	674	678	684	rBV	212	221	0.02%	0.002%
17	3.352	711	719	724	rBV2	293	436	0.04%	0.005%
18	3.471	753	756	760	rVV	251	195	0.02%	0.002%
19	3.516	768	770	774	rVB2	200	163	0.01%	0.002%
20	3.703	823	828	830	rBV	215	213	0.02%	0.002%
21	3.725	833	835	842	rVB2	298	311	0.03%	0.003%
22	3.783	842	853	886	rBV2	78420	233453	20.01%	2.578%
23	4.159	967	970	974	rBV3	396	322	0.03%	0.004%
24	4.243	981	996	1029	rBV	198628	519890	44.55%	5.741%
25	4.551	1088	1092	1093	rBV3	264	213	0.02%	0.002%
26	4.661	1123	1126	1129	rVV3	267	218	0.02%	0.002%
27	4.677	1129	1131	1135	rVB2	310	212	0.02%	0.002%
28	4.780	1158	1163	1168	rVB3	263	271	0.02%	0.003%
29	4.815	1168	1174	1176	rBV3	282	248	0.02%	0.003%
30	4.950	1200	1216	1244	rBV2	435841	1166858	100.00%	12.885%
31	5.172	1283	1285	1288	rVB3	625	261	0.02%	0.003%
32	5.301	1323	1325	1327	rBV2	420	215	0.02%	0.002%
33	5.391	1350	1353	1359	rVV3	156	166	0.01%	0.002%
34	5.532	1386	1397	1436	rBV	343532	740086	63.43%	8.172%
35	5.783	1473	1475	1478	rVB2	339	181	0.02%	0.002%
36	5.825	1478	1488	1512	rBV2	31591	72353	6.20%	0.799%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072524\
 Data File : VW036684.D
 Acq On : 25 Jul 2024 00:33
 Operator : SY/MD
 Sample : P3335-10 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

37	5.944	1521	1525	1526	rBV	530	358	0.03%	0.004%
38	5.985	1526	1538	1576	rVV	250662	531387	45.54%	5.868%
39	6.198	1602	1604	1607	rBV3	638	327	0.03%	0.004%
40	6.304	1635	1637	1643	rBV3	297	306	0.03%	0.003%
41	6.384	1659	1662	1666	rVV	224	186	0.02%	0.002%
42	6.503	1694	1699	1703	rVB2	273	283	0.02%	0.003%
43	6.571	1717	1720	1725	rVB2	222	185	0.02%	0.002%
44	6.674	1747	1752	1754	rBV	315	205	0.02%	0.002%
45	6.799	1788	1791	1796	rBV2	179	171	0.01%	0.002%
46	6.873	1809	1814	1816	rBV2	177	171	0.01%	0.002%
47	6.911	1816	1826	1859	rBV	117991	232369	19.91%	2.566%
48	7.165	1902	1905	1909	rVB2	243	208	0.02%	0.002%
49	7.239	1916	1928	1967	rBV	479962	870309	74.59%	9.610%
50	7.551	2016	2025	2055	rBV2	84537	166298	14.25%	1.836%
51	7.722	2076	2078	2082	rVB2	611	427	0.04%	0.005%
52	7.776	2091	2095	2097	rBV2	407	356	0.03%	0.004%
53	7.792	2097	2100	2104	rVB3	465	310	0.03%	0.003%
54	7.876	2120	2126	2129	rBV2	548	566	0.05%	0.006%
55	7.911	2130	2137	2146	rVB5	2385	3464	0.30%	0.038%
56	8.021	2163	2171	2211	rBV	235554	475776	40.77%	5.254%
57	8.484	2313	2315	2319	rVB	411	205	0.02%	0.002%
58	8.509	2321	2323	2327	rVB2	314	162	0.01%	0.002%
59	8.712	2383	2386	2389	rBV2	358	271	0.02%	0.003%
60	8.783	2395	2408	2447	rBV	559609	941718	80.71%	10.399%
61	9.069	2495	2497	2498	rBV	364	197	0.02%	0.002%
62	9.243	2544	2551	2554	rBV4	225	270	0.02%	0.003%
63	9.316	2570	2574	2576	rBV	384	186	0.02%	0.002%
64	9.500	2629	2631	2633	rBV	334	241	0.02%	0.003%
65	9.661	2678	2681	2685	rVB	225	203	0.02%	0.002%
66	10.149	2822	2833	2869	rBV	381051	611162	52.38%	6.749%
67	10.429	2917	2920	2926	rBV	238	223	0.02%	0.002%
68	10.622	2976	2980	2983	rBV	309	246	0.02%	0.003%
69	10.754	3017	3021	3026	rBV	206	272	0.02%	0.003%
70	10.988	3089	3094	3098	rBV2	224	223	0.02%	0.002%
71	11.011	3098	3101	3104	rVV	263	169	0.01%	0.002%
72	11.033	3106	3108	3112	rVV2	275	187	0.02%	0.002%
73	11.133	3135	3139	3140	rBV2	763	621	0.05%	0.007%
74	11.181	3144	3154	3189	rBV	495111	799774	68.54%	8.831%
75	11.558	3259	3271	3308	rBV	543890	874941	74.98%	9.661%
76	11.731	3322	3325	3330	rBV4	592	588	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036684.D
 Acq On : 25 Jul 2024 00:33
 Operator : SY/MD
 Sample : P3335-10 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

77	11.927	3383	3386	3391	rBV3	246	240	0.02%	0.003%
78	12.098	3433	3439	3445	rBV	350	525	0.04%	0.006%
79	12.522	3569	3571	3578	rVB2	284	243	0.02%	0.003%
80	12.837	3664	3669	3672	rBV2	264	240	0.02%	0.003%
81	13.210	3781	3785	3787	rBV2	578	457	0.04%	0.005%
82	13.262	3798	3801	3803	rBV2	302	202	0.02%	0.002%
83	13.294	3808	3811	3815	rBV2	344	285	0.02%	0.003%
84	13.458	3857	3862	3863	rBV	476	429	0.04%	0.005%
85	13.535	3883	3886	3890	rVB3	439	352	0.03%	0.004%
86	13.557	3890	3893	3895	rBV	221	168	0.01%	0.002%
87	13.651	3919	3922	3926	rVB2	295	262	0.02%	0.003%
88	13.689	3926	3934	3942	rBV4	943	1560	0.13%	0.017%
89	13.808	3968	3971	3975	rVB2	314	203	0.02%	0.002%
90	13.828	3975	3977	3980	rVB2	313	209	0.02%	0.002%
91	13.985	4023	4026	4029	rBV3	249	186	0.02%	0.002%
92	14.291	4119	4121	4126	rVB2	343	162	0.01%	0.002%
93	14.313	4126	4128	4134	rVB4	512	422	0.04%	0.005%
94	14.342	4134	4137	4139	rBV	321	207	0.02%	0.002%
95	14.490	4180	4183	4185	rVV2	254	169	0.01%	0.002%
96	14.712	4249	4252	4254	rBV	319	185	0.02%	0.002%
97	14.799	4277	4279	4281	rBV	288	162	0.01%	0.002%
98	14.963	4328	4330	4332	rBV2	301	181	0.02%	0.002%
99	15.065	4359	4362	4365	rVB3	635	433	0.04%	0.005%
100	15.204	4403	4405	4407	rVB2	485	177	0.02%	0.002%




Sum of corrected areas: 9056144

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036684.D
Acq On : 25 Jul 2024 00:33
Operator : SY/MD
Sample : P3335-10 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

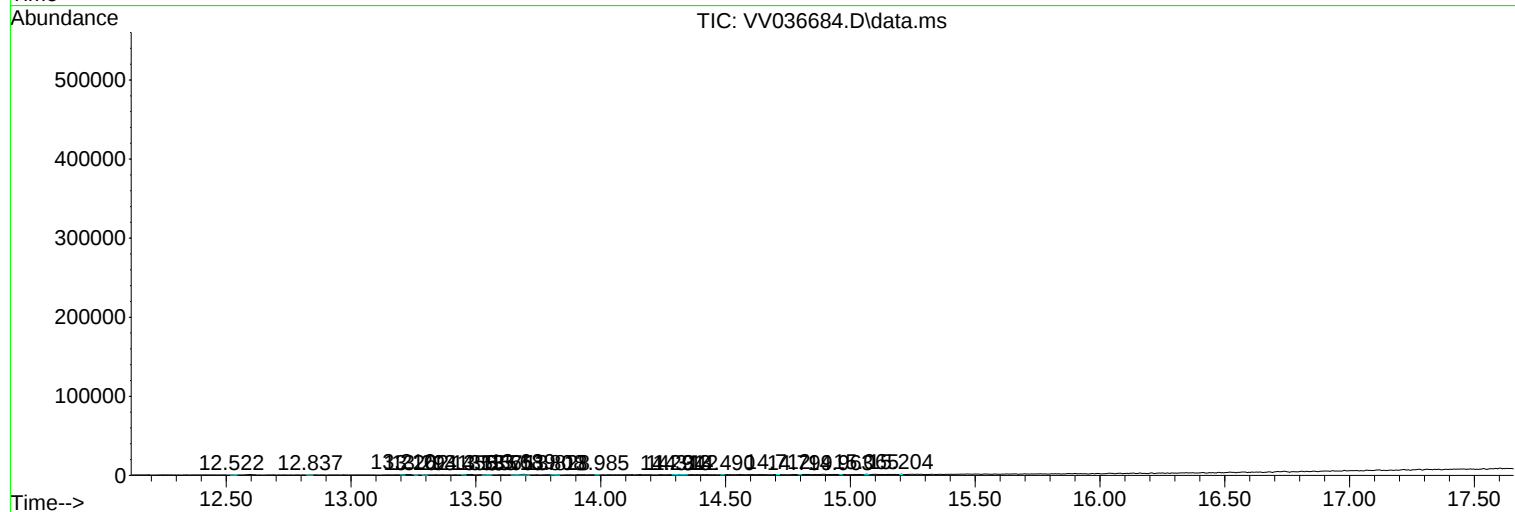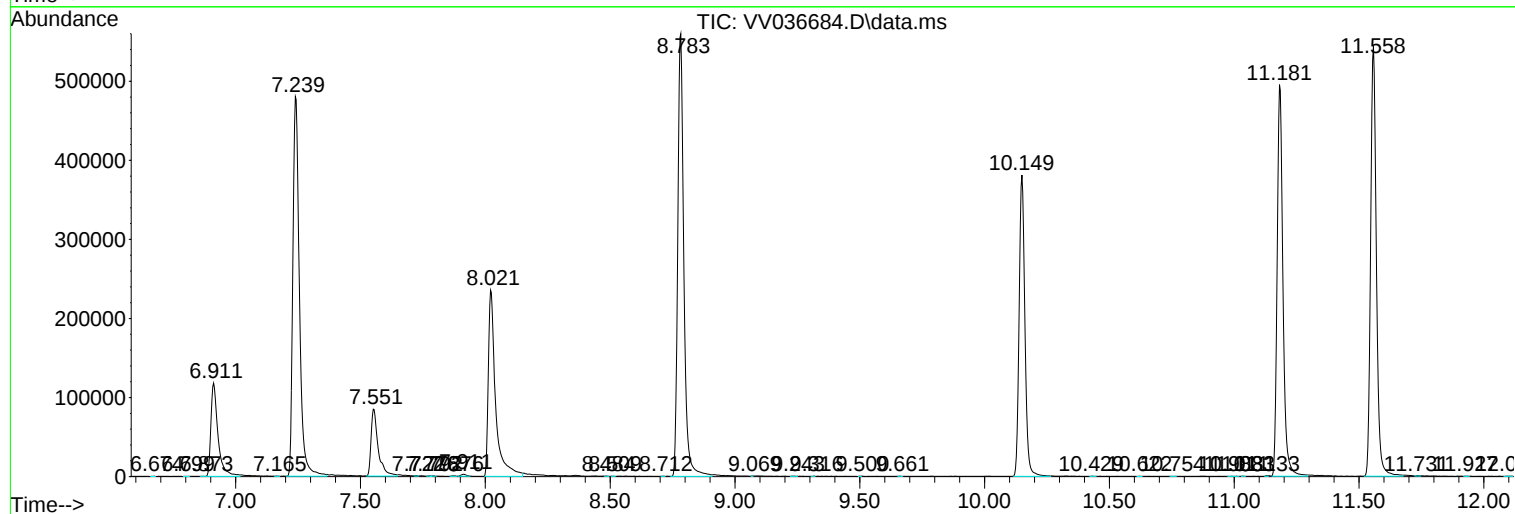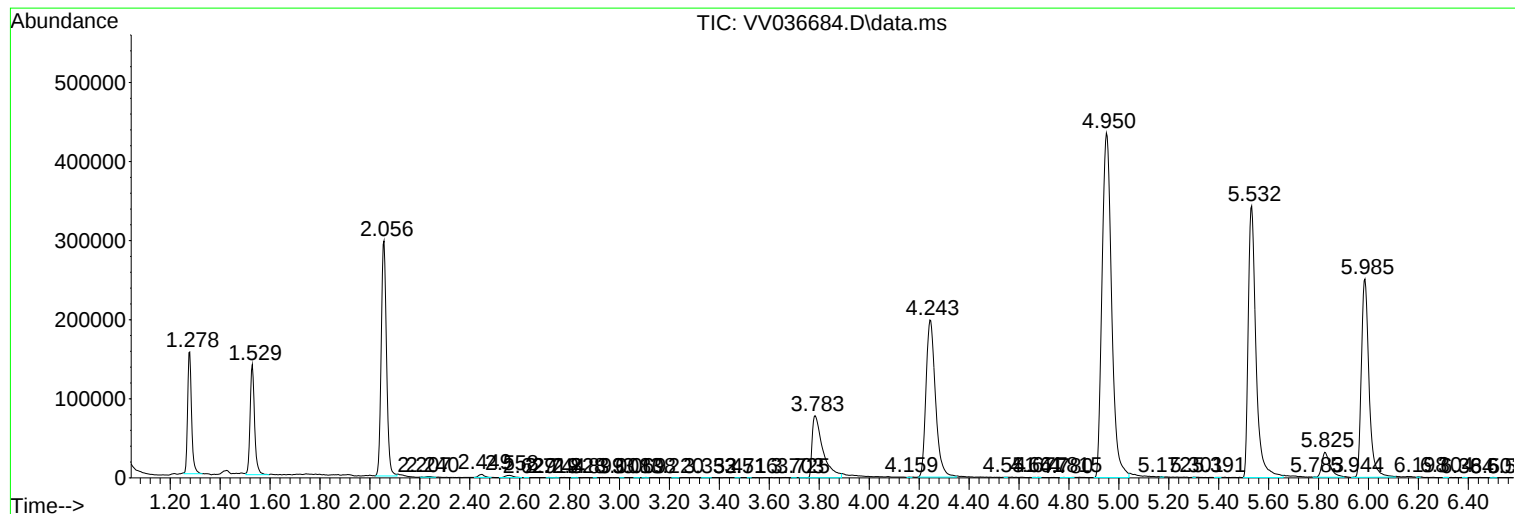

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036684.D
Acq On : 25 Jul 2024 00:33
Operator : SY/MD
Sample : P3335-10 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036684.D
Acq On : 25 Jul 2024 00:33
Operator : SY/MD
Sample : P3335-10 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc