

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036685.D
 Acq On : 25 Jul 2024 00:58
 Operator : SY/MD
 Sample : P3335-12 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M

Title : VOC Analysis

Signal : TIC: VV036685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	94	rVB	154204	165143	14.34%	1.860%
2	1.526	144	151	166	rVB	133985	160774	13.96%	1.811%
3	2.053	305	315	340	rBV	296074	432808	37.57%	4.875%
4	2.224	364	368	370	rVB3	546	442	0.04%	0.005%
5	2.240	371	373	377	rVB3	1272	672	0.06%	0.008%
6	2.346	402	406	410	rBV2	369	274	0.02%	0.003%
7	2.365	410	412	417	rVV2	281	271	0.02%	0.003%
8	2.404	421	424	427	rVB2	290	212	0.02%	0.002%
9	2.442	427	436	448	rBV3	4399	7803	0.68%	0.088%
10	2.558	460	472	483	rBV2	2430	5004	0.43%	0.056%
11	2.622	488	492	496	rBV2	280	218	0.02%	0.002%
12	2.651	496	501	506	rVB2	289	335	0.03%	0.004%
13	2.680	506	510	513	rBV2	304	249	0.02%	0.003%
14	2.751	530	532	538	rVB2	319	282	0.02%	0.003%
15	2.928	581	587	590	rVB2	353	281	0.02%	0.003%
16	3.426	739	742	743	rBV2	423	195	0.02%	0.002%
17	3.696	821	826	831	rBV2	229	347	0.03%	0.004%
18	3.783	844	853	885	rBV2	76116	222445	19.31%	2.506%
19	4.243	975	996	1029	rBV	196795	515343	44.74%	5.805%
20	4.535	1085	1087	1093	rVB5	389	319	0.03%	0.004%
21	4.587	1099	1103	1109	rBV4	381	487	0.04%	0.005%
22	4.616	1110	1112	1116	rVB2	374	203	0.02%	0.002%
23	4.674	1124	1130	1132	rVB3	298	221	0.02%	0.002%
24	4.950	1200	1216	1253	rBV2	434553	1151932	100.00%	12.976%
25	5.355	1340	1342	1349	rVB3	354	287	0.02%	0.003%
26	5.413	1357	1360	1365	rBV3	174	201	0.02%	0.002%
27	5.471	1374	1378	1381	rBV	304	284	0.02%	0.003%
28	5.529	1386	1396	1424	rBV	336981	720429	62.54%	8.115%
29	5.738	1459	1461	1463	rVB2	489	200	0.02%	0.002%
30	5.825	1478	1488	1510	rBV3	30045	70487	6.12%	0.794%
31	5.986	1525	1538	1564	rBV	246386	520037	45.14%	5.858%
32	6.217	1607	1610	1614	rBV2	412	348	0.03%	0.004%
33	6.236	1614	1616	1619	rVB2	557	280	0.02%	0.003%
34	6.256	1619	1622	1626	rBV3	318	285	0.02%	0.003%
35	6.400	1664	1667	1669	rBV	274	210	0.02%	0.002%
36	6.654	1743	1746	1751	rBV2	178	202	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072524\
 Data File : VW036685.D
 Acq On : 25 Jul 2024 00:58
 Operator : SY/MD
 Sample : P3335-12 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

37	6.715	1758	1765	1768	rBV2	266	358	0.03%	0.004%
38	6.912	1815	1826	1855	rBV	113391	223554	19.41%	2.518%
39	7.117	1887	1890	1895	rVB3	604	515	0.04%	0.006%
40	7.239	1917	1928	1963	rBV	490047	874015	75.87%	9.846%
41	7.551	2016	2025	2053	rBV	81305	157960	13.71%	1.779%
42	7.838	2111	2114	2118	rBV2	410	234	0.02%	0.003%
43	7.873	2120	2125	2126	rBV3	352	255	0.02%	0.003%
44	7.915	2131	2138	2146	rVB6	2340	3994	0.35%	0.045%
45	8.021	2163	2171	2198	rBV	223299	440731	38.26%	4.965%
46	8.358	2271	2276	2284	rVB6	701	1000	0.09%	0.011%
47	8.455	2302	2306	2312	rVB3	356	427	0.04%	0.005%
48	8.783	2397	2408	2439	rBV	559048	930556	80.78%	10.483%
49	9.014	2478	2480	2482	rBV2	375	215	0.02%	0.002%
50	9.101	2505	2507	2515	rBV3	548	660	0.06%	0.007%
51	9.146	2515	2521	2523	rVV2	242	296	0.03%	0.003%
52	9.249	2550	2553	2558	rVB2	417	241	0.02%	0.003%
53	9.310	2568	2572	2575	rBV	286	231	0.02%	0.003%
54	9.419	2601	2606	2611	rBV2	233	325	0.03%	0.004%
55	9.448	2612	2615	2620	rVV	236	262	0.02%	0.003%
56	9.747	2703	2708	2711	rBV2	225	207	0.02%	0.002%
57	9.889	2747	2752	2756	rBV3	408	395	0.03%	0.004%
58	10.149	2820	2833	2864	rBV	368151	591262	51.33%	6.660%
59	10.278	2870	2873	2876	rBV3	415	319	0.03%	0.004%
60	10.323	2883	2887	2891	rVB4	368	253	0.02%	0.003%
61	10.362	2897	2899	2908	rVB4	328	276	0.02%	0.003%
62	10.812	3035	3039	3041	rBV2	311	244	0.02%	0.003%
63	10.915	3069	3071	3076	rVB2	357	295	0.03%	0.003%
64	10.944	3076	3080	3082	rBV	317	302	0.03%	0.003%
65	11.040	3107	3110	3113	rBV	228	212	0.02%	0.002%
66	11.136	3135	3140	3144	rBV3	843	1086	0.09%	0.012%
67	11.181	3144	3154	3185	rVV	501705	794111	68.94%	8.945%
68	11.435	3230	3233	3236	rBV	477	271	0.02%	0.003%
69	11.558	3259	3271	3298	rBV	543199	862406	74.87%	9.715%
70	11.789	3341	3343	3348	rVB4	395	305	0.03%	0.003%
71	11.982	3399	3403	3405	rBV	308	235	0.02%	0.003%
72	12.001	3406	3409	3412	rVB2	373	291	0.03%	0.003%
73	12.027	3412	3417	3424	rBV	255	407	0.04%	0.005%
74	12.220	3469	3477	3479	rBV2	326	399	0.03%	0.004%
75	12.406	3533	3535	3540	rVB	429	241	0.02%	0.003%
76	12.442	3543	3546	3551	rBV2	305	301	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036685.D
 Acq On : 25 Jul 2024 00:58
 Operator : SY/MD
 Sample : P3335-12 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20K9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

77	12.522	3568	3571	3576	rBV2	301	286	0.02%	0.003%
78	12.603	3591	3596	3600	rBV2	433	426	0.04%	0.005%
79	12.853	3668	3674	3676	rBV2	217	229	0.02%	0.003%
80	12.998	3716	3719	3725	rBV2	327	346	0.03%	0.004%
81	13.140	3762	3763	3765	rBV	393	219	0.02%	0.002%
82	13.316	3815	3818	3820	rBV2	319	227	0.02%	0.003%
83	13.381	3835	3838	3842	rBV2	580	402	0.03%	0.005%
84	13.448	3856	3859	3861	rBV2	369	258	0.02%	0.003%
85	13.464	3861	3864	3868	rVV2	414	391	0.03%	0.004%
86	13.580	3896	3900	3903	rBV2	170	199	0.02%	0.002%
87	13.625	3912	3914	3917	rBV2	299	224	0.02%	0.003%
88	13.648	3917	3921	3928	rBV3	237	295	0.03%	0.003%
89	13.686	3929	3933	3936	rBV3	518	575	0.05%	0.006%
90	13.869	3988	3990	3995	rBV3	432	498	0.04%	0.006%
91	13.911	4000	4003	4007	rBV3	320	288	0.03%	0.003%
92	14.072	4048	4053	4056	rBV	372	399	0.03%	0.004%
93	14.201	4090	4093	4096	rVB2	386	240	0.02%	0.003%
94	14.233	4097	4103	4105	rBV2	417	472	0.04%	0.005%
95	14.365	4141	4144	4148	rBV2	297	246	0.02%	0.003%
96	14.721	4253	4255	4260	rVB4	368	235	0.02%	0.003%
97	14.760	4264	4267	4269	rBV3	328	198	0.02%	0.002%
98	15.094	4369	4371	4374	rBV2	420	219	0.02%	0.002%
99	15.275	4424	4427	4428	rBV2	594	281	0.02%	0.003%
100	15.937	4629	4633	4638	rBV5	943	917	0.08%	0.010%




Sum of corrected areas: 8877227

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036685.D
Acq On : 25 Jul 2024 00:58
Operator : SY/MD
Sample : P3335-12 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

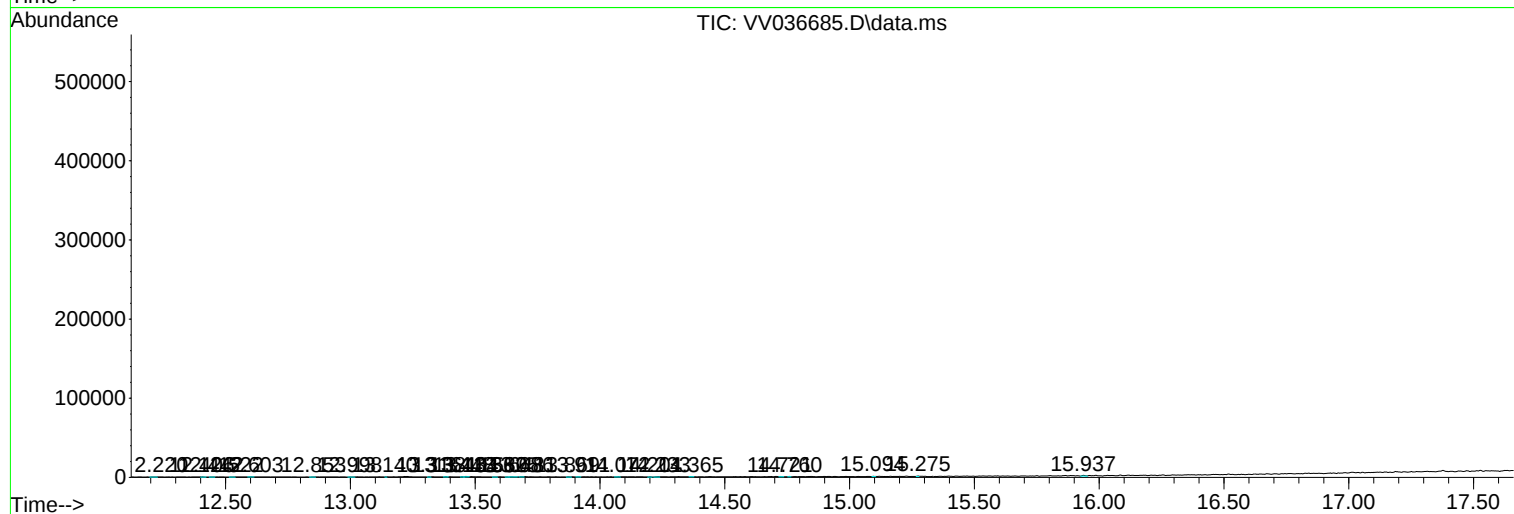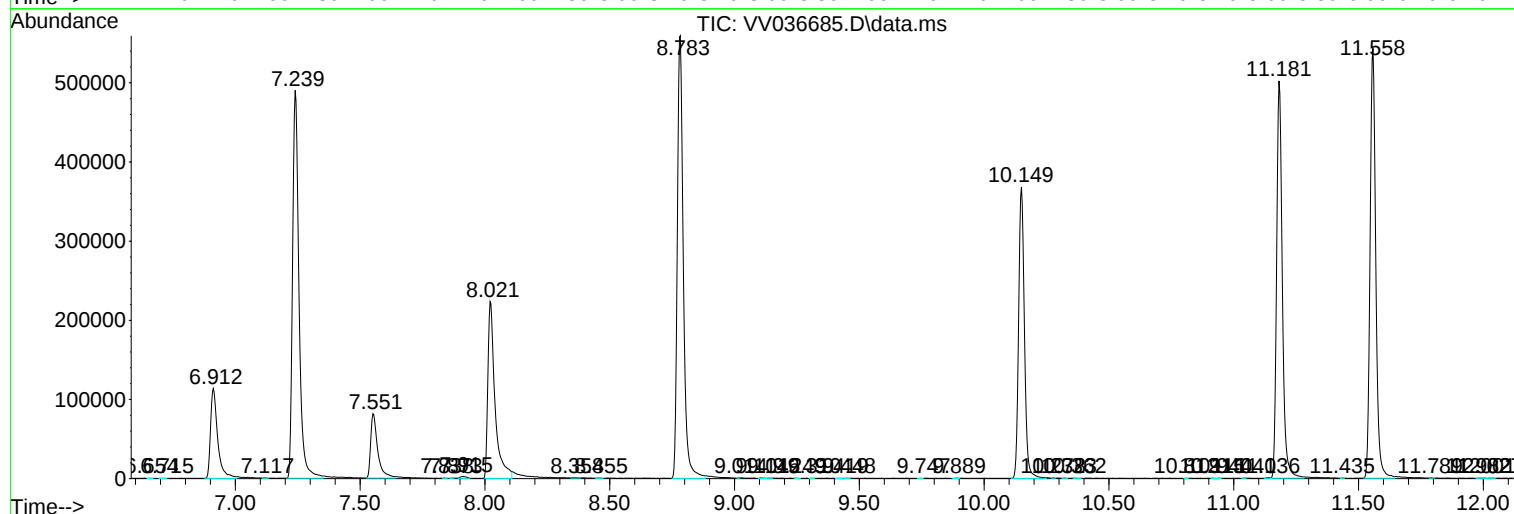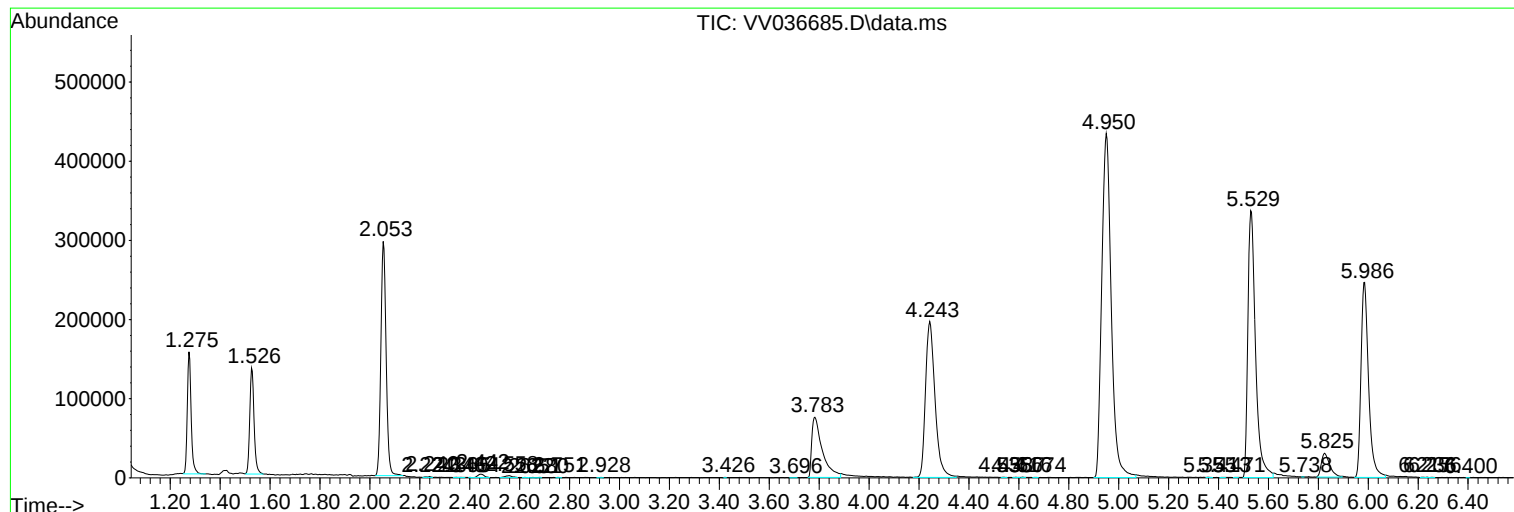

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036685.D
Acq On : 25 Jul 2024 00:58
Operator : SY/MD
Sample : P3335-12 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036685.D
Acq On : 25 Jul 2024 00:58
Operator : SY/MD
Sample : P3335-12 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc