

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036686.D
 Acq On : 25 Jul 2024 01:22
 Operator : SY/MD
 Sample : P3335-13 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M

Title : VOC Analysis

Signal : TIC: VV036686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	88	rVB	158084	167392	14.15%	1.832%
2	1.529	144	152	174	rVB	140228	173393	14.65%	1.898%
3	1.992	294	296	299	rVB3	1110	535	0.05%	0.006%
4	2.053	304	315	333	rBV	309986	456776	38.60%	5.000%
5	2.233	369	371	381	rVB3	1091	1166	0.10%	0.013%
6	2.310	390	395	396	rBV	249	177	0.01%	0.002%
7	2.375	411	415	417	rBV	246	189	0.02%	0.002%
8	2.445	427	437	447	rVB4	3850	7019	0.59%	0.077%
9	2.494	447	452	455	rBV3	404	432	0.04%	0.005%
10	2.555	462	471	482	rBV4	1534	3247	0.27%	0.036%
11	2.641	496	498	503	rVB2	302	264	0.02%	0.003%
12	2.867	564	568	571	rBV2	240	200	0.02%	0.002%
13	3.005	607	611	612	rBV	254	195	0.02%	0.002%
14	3.130	647	650	656	rVB	264	276	0.02%	0.003%
15	3.169	656	662	669	rBV2	319	528	0.04%	0.006%
16	3.336	710	714	717	rBV	194	199	0.02%	0.002%
17	3.584	786	791	796	rVB2	245	178	0.02%	0.002%
18	3.699	822	827	831	rBV	273	252	0.02%	0.003%
19	3.728	831	836	839	rBV2	261	284	0.02%	0.003%
20	3.783	843	853	896	rBV	74868	232227	19.62%	2.542%
21	4.185	974	978	980	rBV3	387	306	0.03%	0.003%
22	4.243	980	996	1026	rVV	198415	520197	43.96%	5.694%
23	4.632	1112	1117	1120	rBV3	486	403	0.03%	0.004%
24	4.719	1142	1144	1149	rVB2	238	222	0.02%	0.002%
25	4.754	1149	1155	1156	rBV	285	237	0.02%	0.003%
26	4.950	1201	1216	1255	rBV2	443275	1183345	100.00%	12.953%
27	5.159	1280	1281	1284	rVB	611	212	0.02%	0.002%
28	5.175	1284	1286	1288	rBV3	643	321	0.03%	0.004%
29	5.481	1378	1381	1386	rBV2	307	303	0.03%	0.003%
30	5.532	1386	1397	1432	rBV	337883	722740	61.08%	7.911%
31	5.825	1477	1488	1519	rVB	33619	79338	6.70%	0.868%
32	5.982	1526	1537	1570	rBV	251289	530622	44.84%	5.808%
33	6.201	1603	1605	1608	rVB4	392	181	0.02%	0.002%
34	6.773	1778	1783	1787	rBV2	289	383	0.03%	0.004%
35	6.815	1791	1796	1798	rBV2	369	336	0.03%	0.004%
36	6.911	1816	1826	1852	rBV	115965	227838	19.25%	2.494%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036686.D
 Acq On : 25 Jul 2024 01:22
 Operator : SY/MD
 Sample : P3335-13 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

37	7.153	1899	1901	1904	rBV3	341	205	0.02%	0.002%
38	7.239	1917	1928	1967	rBV	509257	908653	76.79%	9.946%
39	7.551	2016	2025	2053	rBV	83013	160624	13.57%	1.758%
40	7.808	2102	2105	2110	rBV3	420	339	0.03%	0.004%
41	7.863	2118	2122	2123	rBV2	261	178	0.02%	0.002%
42	7.911	2131	2137	2152	rVB6	2171	3867	0.33%	0.042%
43	8.021	2162	2171	2212	rBV	220519	453421	38.32%	4.963%
44	8.278	2249	2251	2256	rVB3	555	407	0.03%	0.004%
45	8.316	2261	2263	2266	rVB2	465	196	0.02%	0.002%
46	8.529	2326	2329	2333	rBV2	208	185	0.02%	0.002%
47	8.609	2353	2354	2358	rVB2	339	202	0.02%	0.002%
48	8.699	2381	2382	2385	rVB2	386	184	0.02%	0.002%
49	8.722	2385	2389	2392	rBV	276	255	0.02%	0.003%
50	8.783	2397	2408	2448	rBV	561979	944326	79.80%	10.337%
51	9.117	2509	2512	2515	rVB2	440	235	0.02%	0.003%
52	9.204	2535	2539	2543	rBV2	492	306	0.03%	0.003%
53	9.313	2568	2573	2576	rBV	372	364	0.03%	0.004%
54	9.413	2596	2604	2610	rBV2	215	368	0.03%	0.004%
55	9.509	2632	2634	2641	rVB2	313	302	0.03%	0.003%
56	9.577	2651	2655	2659	rVB	247	182	0.02%	0.002%
57	9.677	2682	2686	2690	rVB	210	185	0.02%	0.002%
58	9.728	2696	2702	2704	rBV	317	267	0.02%	0.003%
59	9.873	2744	2747	2751	rVB	285	203	0.02%	0.002%
60	10.037	2795	2798	2804	rVB	163	178	0.02%	0.002%
61	10.149	2822	2833	2860	rBV	378955	598051	50.54%	6.546%
62	10.413	2910	2915	2917	rBV	441	425	0.04%	0.005%
63	10.612	2974	2977	2980	rVV2	337	288	0.02%	0.003%
64	10.628	2980	2982	2987	rVB2	268	214	0.02%	0.002%
65	10.866	3052	3056	3061	rBV2	308	431	0.04%	0.005%
66	11.066	3115	3118	3120	rBV	243	185	0.02%	0.002%
67	11.133	3136	3139	3144	rBV3	702	881	0.07%	0.010%
68	11.181	3144	3154	3187	rVV	517944	820115	69.30%	8.977%
69	11.445	3233	3236	3239	rBV2	262	233	0.02%	0.003%
70	11.557	3258	3271	3301	rBV	576694	917556	77.54%	10.044%
71	11.795	3343	3345	3347	rVV2	353	208	0.02%	0.002%
72	11.808	3347	3349	3355	rVB3	416	258	0.02%	0.003%
73	11.927	3381	3386	3390	rBV2	343	427	0.04%	0.005%
74	12.053	3423	3425	3429	rVB2	318	190	0.02%	0.002%
75	12.088	3431	3436	3440	rBV2	302	309	0.03%	0.003%
76	12.114	3440	3444	3447	rBV2	277	222	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036686.D
 Acq On : 25 Jul 2024 01:22
 Operator : SY/MD
 Sample : P3335-13 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20L0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

77	12.281	3494	3496	3501	rVB2	326	239	0.02%	0.003%
78	12.480	3554	3558	3560	rBV	375	237	0.02%	0.003%
79	12.529	3570	3573	3578	rBV3	379	380	0.03%	0.004%
80	12.564	3578	3584	3586	rVB2	331	316	0.03%	0.003%
81	12.583	3586	3590	3591	rBV2	321	223	0.02%	0.002%
82	12.821	3661	3664	3670	rVB2	371	251	0.02%	0.003%
83	12.898	3685	3688	3693	rBV2	354	329	0.03%	0.004%
84	12.959	3703	3707	3711	rVB3	376	290	0.02%	0.003%
85	13.213	3783	3786	3787	rBV	666	389	0.03%	0.004%
86	13.307	3811	3815	3819	rVB3	272	273	0.02%	0.003%
87	13.368	3829	3834	3838	rBV4	370	426	0.04%	0.005%
88	13.464	3855	3864	3871	rBV4	702	1266	0.11%	0.014%
89	13.551	3887	3891	3894	rVB3	392	311	0.03%	0.003%
90	13.580	3894	3900	3901	rBV2	283	257	0.02%	0.003%
91	13.840	3979	3981	3985	rVB2	309	193	0.02%	0.002%
92	13.869	3987	3990	3994	rBV2	337	276	0.02%	0.003%
93	13.946	4005	4014	4015	rBV3	455	636	0.05%	0.007%
94	14.188	4086	4089	4091	rBV2	303	238	0.02%	0.003%
95	14.268	4112	4114	4119	rBV3	235	200	0.02%	0.002%
96	14.541	4197	4199	4203	rBV2	388	243	0.02%	0.003%
97	14.667	4235	4238	4242	rVB2	499	338	0.03%	0.004%
98	14.824	4283	4287	4289	rBV2	271	227	0.02%	0.002%
99	14.847	4291	4294	4295	rBV2	313	175	0.01%	0.002%
100	14.982	4333	4336	4339	rBV	513	330	0.03%	0.004%




Sum of corrected areas: 9135581

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036686.D
Acq On : 25 Jul 2024 01:22
Operator : SY/MD
Sample : P3335-13 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20L0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

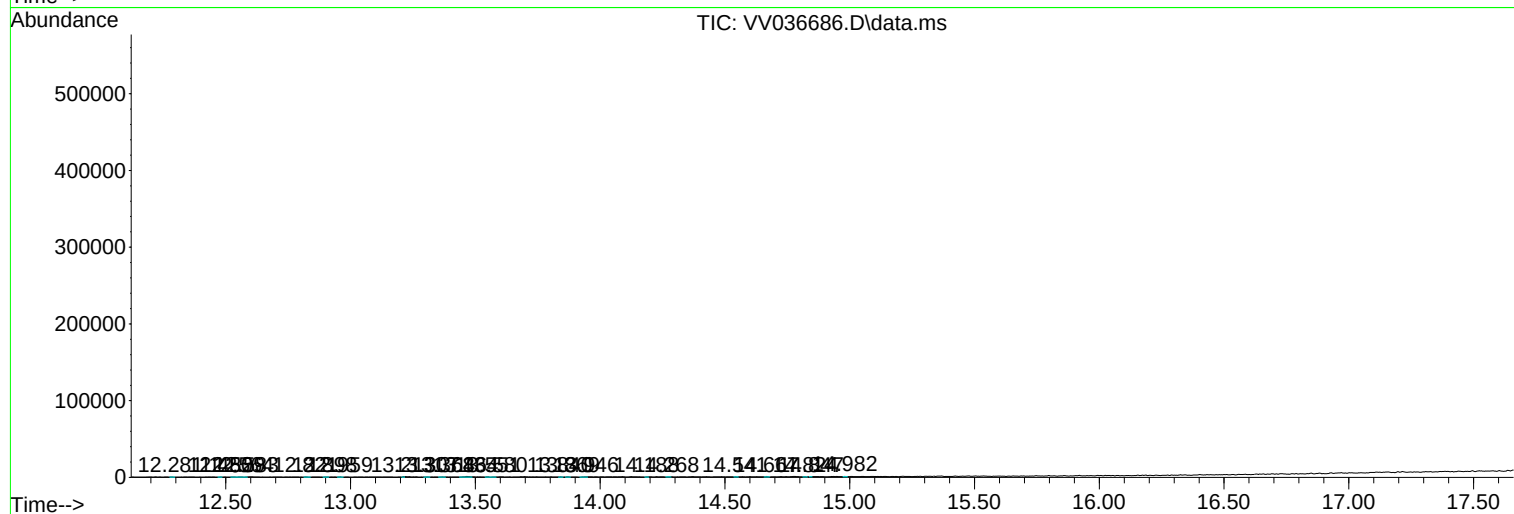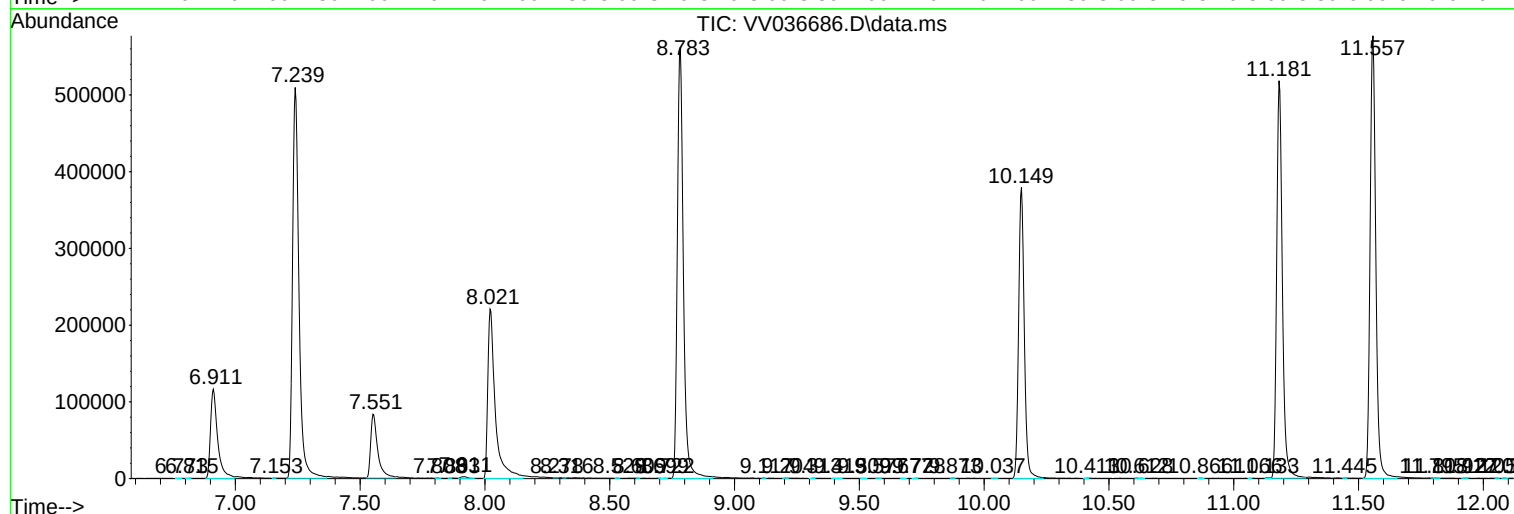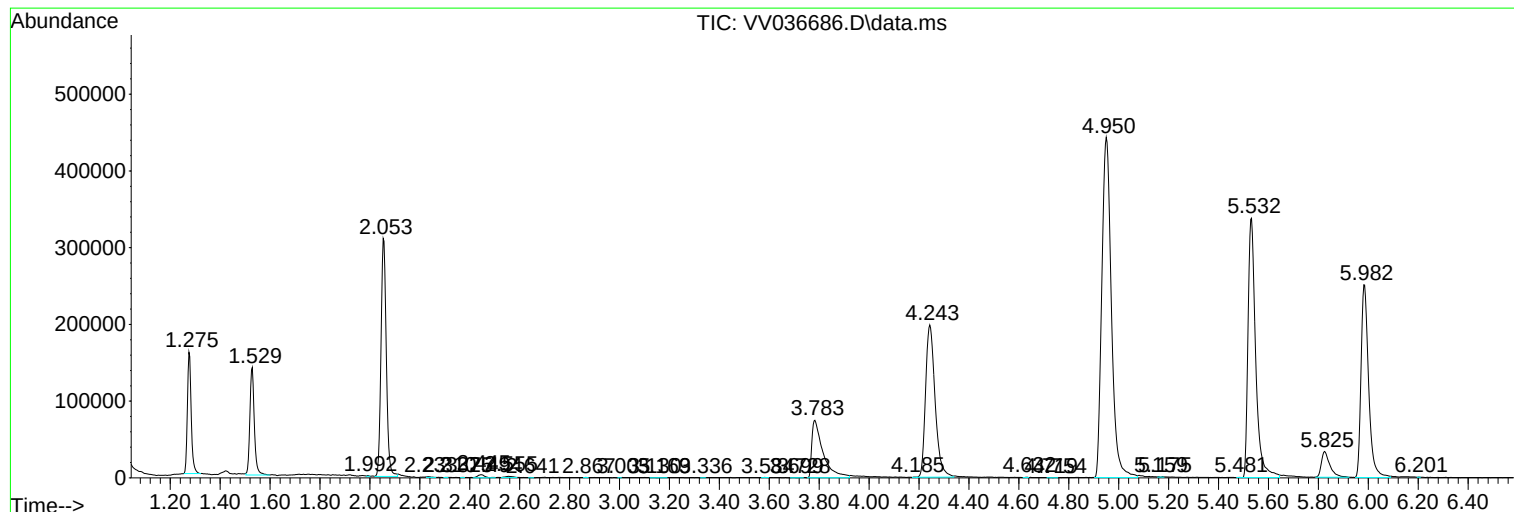

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036686.D
Acq On : 25 Jul 2024 01:22
Operator : SY/MD
Sample : P3335-13 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20L0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036686.D
Acq On : 25 Jul 2024 01:22
Operator : SY/MD
Sample : P3335-13 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20L0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc