

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036688.D
 Acq On : 25 Jul 2024 02:10
 Operator : SY/MD
 Sample : P3335-15 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M

Title : VOC Analysis

Signal : TIC: VV036688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	94	rVB	156988	169085	14.62%	1.756%
2	1.526	144	151	164	rVB	135677	160589	13.88%	1.667%
3	2.053	305	315	346	rVB	308387	463477	40.07%	4.812%
4	2.233	365	371	378	rVB3	854	1205	0.10%	0.013%
5	2.446	429	437	446	rBV4	3427	5510	0.48%	0.057%
6	2.552	462	470	474	rBV3	1347	2197	0.19%	0.023%
7	2.622	486	492	494	rBV2	188	228	0.02%	0.002%
8	2.667	502	506	510	rBV2	239	248	0.02%	0.003%
9	2.703	514	517	523	rVV2	420	417	0.04%	0.004%
10	2.831	552	557	559	rBV	226	196	0.02%	0.002%
11	2.976	599	602	607	rVV2	223	188	0.02%	0.002%
12	3.021	613	616	619	rBV2	219	194	0.02%	0.002%
13	3.092	634	638	640	rBV2	264	227	0.02%	0.002%
14	3.323	706	710	713	rBV	239	174	0.02%	0.002%
15	3.368	717	724	727	rBV2	326	468	0.04%	0.005%
16	3.381	727	728	735	rVB3	208	169	0.01%	0.002%
17	3.462	749	753	759	rVV2	162	200	0.02%	0.002%
18	3.548	777	780	782	rVB3	261	167	0.01%	0.002%
19	3.780	844	852	885	rBV	72607	226246	19.56%	2.349%
20	4.243	980	996	1028	rBV	195656	514616	44.49%	5.343%
21	4.532	1081	1086	1088	rBV4	446	421	0.04%	0.004%
22	4.548	1088	1091	1093	rBV2	259	207	0.02%	0.002%
23	4.767	1155	1159	1161	rBV3	234	170	0.01%	0.002%
24	4.950	1201	1216	1247	rBV2	440169	1156641	100.00%	12.010%
25	5.201	1292	1294	1299	rBV4	336	242	0.02%	0.003%
26	5.230	1301	1303	1307	rVB3	547	291	0.03%	0.003%
27	5.317	1328	1330	1335	rVB3	311	250	0.02%	0.003%
28	5.352	1339	1341	1347	rVB2	357	295	0.03%	0.003%
29	5.529	1384	1396	1430	rBV	340627	723072	62.51%	7.508%
30	5.828	1475	1489	1524	rVV3	316815	691177	59.76%	7.177%
31	5.982	1525	1537	1565	rVV	249262	516694	44.67%	5.365%
32	6.410	1668	1670	1673	rBV	271	179	0.02%	0.002%
33	6.455	1681	1684	1687	rVB2	423	245	0.02%	0.003%
34	6.516	1698	1703	1705	rVV2	245	180	0.02%	0.002%
35	6.535	1705	1709	1714	rVB2	169	195	0.02%	0.002%
36	6.632	1734	1739	1741	rBV2	168	189	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072524\
 Data File : VW036688.D
 Acq On : 25 Jul 2024 02:10
 Operator : SY/MD
 Sample : P3335-15 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

37	6.741	1768	1773	1776	rBV2	232	281	0.02%	0.003%
38	6.912	1816	1826	1856	rBV	114333	225802	19.52%	2.345%
39	7.082	1877	1879	1884	rVB3	433	376	0.03%	0.004%
40	7.108	1884	1887	1891	rBV2	360	324	0.03%	0.003%
41	7.240	1917	1928	1964	rBV	498641	897622	77.61%	9.320%
42	7.551	2016	2025	2059	rBV	81555	161209	13.94%	1.674%
43	7.796	2099	2101	2109	rVB3	361	354	0.03%	0.004%
44	7.854	2117	2119	2122	rVV	394	215	0.02%	0.002%
45	7.873	2122	2125	2129	rVV3	508	491	0.04%	0.005%
46	7.912	2131	2137	2146	rVB4	2141	3167	0.27%	0.033%
47	7.976	2153	2157	2162	rVB3	235	171	0.01%	0.002%
48	8.021	2162	2171	2212	rBV	219468	446430	38.60%	4.635%
49	8.227	2233	2235	2239	rVB3	981	616	0.05%	0.006%
50	8.494	2314	2318	2320	rBV3	391	255	0.02%	0.003%
51	8.564	2337	2340	2343	rVB2	338	175	0.02%	0.002%
52	8.587	2343	2347	2353	rVB2	267	317	0.03%	0.003%
53	8.645	2362	2365	2369	rBV	256	232	0.02%	0.002%
54	8.703	2379	2383	2388	rBV4	431	325	0.03%	0.003%
55	8.783	2396	2408	2441	rBV	560920	941113	81.37%	9.772%
56	9.024	2480	2483	2486	rBV2	468	268	0.02%	0.003%
57	9.117	2510	2512	2516	rBV2	433	312	0.03%	0.003%
58	9.243	2548	2551	2555	rBV	359	204	0.02%	0.002%
59	9.413	2601	2604	2606	rBV3	321	270	0.02%	0.003%
60	9.686	2686	2689	2692	rBV	272	193	0.02%	0.002%
61	9.796	2720	2723	2727	rVB2	233	179	0.02%	0.002%
62	10.011	2787	2790	2794	rBV	196	227	0.02%	0.002%
63	10.101	2815	2818	2822	rBV2	212	247	0.02%	0.003%
64	10.149	2822	2833	2855	rBV	370031	583183	50.42%	6.055%
65	10.384	2902	2906	2912	rVB3	346	362	0.03%	0.004%
66	10.436	2916	2922	2925	rBV2	209	199	0.02%	0.002%
67	10.625	2974	2981	2984	rBV2	206	219	0.02%	0.002%
68	10.686	2996	3000	3003	rBV2	191	207	0.02%	0.002%
69	10.821	3038	3042	3049	rBV2	317	441	0.04%	0.005%
70	10.911	3066	3070	3073	rBV	249	204	0.02%	0.002%
71	11.079	3119	3122	3126	rBV2	289	202	0.02%	0.002%
72	11.182	3143	3154	3180	rBV	513783	818402	70.76%	8.498%
73	11.432	3230	3232	3238	rVB4	410	393	0.03%	0.004%
74	11.558	3256	3271	3300	rBV	563434	901170	77.91%	9.357%
75	12.046	3420	3423	3427	rBV2	280	225	0.02%	0.002%
76	12.091	3433	3437	3439	rBV2	269	191	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036688.D
 Acq On : 25 Jul 2024 02:10
 Operator : SY/MD
 Sample : P3335-15 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

77	12.387	3526	3529	3532	rBV	224	201	0.02%	0.002%
78	12.429	3539	3542	3546	rVB2	505	306	0.03%	0.003%
79	12.455	3546	3550	3553	rBV	367	330	0.03%	0.003%
80	12.593	3589	3593	3594	rBV3	565	370	0.03%	0.004%
81	12.689	3619	3623	3627	rVB2	484	491	0.04%	0.005%
82	12.712	3627	3630	3634	rBV	391	343	0.03%	0.004%
83	12.751	3638	3642	3645	rBV2	275	248	0.02%	0.003%
84	13.104	3749	3752	3756	rBV2	266	213	0.02%	0.002%
85	13.149	3764	3766	3772	rVB2	311	216	0.02%	0.002%
86	13.214	3782	3786	3791	rBV4	542	632	0.05%	0.007%
87	13.329	3819	3822	3825	rBV2	348	199	0.02%	0.002%
88	13.349	3825	3828	3833	rBV2	178	190	0.02%	0.002%
89	13.448	3855	3859	3861	rBV	285	177	0.02%	0.002%
90	13.477	3865	3868	3877	rVB2	406	431	0.04%	0.004%
91	13.574	3895	3898	3901	rBV2	358	248	0.02%	0.003%
92	13.603	3904	3907	3911	rVV	312	297	0.03%	0.003%
93	13.741	3946	3950	3952	rBV	290	198	0.02%	0.002%
94	13.882	3991	3994	3999	rBV	378	369	0.03%	0.004%
95	14.001	4027	4031	4036	rBV3	355	355	0.03%	0.004%
96	14.474	4175	4178	4184	rBV2	302	297	0.03%	0.003%
97	14.506	4185	4188	4191	rBV3	345	306	0.03%	0.003%
98	15.223	4408	4411	4413	rBV2	357	227	0.02%	0.002%
99	15.722	4565	4566	4570	rBV3	575	351	0.03%	0.004%
100	15.905	4620	4623	4626	rBV3	1094	706	0.06%	0.007%


Sum of corrected areas: 9630723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036688.D
Acq On : 25 Jul 2024 02:10
Operator : SY/MD
Sample : P3335-15 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

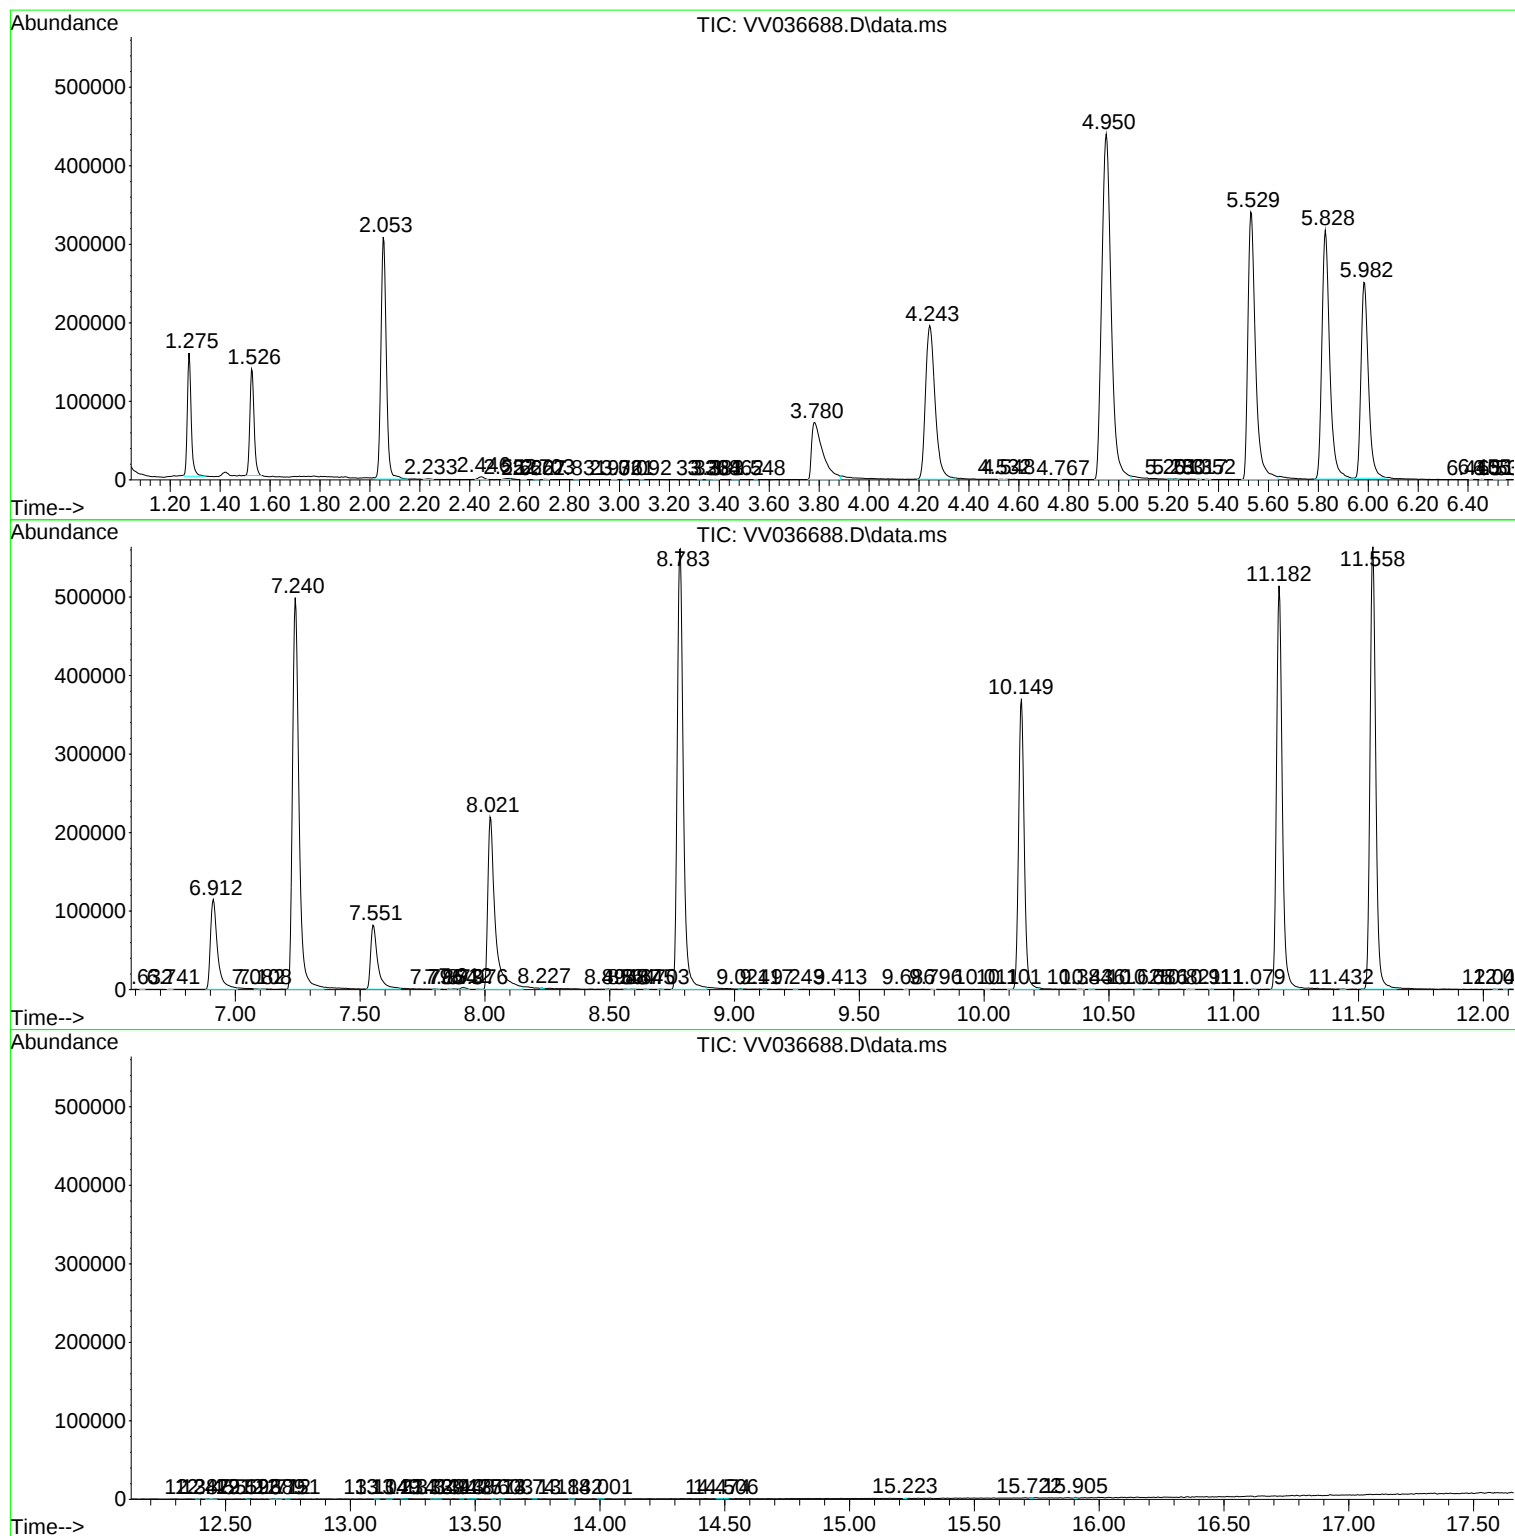

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036688.D
Acq On : 25 Jul 2024 02:10
Operator : SY/MD
Sample : P3335-15 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036688.D
Acq On : 25 Jul 2024 02:10
Operator : SY/MD
Sample : P3335-15 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
