

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036689.D
 Acq On : 25 Jul 2024 02:34
 Operator : SY/MD
 Sample : P3335-16 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

Signal : TIC: VV036689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	87	rVB	156632	165079	14.12%	1.670%
2	1.526	145	151	165	rVB	134876	163827	14.01%	1.658%
3	2.053	306	315	338	rVB	315137	464786	39.75%	4.702%
4	2.404	421	424	427	rVB2	349	225	0.02%	0.002%
5	2.449	427	438	448	rBV4	3904	7260	0.62%	0.073%
6	2.555	462	471	484	rVB2	3135	6068	0.52%	0.061%
7	2.645	496	499	501	rBV2	292	147	0.01%	0.001%
8	2.654	501	502	503	rBV2	182	56	0.00%	0.001%
9	2.664	503	505	507	rVV	187	78	0.01%	0.001%
10	2.693	511	514	516	rBV	336	206	0.02%	0.002%
11	2.741	528	529	531	rBV	86	48	0.00%	0.000%
12	2.777	538	540	541	rBV	121	45	0.00%	0.000%
13	2.860	565	566	568	rBV	122	45	0.00%	0.000%
14	2.925	584	586	589	rBV2	90	69	0.01%	0.001%
15	2.960	593	597	600	rBV2	152	173	0.01%	0.002%
16	3.018	610	615	621	rBV	221	287	0.02%	0.003%
17	3.044	621	623	625	rBV	120	80	0.01%	0.001%
18	3.060	625	628	629	rBV	130	61	0.01%	0.001%
19	3.111	640	644	646	rBV	202	98	0.01%	0.001%
20	3.127	648	649	652	rVV2	111	60	0.01%	0.001%
21	3.175	661	664	668	rBV2	204	159	0.01%	0.002%
22	3.198	669	671	673	rVB	115	47	0.00%	0.000%
23	3.214	673	676	677	rBV2	276	128	0.01%	0.001%
24	3.259	688	690	692	rBV	133	94	0.01%	0.001%
25	3.304	700	704	706	rBV	193	147	0.01%	0.001%
26	3.368	717	724	726	rBV	214	250	0.02%	0.003%
27	3.497	760	764	769	rBV2	173	250	0.02%	0.003%
28	3.555	779	782	783	rBV2	135	57	0.00%	0.001%
29	3.606	793	798	802	rBV	169	179	0.02%	0.002%
30	3.635	806	807	809	rVB	146	31	0.00%	0.000%
31	3.648	809	811	814	rBV	173	78	0.01%	0.001%
32	3.661	814	815	817	rBV	106	53	0.00%	0.001%
33	3.783	844	853	888	rBV2	76940	241740	20.67%	2.446%
34	4.243	981	996	1032	rBV	198107	512053	43.79%	5.181%
35	4.635	1117	1118	1122	rVB2	310	203	0.02%	0.002%
36	4.661	1124	1126	1131	rVB3	381	251	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036689.D
 Acq On : 25 Jul 2024 02:34
 Operator : SY/MD
 Sample : P3335-16 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

37	4.738	1147	1150	1153	rBV	229	133	0.01%	0.001%
38	4.777	1160	1162	1165	rBV	200	138	0.01%	0.001%
39	4.834	1178	1180	1182	rBB2	188	70	0.01%	0.001%
40	4.899	1197	1200	1201	rBV2	191	83	0.01%	0.001%
41	4.950	1201	1216	1252	rBV2	438471	1169264	100.00%	11.830%
42	5.387	1349	1352	1357	rVB2	374	296	0.03%	0.003%
43	5.420	1357	1362	1365	rBV2	411	276	0.02%	0.003%
44	5.449	1365	1371	1375	rBV3	273	370	0.03%	0.004%
45	5.529	1386	1396	1429	rBV	351107	741849	63.45%	7.506%
46	5.828	1476	1489	1525	rBV3	369241	796758	68.14%	8.061%
47	5.982	1526	1537	1565	rVV	248971	518708	44.36%	5.248%
48	6.355	1650	1653	1657	rVV5	380	257	0.02%	0.003%
49	6.381	1659	1661	1665	rVB2	355	210	0.02%	0.002%
50	6.420	1671	1673	1675	rBB2	152	61	0.01%	0.001%
51	6.465	1684	1687	1690	rBV	159	157	0.01%	0.002%
52	6.641	1739	1742	1744	rVB2	135	86	0.01%	0.001%
53	6.658	1744	1747	1749	rBV	222	157	0.01%	0.002%
54	6.683	1753	1755	1758	rVB2	271	152	0.01%	0.002%
55	6.812	1793	1795	1798	rBV	150	121	0.01%	0.001%
56	6.854	1805	1808	1810	rBV2	125	91	0.01%	0.001%
57	6.912	1816	1826	1853	rBV	113259	223957	19.15%	2.266%
58	7.133	1893	1895	1898	rBV2	275	135	0.01%	0.001%
59	7.239	1917	1928	1966	rBV	523349	929195	79.47%	9.401%
60	7.551	2017	2025	2047	rBV	82083	153688	13.14%	1.555%
61	7.825	2109	2110	2113	rBV	337	111	0.01%	0.001%
62	7.915	2131	2138	2145	rVB6	1917	2967	0.25%	0.030%
63	7.944	2145	2147	2149	rVB	126	32	0.00%	0.000%
64	7.976	2153	2157	2162	rVB3	290	312	0.03%	0.003%
65	8.021	2162	2171	2202	rBV	211391	430715	36.84%	4.358%
66	8.551	2334	2336	2337	rBV	246	78	0.01%	0.001%
67	8.590	2346	2348	2351	rVB2	340	179	0.02%	0.002%
68	8.654	2365	2368	2370	rBV2	207	148	0.01%	0.001%
69	8.725	2387	2390	2393	rVB2	297	211	0.02%	0.002%
70	8.744	2393	2396	2397	rBV2	197	139	0.01%	0.001%
71	8.783	2397	2408	2442	rBV	580685	974457	83.34%	9.859%
72	9.249	2550	2553	2557	rBV	266	190	0.02%	0.002%
73	9.288	2562	2565	2569	rBV	211	234	0.02%	0.002%
74	9.310	2570	2572	2575	rVB2	340	185	0.02%	0.002%
75	9.333	2575	2579	2582	rBV2	136	162	0.01%	0.002%
76	9.513	2632	2635	2638	rBV	292	238	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036689.D
 Acq On : 25 Jul 2024 02:34
 Operator : SY/MD
 Sample : P3335-16 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

77	9.677	2683	2686	2690	rBV	202	135	0.01%	0.001%
78	9.699	2690	2693	2695	rBV2	176	135	0.01%	0.001%
79	9.741	2703	2706	2709	rVB2	273	191	0.02%	0.002%
80	9.760	2709	2712	2714	rBV	167	121	0.01%	0.001%
81	9.841	2735	2737	2739	rBV	116	66	0.01%	0.001%
82	9.998	2782	2786	2790	rBV2	270	332	0.03%	0.003%
83	10.108	2818	2820	2821	rBV	136	56	0.00%	0.001%
84	10.149	2821	2833	2863	rVV	364144	584346	49.98%	5.912%
85	10.587	2966	2969	2973	rBV	123	122	0.01%	0.001%
86	10.818	3039	3041	3043	rBV	95	49	0.00%	0.000%
87	11.008	3097	3100	3103	rBV2	191	179	0.02%	0.002%
88	11.181	3144	3154	3182	rBV	533867	863091	73.81%	8.732%
89	11.558	3259	3271	3294	rBV	576416	921657	78.82%	9.325%
90	12.024	3411	3416	3418	rBV2	368	349	0.03%	0.004%
91	12.101	3437	3440	3443	rBV2	262	250	0.02%	0.003%
92	12.358	3517	3520	3522	rBV	239	163	0.01%	0.002%
93	12.390	3528	3530	3532	rBV2	209	102	0.01%	0.001%
94	12.802	3656	3658	3660	rBV	303	117	0.01%	0.001%
95	12.837	3666	3669	3672	rBV	340	176	0.02%	0.002%
96	13.117	3755	3756	3758	rVB	228	68	0.01%	0.001%
97	13.214	3782	3786	3788	rBV3	653	545	0.05%	0.006%
98	13.442	3855	3857	3861	rBV	337	293	0.03%	0.003%
99	13.686	3930	3933	3935	rBV3	465	342	0.03%	0.003%
100	13.911	4001	4003	4005	rBV	212	107	0.01%	0.001%




Sum of corrected areas: 9883980

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036689.D
Acq On : 25 Jul 2024 02:34
Operator : SY/MD
Sample : P3335-16 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

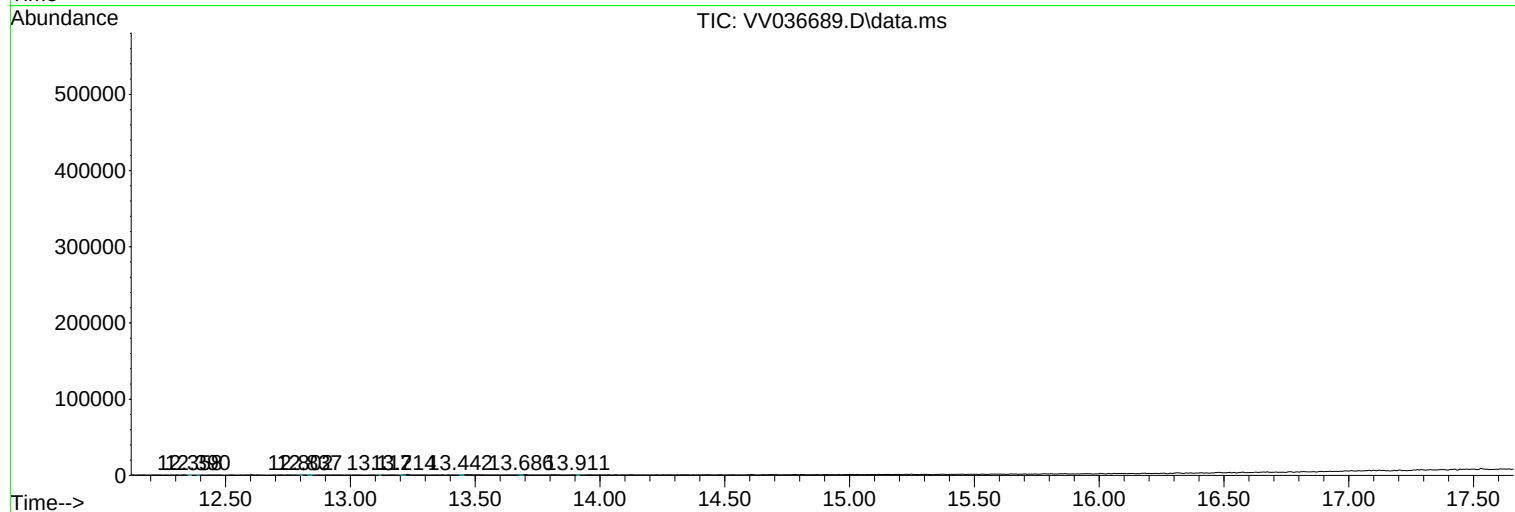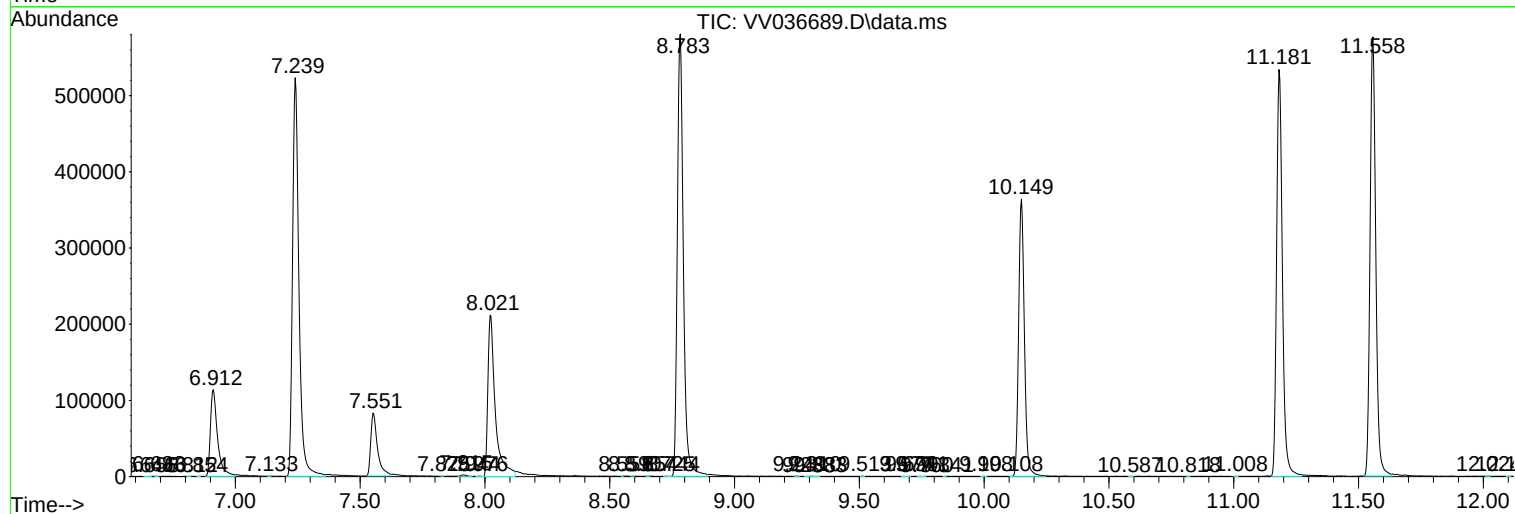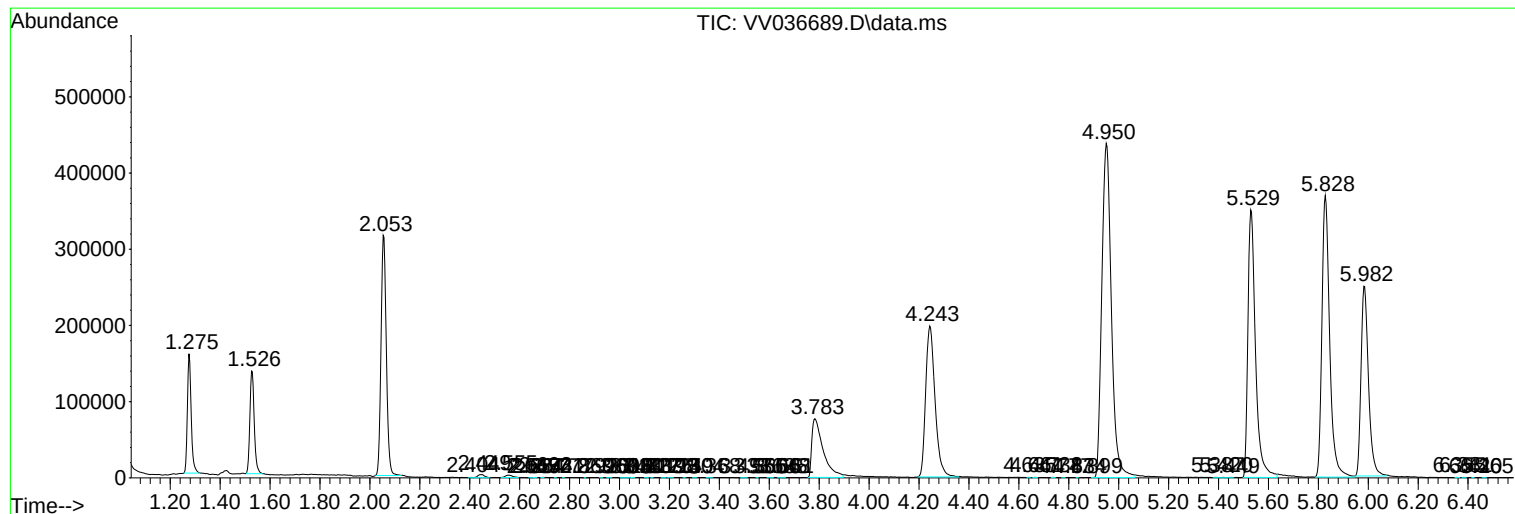

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036689.D
Acq On : 25 Jul 2024 02:34
Operator : SY/MD
Sample : P3335-16 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036689.D
Acq On : 25 Jul 2024 02:34
Operator : SY/MD
Sample : P3335-16 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------