

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036690.D
 Acq On : 25 Jul 2024 02:58
 Operator : SY/MD
 Sample : P3335-17 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

Signal : TIC: VV036690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	88	rVB	156830	167318	14.38%	1.830%
2	1.529	144	152	165	rVB	133964	161368	13.86%	1.765%
3	2.053	304	315	336	rBV	307338	451622	38.80%	4.939%
4	2.172	349	352	357	rVB3	512	450	0.04%	0.005%
5	2.227	362	369	370	rBV2	697	611	0.05%	0.007%
6	2.336	399	403	406	rBV2	291	248	0.02%	0.003%
7	2.445	425	437	448	rVB5	3405	6286	0.54%	0.069%
8	2.490	448	451	454	rVB3	444	318	0.03%	0.003%
9	2.510	454	457	460	rBV2	232	229	0.02%	0.003%
10	2.555	460	471	484	rVV2	2087	4472	0.38%	0.049%
11	2.606	484	487	491	rVB3	253	216	0.02%	0.002%
12	3.426	739	742	747	rBV	250	296	0.03%	0.003%
13	3.535	770	776	779	rBV	250	231	0.02%	0.003%
14	3.783	842	853	901	rBV2	74102	226471	19.46%	2.477%
15	4.085	944	947	949	rBV2	522	368	0.03%	0.004%
16	4.114	953	956	963	rBV2	496	544	0.05%	0.006%
17	4.243	977	996	1031	rBV	196779	514291	44.19%	5.624%
18	4.535	1083	1087	1091	rBV2	435	436	0.04%	0.005%
19	4.609	1108	1110	1114	rVB2	629	304	0.03%	0.003%
20	4.635	1114	1118	1123	rBV2	440	410	0.04%	0.004%
21	4.661	1123	1126	1131	rVB2	360	349	0.03%	0.004%
22	4.706	1131	1140	1143	rBV3	483	600	0.05%	0.007%
23	4.812	1170	1173	1178	rBV2	224	218	0.02%	0.002%
24	4.883	1193	1195	1201	rVB2	324	234	0.02%	0.003%
25	4.950	1201	1216	1259	rBV2	431971	1163876	100.00%	12.728%
26	5.381	1345	1350	1351	rBV2	506	285	0.02%	0.003%
27	5.449	1367	1371	1372	rBV	361	275	0.02%	0.003%
28	5.468	1375	1377	1381	rVB2	350	208	0.02%	0.002%
29	5.529	1386	1396	1436	rBV	350291	749328	64.38%	8.194%
30	5.825	1476	1488	1522	rVB5	42127	110387	9.48%	1.207%
31	5.985	1526	1538	1571	rBV	245251	520319	44.71%	5.690%
32	6.146	1584	1588	1589	rBV2	517	351	0.03%	0.004%
33	6.204	1604	1606	1611	rVB3	765	430	0.04%	0.005%
34	6.230	1611	1614	1617	rVB2	492	306	0.03%	0.003%
35	6.265	1621	1625	1630	rBV3	717	857	0.07%	0.009%
36	6.580	1720	1723	1726	rVB	400	220	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072524\
Data File : VW036690.D
Acq On : 25 Jul 2024 02:58
Operator : SY/MD
Sample : P3335-17 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Title : VOC Analysis

37	6.603	1726	1730	1735	rBV2	299	340	0.03%	0.004%
38	6.911	1814	1826	1854	rBV	112550	223126	19.17%	2.440%
39	7.101	1883	1885	1889	rVB3	360	263	0.02%	0.003%
40	7.239	1918	1928	1963	rBV	505726	911518	78.32%	9.968%
41	7.551	2016	2025	2051	rBV	80192	154908	13.31%	1.694%
42	7.715	2074	2076	2080	rVB2	679	371	0.03%	0.004%
43	7.767	2089	2092	2093	rBV2	422	259	0.02%	0.003%
44	7.915	2130	2138	2147	rVB6	1939	3279	0.28%	0.036%
45	8.021	2162	2171	2213	rBV	212911	444535	38.19%	4.861%
46	8.464	2306	2309	2316	rBV3	316	352	0.03%	0.004%
47	8.529	2326	2329	2333	rBV3	316	252	0.02%	0.003%
48	8.580	2342	2345	2348	rBV2	488	345	0.03%	0.004%
49	8.596	2348	2350	2357	rVB3	382	344	0.03%	0.004%
50	8.628	2357	2360	2366	rBV2	325	312	0.03%	0.003%
51	8.783	2396	2408	2431	rBV	573840	963203	82.76%	10.533%
52	9.156	2521	2524	2528	rVB3	273	222	0.02%	0.002%
53	9.181	2528	2532	2535	rBV3	363	292	0.03%	0.003%
54	9.333	2576	2579	2583	rVB2	301	220	0.02%	0.002%
55	9.378	2589	2593	2598	rVB2	252	228	0.02%	0.002%
56	9.516	2631	2636	2640	rVB2	279	317	0.03%	0.003%
57	9.551	2640	2647	2649	rBV2	216	287	0.02%	0.003%
58	9.638	2671	2674	2679	rVV2	237	234	0.02%	0.003%
59	9.870	2743	2746	2748	rBV	463	334	0.03%	0.004%
60	10.098	2814	2817	2822	rBV	339	361	0.03%	0.004%
61	10.149	2822	2833	2857	rBV	364905	584843	50.25%	6.396%
62	10.336	2887	2891	2896	rBV3	305	288	0.02%	0.003%
63	10.361	2896	2899	2903	rVB2	403	337	0.03%	0.004%
64	10.493	2936	2940	2946	rBV2	195	223	0.02%	0.002%
65	10.616	2973	2978	2981	rBV2	289	365	0.03%	0.004%
66	10.918	3067	3072	3075	rBV	223	224	0.02%	0.002%
67	11.133	3135	3139	3144	rBV2	687	663	0.06%	0.007%
68	11.181	3144	3154	3183	rBV	533241	847281	72.80%	9.266%
69	11.426	3227	3230	3233	rBV	391	274	0.02%	0.003%
70	11.493	3247	3251	3256	rVB5	339	378	0.03%	0.004%
71	11.558	3258	3271	3298	rBV	566178	909874	78.18%	9.950%
72	11.979	3398	3402	3406	rBV3	394	390	0.03%	0.004%
73	12.078	3430	3433	3438	rVB2	249	263	0.02%	0.003%
74	12.104	3438	3441	3444	rBV	328	257	0.02%	0.003%
75	12.419	3536	3539	3541	rBV	306	232	0.02%	0.003%
76	12.538	3571	3576	3579	rBV2	225	234	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
 Data File : VV036690.D
 Acq On : 25 Jul 2024 02:58
 Operator : SY/MD
 Sample : P3335-17 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E20N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
 Title : VOC Analysis

77	12.606	3594	3597	3599	rVB3	556	371	0.03%	0.004%
78	12.873	3676	3680	3683	rVB3	271	228	0.02%	0.002%
79	12.898	3683	3688	3690	rBV2	277	224	0.02%	0.002%
80	13.049	3731	3735	3739	rBV3	261	258	0.02%	0.003%
81	13.098	3745	3750	3752	rBV2	252	210	0.02%	0.002%
82	13.168	3769	3772	3776	rVB2	314	244	0.02%	0.003%
83	13.406	3841	3846	3853	rVB2	295	296	0.03%	0.003%
84	13.464	3860	3864	3867	rBV2	416	381	0.03%	0.004%
85	13.529	3881	3884	3888	rBV2	390	234	0.02%	0.003%
86	13.609	3905	3909	3915	rVB2	321	327	0.03%	0.004%
87	13.686	3928	3933	3940	rVB3	540	607	0.05%	0.007%
88	13.789	3962	3965	3970	rVB2	312	278	0.02%	0.003%
89	13.869	3987	3990	3994	rBV2	227	208	0.02%	0.002%
90	13.898	3994	3999	4003	rBV2	308	340	0.03%	0.004%
91	14.426	4159	4163	4165	rBV2	372	282	0.02%	0.003%
92	14.548	4198	4201	4204	rBV2	313	216	0.02%	0.002%
93	14.712	4248	4252	4254	rBV2	543	505	0.04%	0.006%
94	14.828	4285	4288	4290	rBV	342	235	0.02%	0.003%
95	14.882	4303	4305	4311	rVB2	398	364	0.03%	0.004%
96	15.291	4428	4432	4435	rBV4	577	437	0.04%	0.005%
97	15.326	4441	4443	4447	rVB3	551	295	0.03%	0.003%
98	15.355	4447	4452	4453	rBV3	556	439	0.04%	0.005%
99	15.667	4547	4549	4550	rBV	528	266	0.02%	0.003%
100	15.943	4632	4635	4636	rBV2	744	385	0.03%	0.004%




Sum of corrected areas: 9144390

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036690.D
Acq On : 25 Jul 2024 02:58
Operator : SY/MD
Sample : P3335-17 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

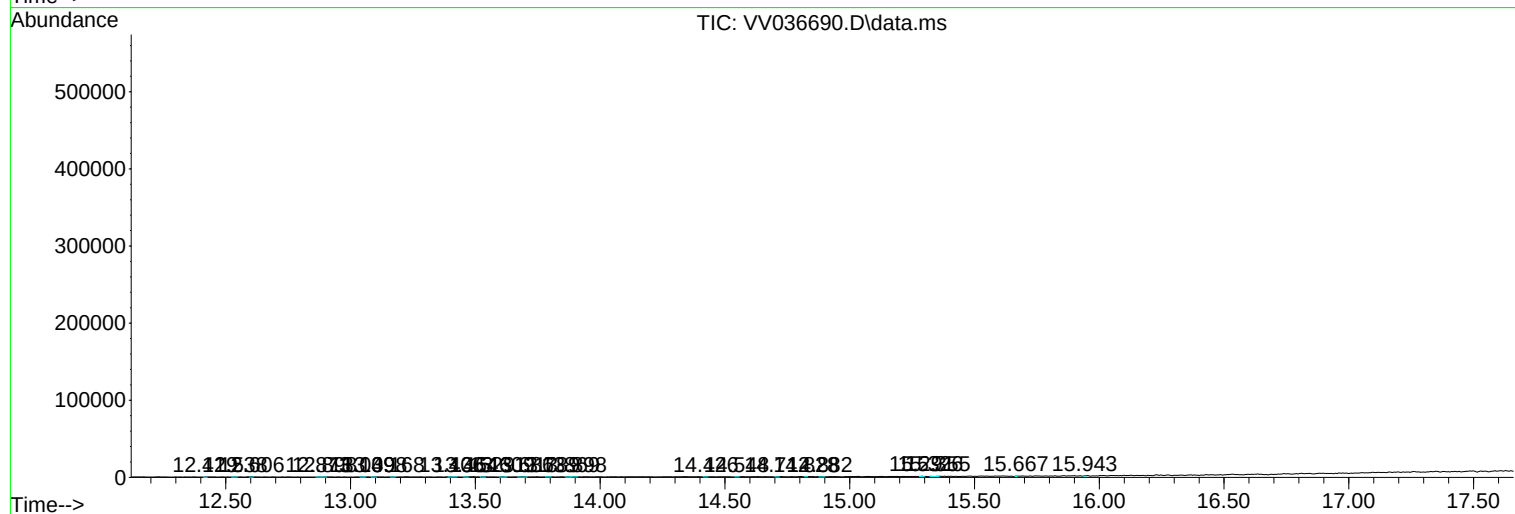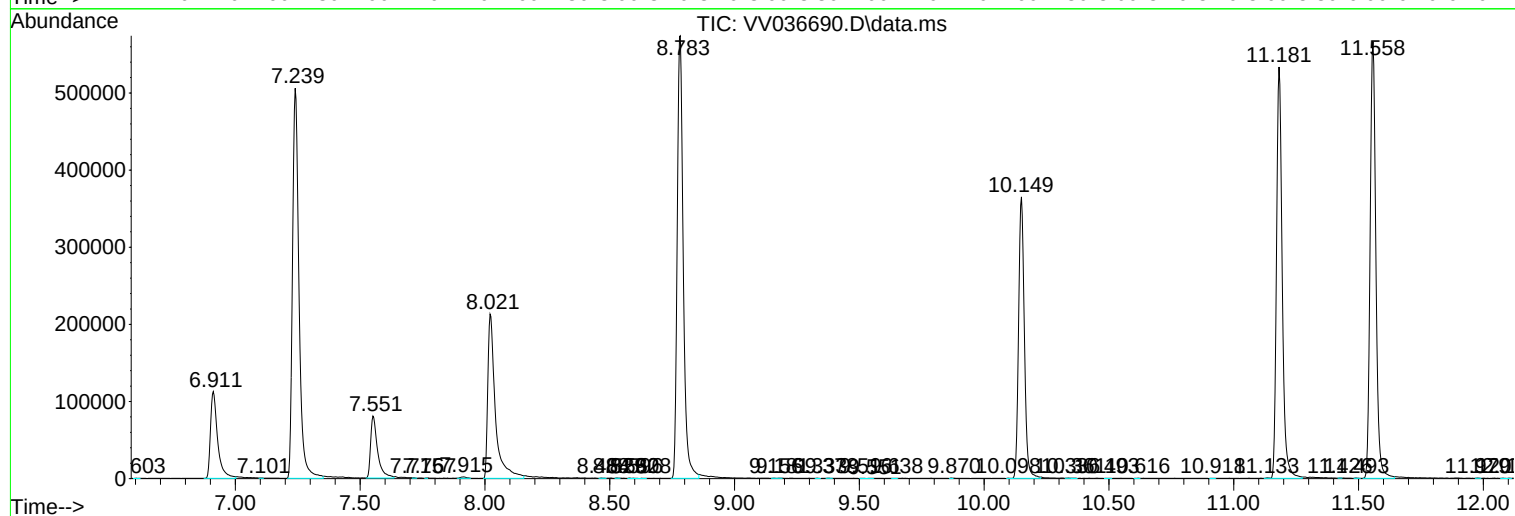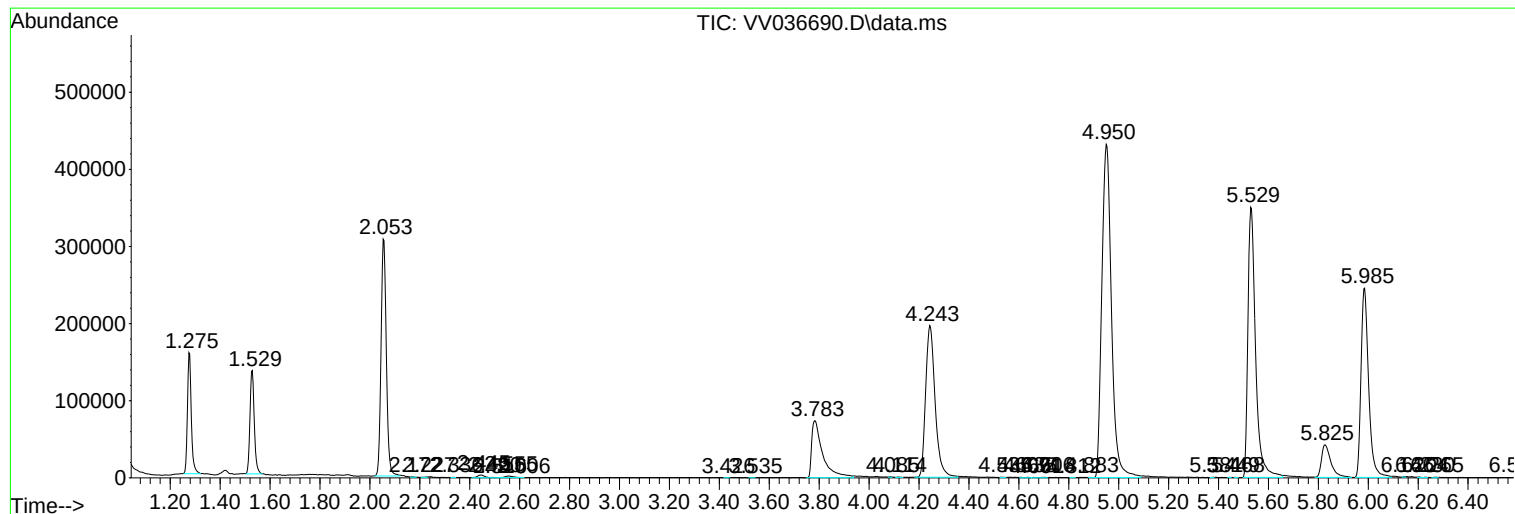

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036690.D
Acq On : 25 Jul 2024 02:58
Operator : SY/MD
Sample : P3335-17 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036690.D
Acq On : 25 Jul 2024 02:58
Operator : SY/MD
Sample : P3335-17 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E20N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc