
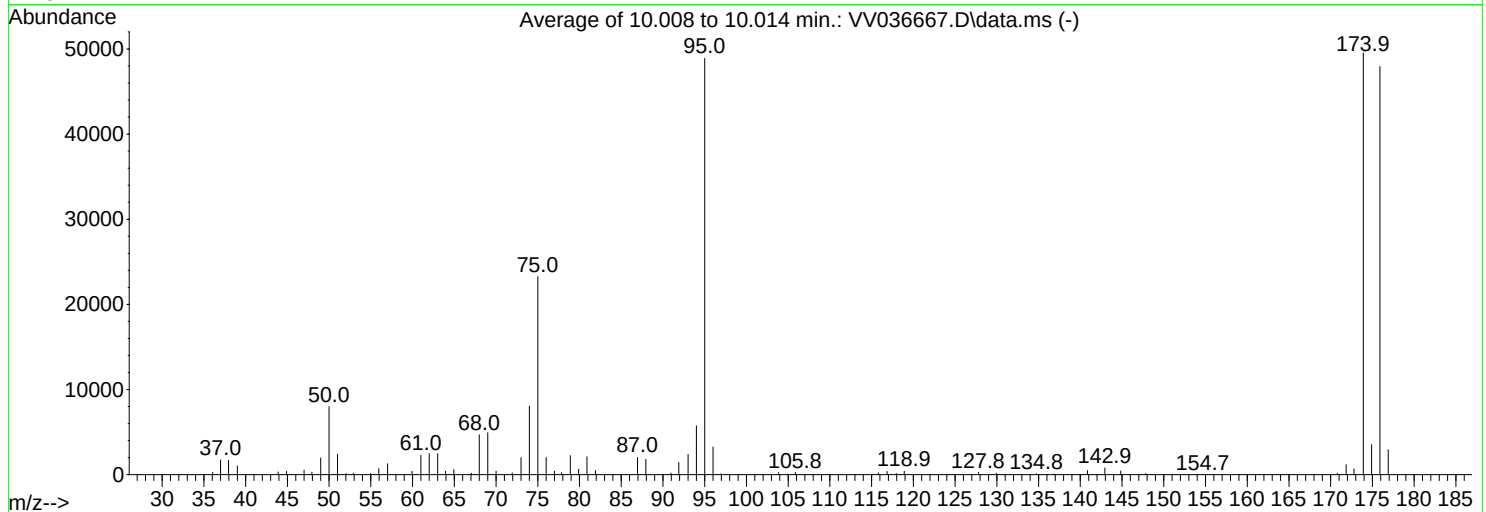


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072524\
Data File : VV036667.D
Acq On : 24 Jul 2024 13:01
Operator : SY/MD
Sample : BFB349
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB349

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072424WMA.M
Title : VOC Analysis
Last Update : Thu Jul 25 03:06:08 2024

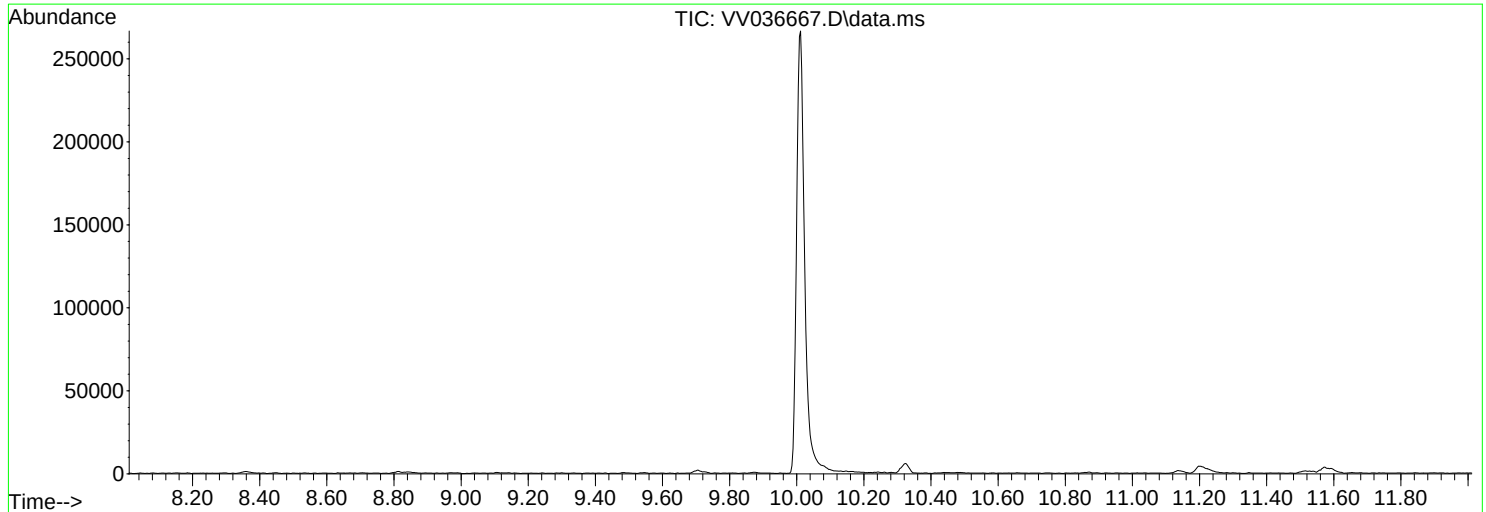

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	7996	PASS
75	95	30	80	47.5	23243	PASS
95	95	100	100	100.0	48915	PASS
96	95	5	9	6.6	3244	PASS
173	174	0.00	2	1.4	676	PASS
174	95	50	120	101.3	49549	PASS
175	174	5	9	7.1	3526	PASS
176	174	95	105	96.8	47957	PASS
177	176	5	10	6.1	2924	PASS

m/z	Abundance
40.00	134.0
43.90	281.0

Instrument :
MSVOA_V
ClientSampleId :
BFB349

m/z	Abundance
36.00	322.0
37.00	1857.0
37.90	1819.0
39.00	973.0
39.90	184.0
44.00	607.0
44.90	404.0
47.00	618.0
47.90	352.0
49.00	2012.0
50.00	8487.0
51.00	2470.0
52.10	108.0
52.90	147.0
55.00	169.0
55.90	736.0
57.00	1356.0
59.90	407.0
61.00	2556.0
62.00	2667.0
63.00	2496.0
63.90	426.0
65.00	623.0
67.10	154.0
68.00	4831.0
69.00	5232.0
70.00	415.0
71.90	244.0
73.00	1970.0
74.00	8207.0
75.00	23984.0
76.00	2168.0
77.00	386.0
77.90	244.0
78.90	2235.0
79.90	613.0
80.90	2293.0
81.90	488.0
87.00	2074.0
88.00	1816.0
90.90	194.0
91.90	1584.0
93.00	2448.0
94.00	5823.0
95.00	50368.0
96.00	3390.0
97.00	112.0
103.80	236.0
104.90	105.0
105.90	276.0
115.80	219.0
116.90	388.0
118.00	169.0
118.90	414.0
127.80	266.0
130.00	161.0
134.70	105.0
136.80	118.0
140.90	476.0
142.90	740.0
144.80	433.0
145.80	109.0
147.90	154.0
154.70	111.0
170.80	194.0
171.90	1133.0
172.80	672.0
173.90	49296.0
174.90	3487.0
175.90	48048.0
176.90	3023.0

Instrument :
MSVOA_V
ClientSampleId :
BFB349

m/z	Abundance
36.10	275.0
37.00	1770.0
38.00	1747.0
39.00	1071.0
39.90	172.0
43.90	634.0
44.90	392.0
47.00	553.0
48.00	316.0
49.00	2061.0
50.00	8186.0
51.00	2461.0
52.10	145.0
52.90	172.0
55.00	149.0
56.00	732.0
57.00	1322.0
59.90	403.0
61.00	2354.0
62.00	2515.0
63.00	2607.0
63.90	418.0
65.00	619.0
66.10	109.0
67.10	154.0
68.00	4825.0
69.00	5037.0
70.00	395.0
72.00	219.0
73.00	2031.0
74.00	8320.0
75.00	23832.0
76.00	2075.0
77.00	419.0
77.90	234.0
78.90	2315.0
79.90	663.0
80.90	2161.0
81.90	488.0
86.90	2116.0
87.90	1850.0
91.00	191.0
91.90	1456.0
93.00	2419.0
94.00	5877.0
95.00	50640.0
96.00	3310.0
97.00	122.0
103.80	255.0
104.90	109.0
105.90	263.0
114.90	109.0
115.80	229.0
116.80	359.0
118.00	159.0
118.90	432.0
127.80	274.0
130.00	182.0
134.80	109.0
136.90	109.0
140.80	486.0
143.00	822.0
144.80	449.0
147.80	144.0
159.00	105.0
170.80	191.0
171.90	1206.0
172.80	693.0
173.90	51376.0
174.90	3635.0
175.90	49720.0
176.90	3008.0

Instrument :
MSVOA_V
ClientSampleId :
BFB349

m/z	Abundance
36.10	199.0
37.00	1555.0
38.00	1460.0
39.00	994.0
40.00	135.0
43.90	569.0
44.90	345.0
47.00	424.0
48.00	252.0
49.00	1801.0
50.00	7314.0
51.00	2228.0
52.00	152.0
52.90	173.0
54.90	119.0
56.00	649.0
57.00	1186.0
60.00	384.0
61.00	1935.0
62.00	2212.0
63.00	2314.0
64.00	369.0
64.90	581.0
67.00	145.0
68.00	4391.0
69.00	4507.0
70.00	417.0
72.00	181.0
73.00	1988.0
74.00	7609.0
75.00	21912.0
76.00	1818.0
77.00	437.0
77.80	198.0
78.90	2147.0
79.90	638.0
80.90	1882.0
81.90	470.0
87.00	1917.0
87.90	1696.0
90.90	195.0
91.90	1275.0
93.00	2221.0
94.00	5501.0
95.00	45736.0
96.00	3033.0
96.90	106.0
103.90	235.0
105.80	232.0
115.00	119.0
115.80	169.0
116.80	357.0
117.90	134.0
118.90	416.0
127.80	231.0
129.90	160.0
134.80	107.0
140.80	496.0
142.90	786.0
144.90	407.0
147.80	120.0
170.80	148.0
171.80	1141.0
172.80	662.0
173.90	47976.0
174.90	3455.0
175.90	46104.0
176.90	2740.0

Instrument :
MSVOA_V
ClientSampleId :
BFB349