

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072618\
 Data File : VV006708.D
 Acq On : 26 Jul 2018 17:02
 Operator : SY/MD
 Sample : J4148-02
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SW7

Quant Time: Jul 27 00:58:54 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 27 00:52:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	248815	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	228491	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	95130	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	94933	7.33	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	146.60%#
7) Chloroethane-d5	1.58	69	67545	6.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	132.80%#
11) 1,1-Dichloroethene-d2	2.13	63	124825	4.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.20%
20) 2-Butanone-d5	3.97	46	209443	51.76	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.52%
24) Chloroform-d	4.40	84	147604	6.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	121.40%
26) 1,2-Dichloroethane-d4	5.09	65	74003	6.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	125.00%
32) Benzene-d6	5.10	84	319134	6.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	136.00%#
36) 1,2-Dichloropropane-d6	6.12	67	99455	6.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	125.40%
41) Toluene-d8	7.36	98	276332	6.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	134.60%#
43) trans-1,3-Dichloropropene-	7.67	79	31927	6.17	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	123.40%
46) 2-Hexanone-d5	8.14	63	166148	50.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.36%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	69317	5.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	96219	6.79	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	135.80%#


Target Compounds					Ovalue
13) Acetone	2.22	43	8792	3.42 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072618\
Data File : VV006708.D
Acq On : 26 Jul 2018 17:02
Operator : SY/MD
Sample : J4148-02
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SW7

Quant Time: Jul 27 00:58:54 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 27 00:52:23 2018
Response via : Initial Calibration

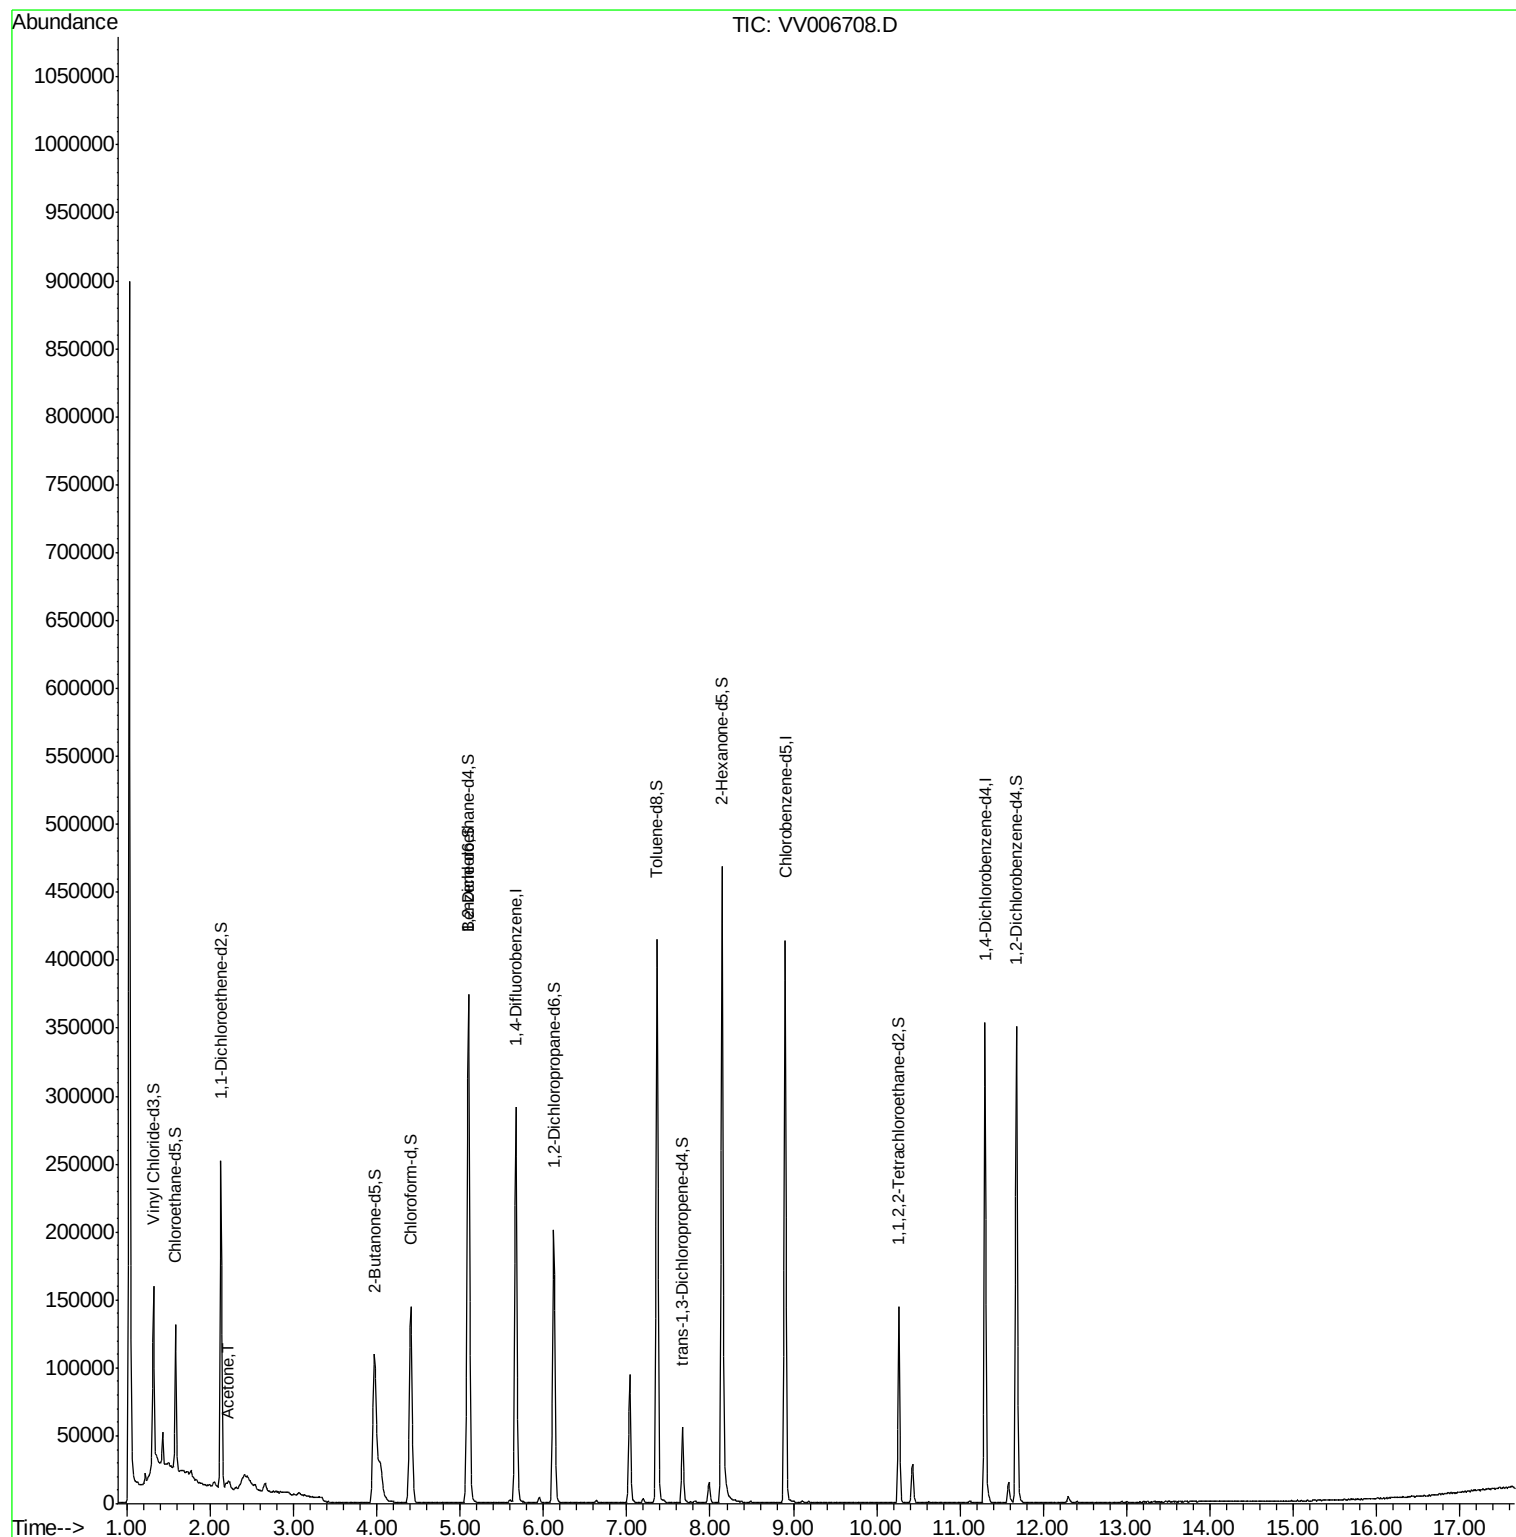

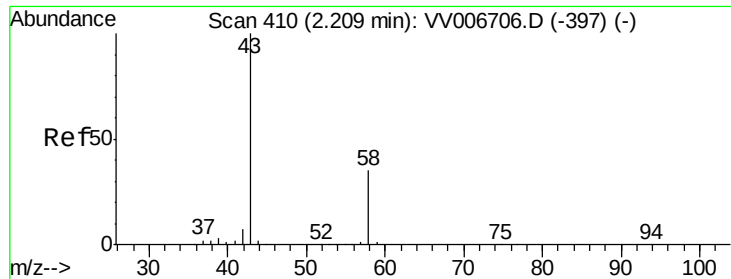

#13

Acetone

Concen: 3.42 ug/L

RT: 2.22 min Scan# 412

Delta R.T. 0.01 min

Lab File: VV006708.D

Acq: 26 Jul 2018 17:02

Instrument :
MSVOA_V
ClientSampleId :
C0SW7

Tot Ion: 43 Resp: 8792

Ion Ratio Lower Upper

43 100

58 38.5 0.0 71.4

